
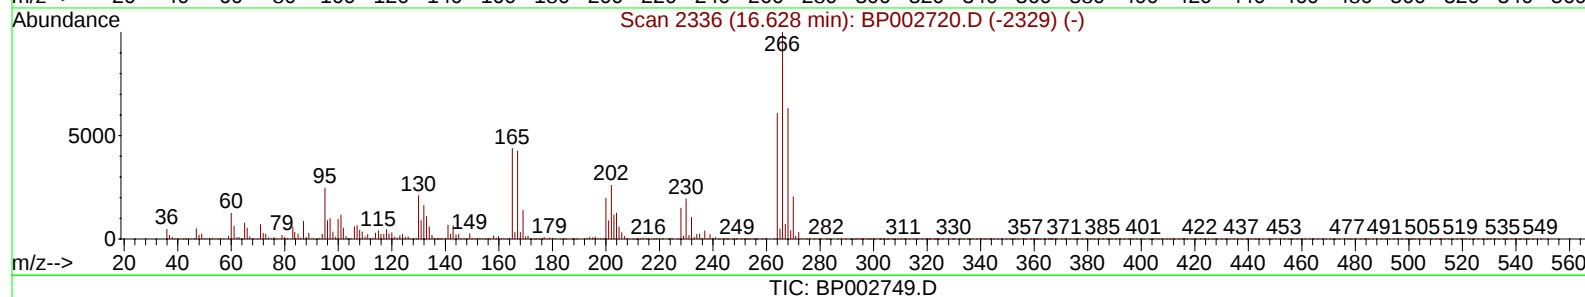
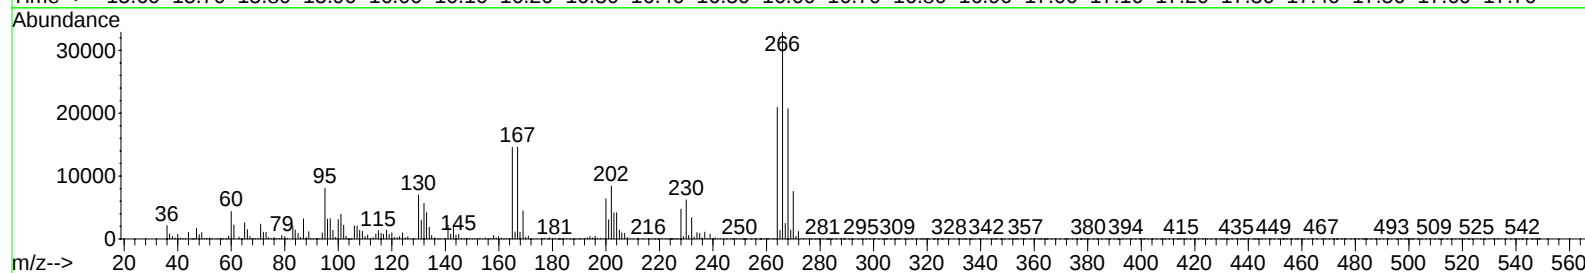


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071520\
 Data File : BP002749.D
 Acq On : 15 Jul 2020 11:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 16:44:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

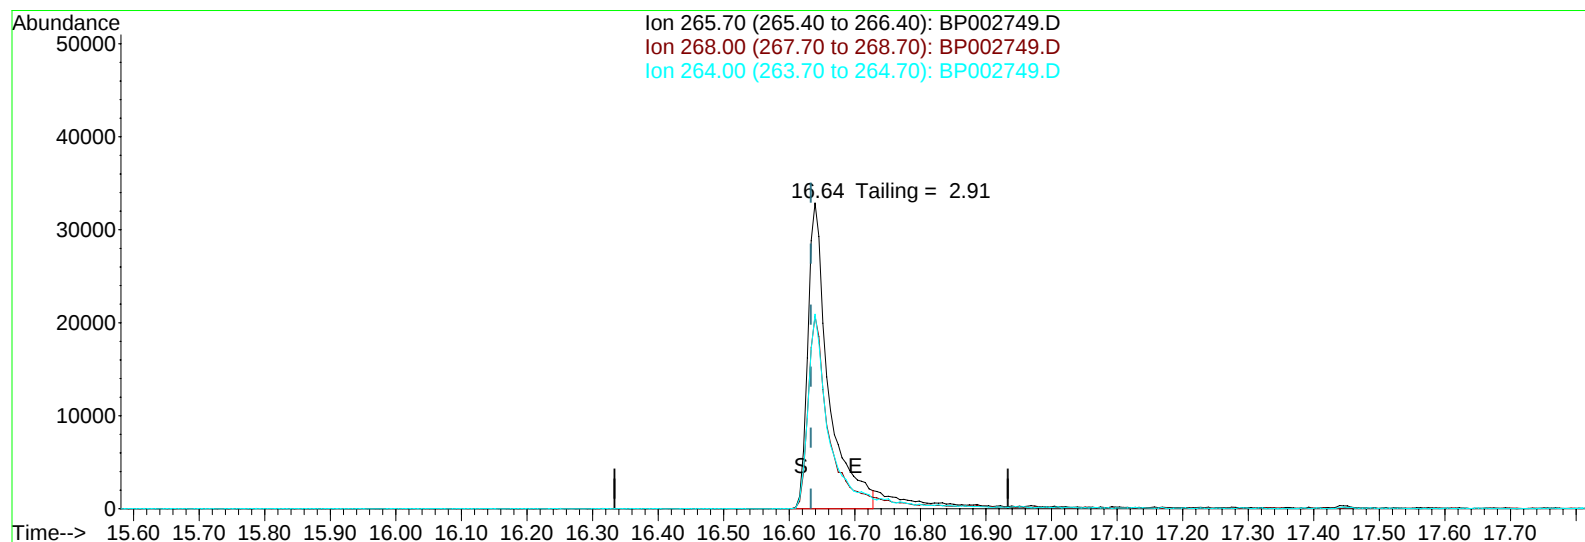

(70) Pentachlorophenol (C)




16.639min (+0.006) 59406.94ng

response 78160

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.97
264.00	60.70	63.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071520\
 Data File : BP002749.D
 Acq On : 15 Jul 2020 11:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 16:44:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

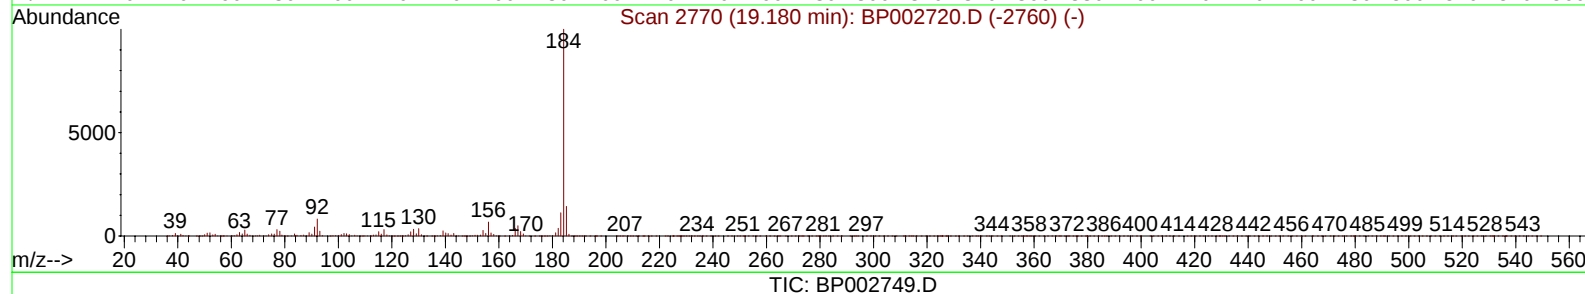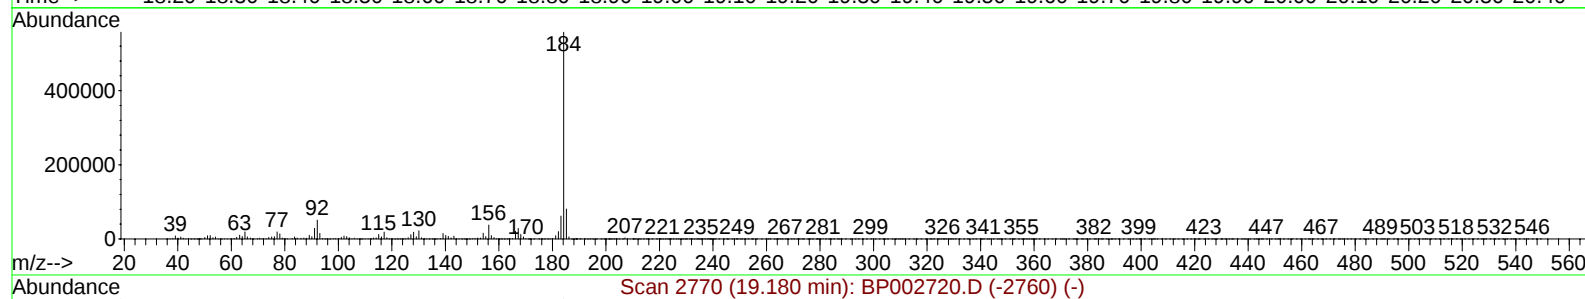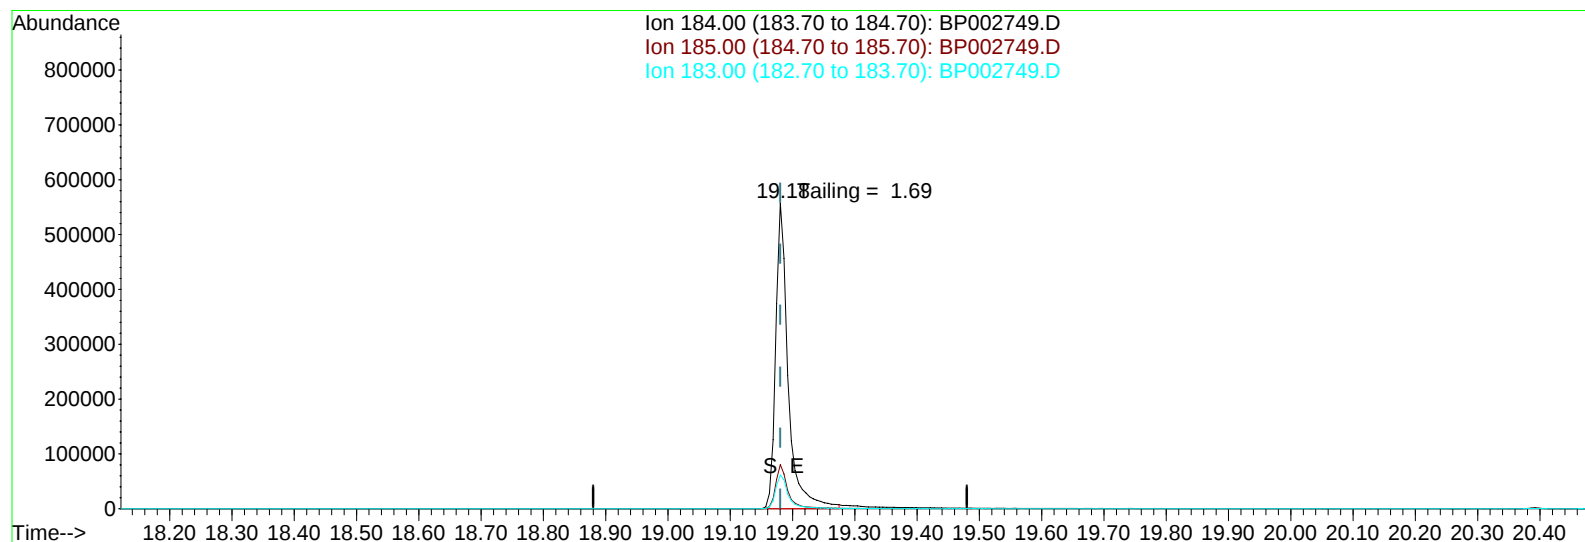

(77) Benzidine

19.180min (+0.000) 123798.65ng

response 810107

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.47
183.00	11.20	11.05
0.00	0.00	0.00