

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071520\
 Data File : BP002757.D
 Acq On : 15 Jul 2020 16:47
 Operator : CG/JU
 Sample : L3300-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-8A-D


Quant Time: Jul 16 01:54:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	148114	20.00	ng	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071520\
Data File : BP002757.D
Acq On : 15 Jul 2020 16:47
Operator : CG/JU
Sample : L3300-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-8A-D

Quant Time: Jul 16 01:54:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

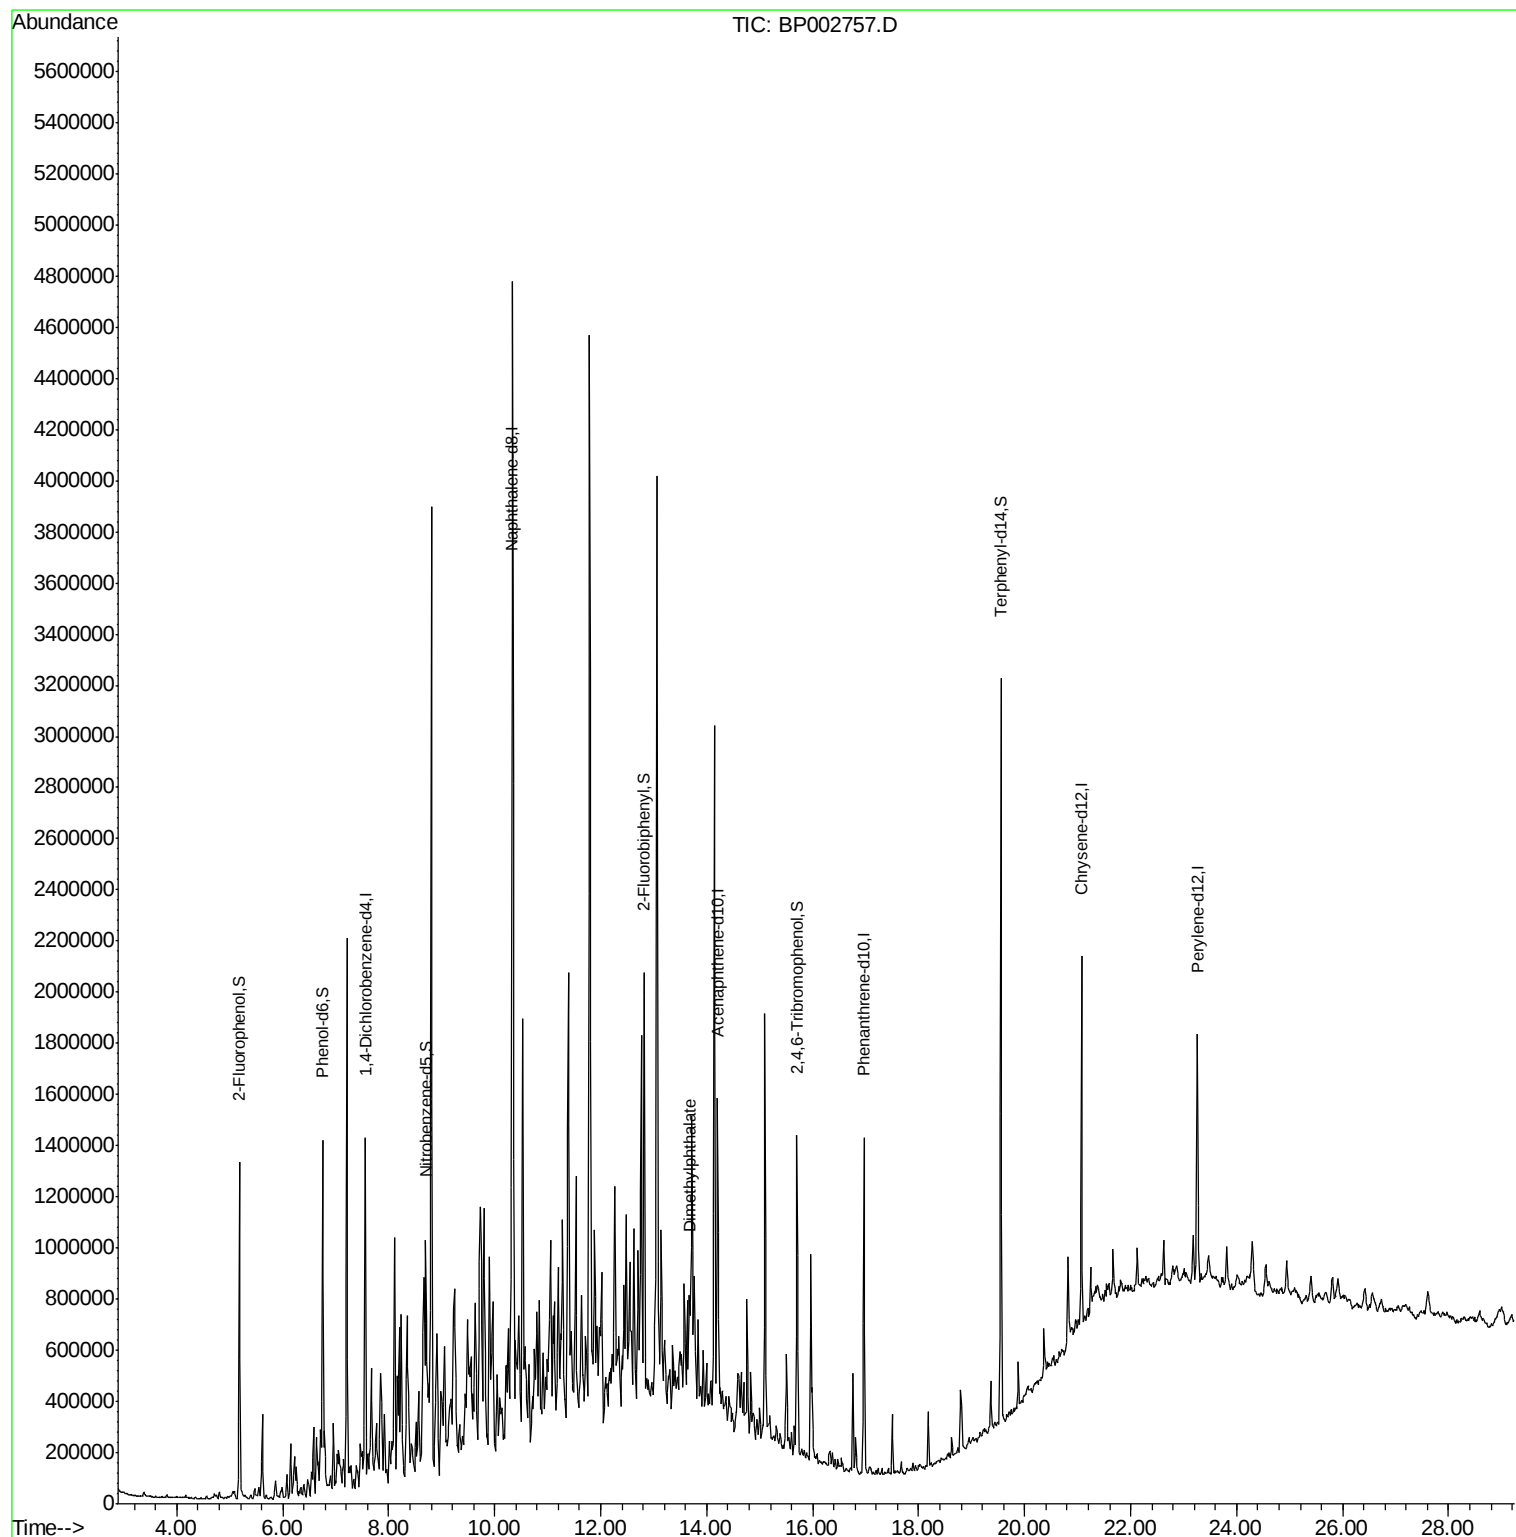

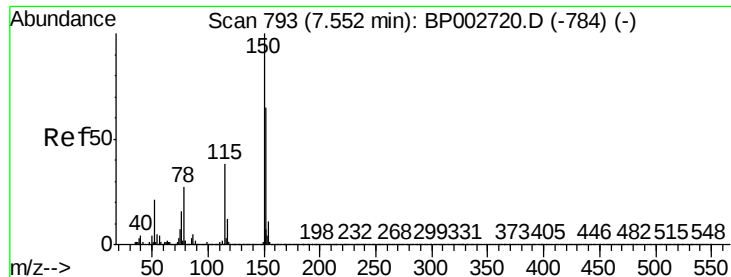


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.55 min Scan# 793
Delta R.T. 0.00 min
Lab File: BP002757.D
Acq: 15 Jul 2020 16:47

Instrument :
BNA_P
ClientSampleId :
TP-8A-D

Tot Ion	Ratio	Lower	Upper
152	100		
150	159.2	123.7</	

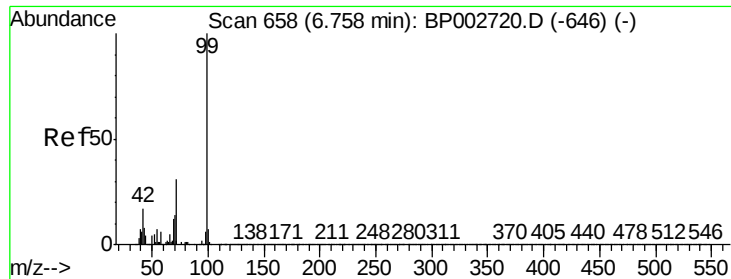

#7

Phenol-d6


Concen: 60.325 ng

RT: 6.75 min Scan# 657

Delta R.T. -0.01 min

Lab File: BP002757.D


Acq: 1

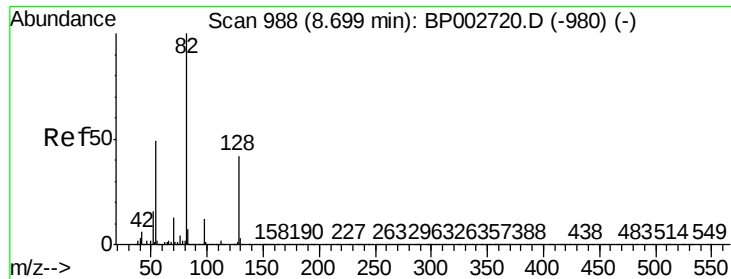

#23
Nitrobenzene-d5
Concen: 48.588 ng
RT: 8.70 min Scan# 988
Delta R.T. -0.01 min
Lab File: BP002757.D
Acq: 15 Jul 2020 16:47

Instrument :
BNA_P
ClientSampleId :
TP-8A-D


Tot Ion	82	Resp	468164
Ion Ratio	Lower	Upper	
82	100		

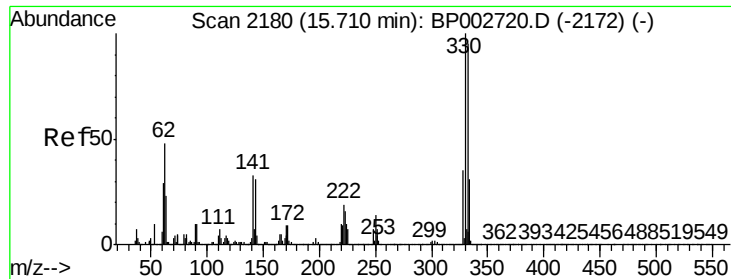

#42
 2,4,6-Tribromophenol
 Concen: 60.731 ng
 RT: 15.71 min Scan# 2180
 Delta R.T. 0.00 min
 Lab File: BP002757.D
 Acq: 15 Jul 2020 16:47

Instrument :
 BNA_P
 ClientSampleId :
 TP-8A-D


Tot Ion	Ratio	Lower	Upper
330	100		
332	94.9		

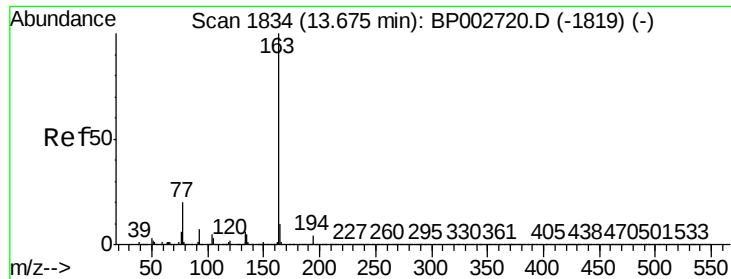

#50
Dimethylphthalate
Concen: 6.391 ng
RT: 13.67 min Scan# 1833
Delta R.T. -0.01 min
Lab File: BP002757.D
Acq: 15 Jul 2020 16:47

Instrument :
BNA_P
ClientSampleId :
TP-8A-D


Tot Ion:163 Resp: 170941
Ion Ratio Lower Upper
163 100
194 4.7 3.4 5.2
164 9.7 7.8 11.8

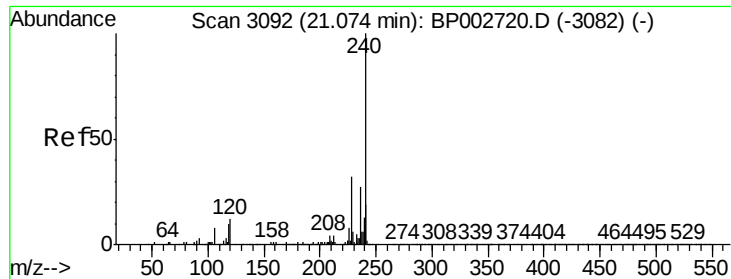


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.07 min Scan# 3091
Delta R.T. -0.01 min
Lab File: BP002757.D
Acq: 15 Jul 2020 16:47

Instrument :
BNA_P
ClientSampleId :
TP-8A-D

Tot Ion:240 Resp: 670009
Ion Ratio Lower Upper
240 100
120 12.7 9.4 14.2
236 28.8 21.3 31.9

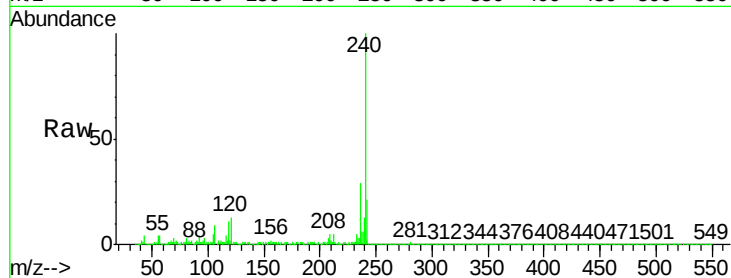

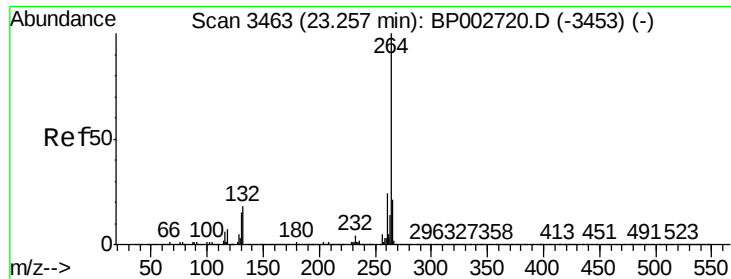

#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.26 min Scan# 3463
Delta R.T. -0.01 min
Lab File: BP002757.D
Acq: 15 Jul 2020 16:47

Instrument :
BNA_P
ClientSampleId :
TP-8A-D

Tot Ion	Ratio	Lower	Upper
264	100		