

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP071520\
 Data File : BP002751.D
 Acq On : 15 Jul 2020 13:13
 Operator : CG/JU
 Sample : PB130217BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB130217BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.181	384	390	417	rBV	3278177	4939542	70.63%	11.993%
2	6.758	650	658	677	rBV	3007794	4962966	70.97%	12.050%
3	7.558	787	794	808	rBV	741964	1196601	17.11%	2.905%
4	8.705	980	989	1008	rBV	1886885	3247503	46.44%	7.885%
5	10.328	1257	1265	1285	rBV	901583	1636183	23.40%	3.973%
6	12.822	1682	1689	1713	rBV	3875714	6411580	91.68%	15.567%
7	14.210	1918	1925	1939	rBV	1315600	2054241	29.37%	4.988%
8	15.710	2173	2180	2210	rBV	2616038	4095833	58.57%	9.945%
9	16.969	2388	2394	2412	rBV	1448260	2247991	32.14%	5.458%
10	19.557	2829	2834	2849	rBV2	5278789	6993303	100.00%	16.980%
11	21.075	3087	3092	3107	rBV	1439726	1874426	26.80%	4.551%
12	23.263	3458	3464	3482	rVB2	767842	1525554	21.81%	3.704%


Sum of corrected areas: 41185723

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071520\
Data File : BP002751.D
Acq On : 15 Jul 2020 13:13
Operator : CG/JU
Sample : PB130217BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130217BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

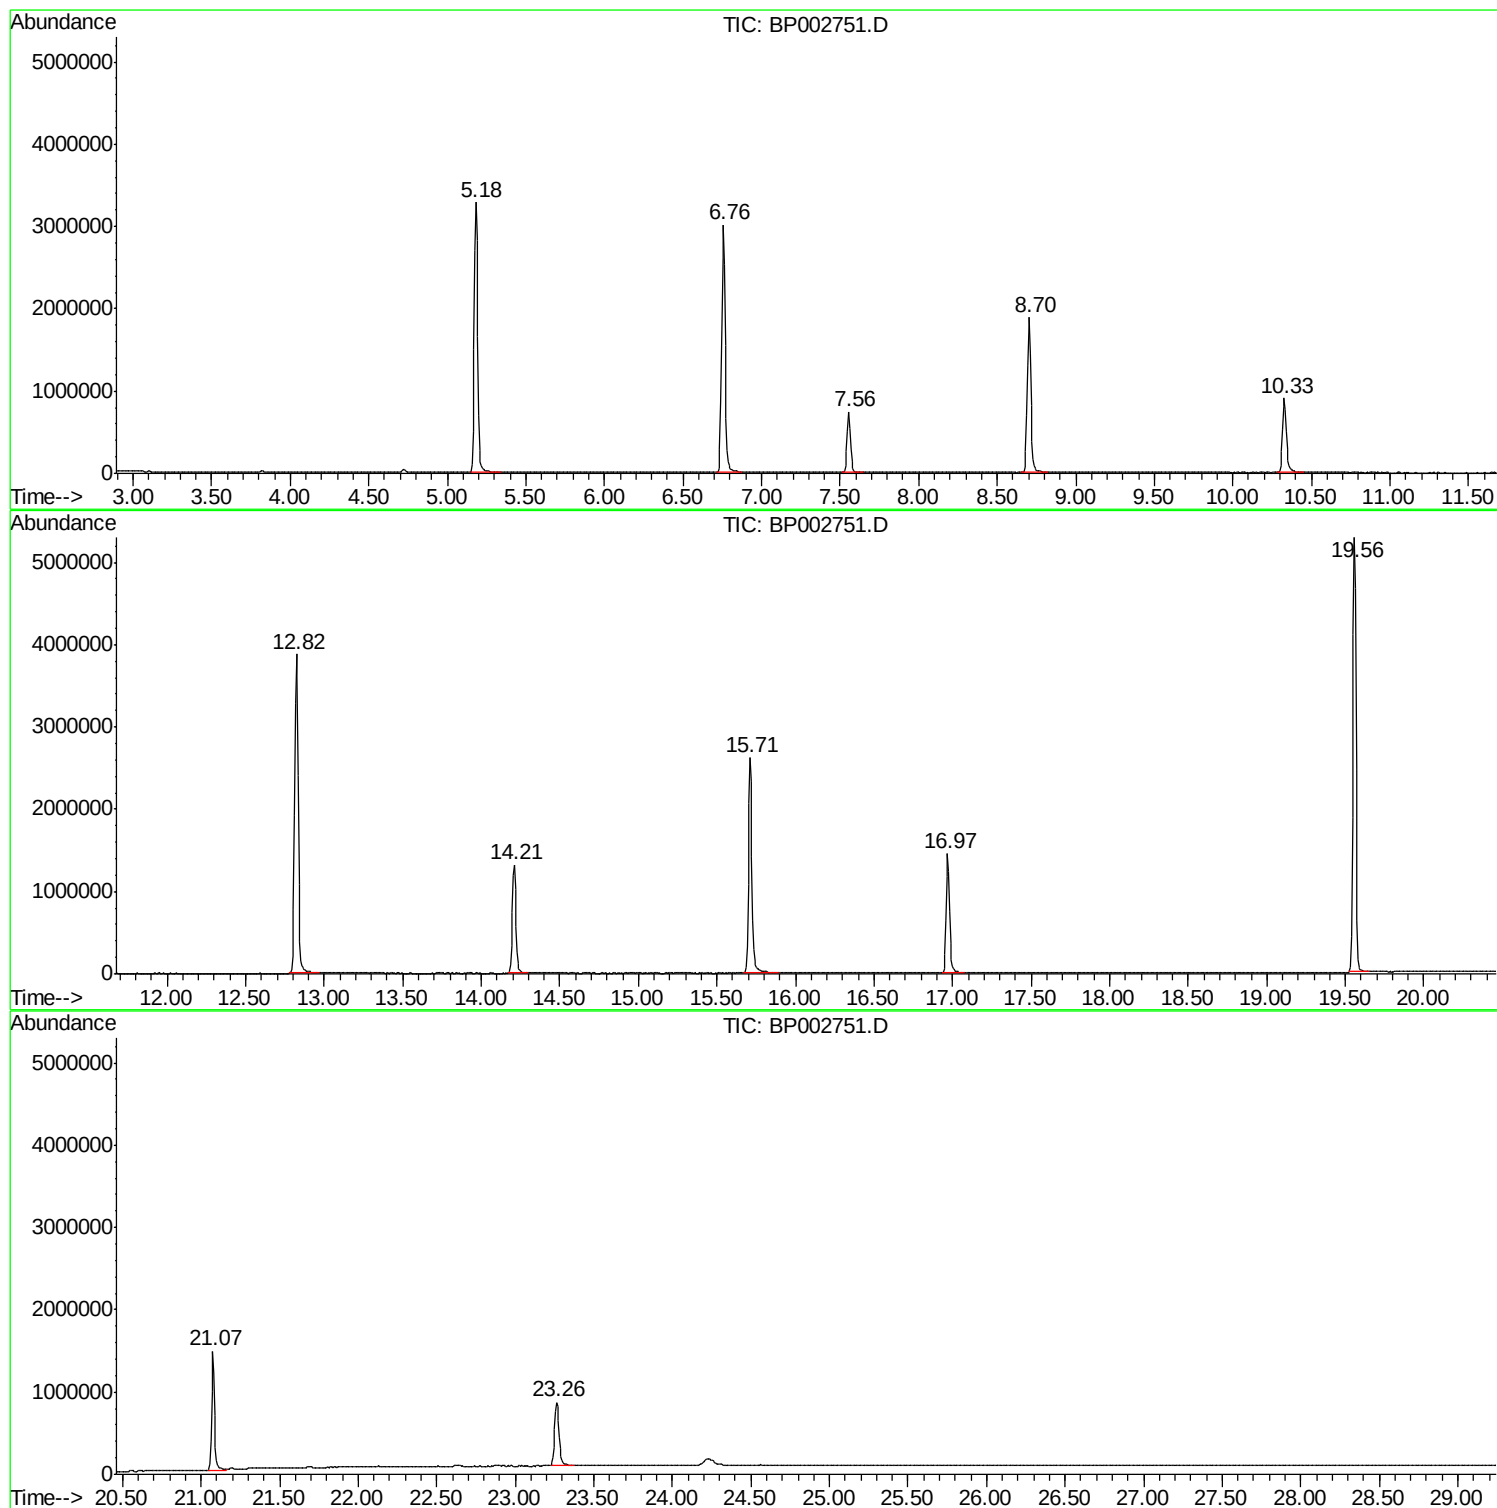

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP071520\
Data File : BP002751.D
Acq On : 15 Jul 2020 13:13
Operator : CG/JU
Sample : PB130217BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130217BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP071520\
Data File : BP002751.D
Acq On : 15 Jul 2020 13:13
Operator : CG/JU
Sample : PB130217BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130217BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc