


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071520\
 Data File : BP002749.D
 Acq On : 15 Jul 2020 11:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:54:03 2020

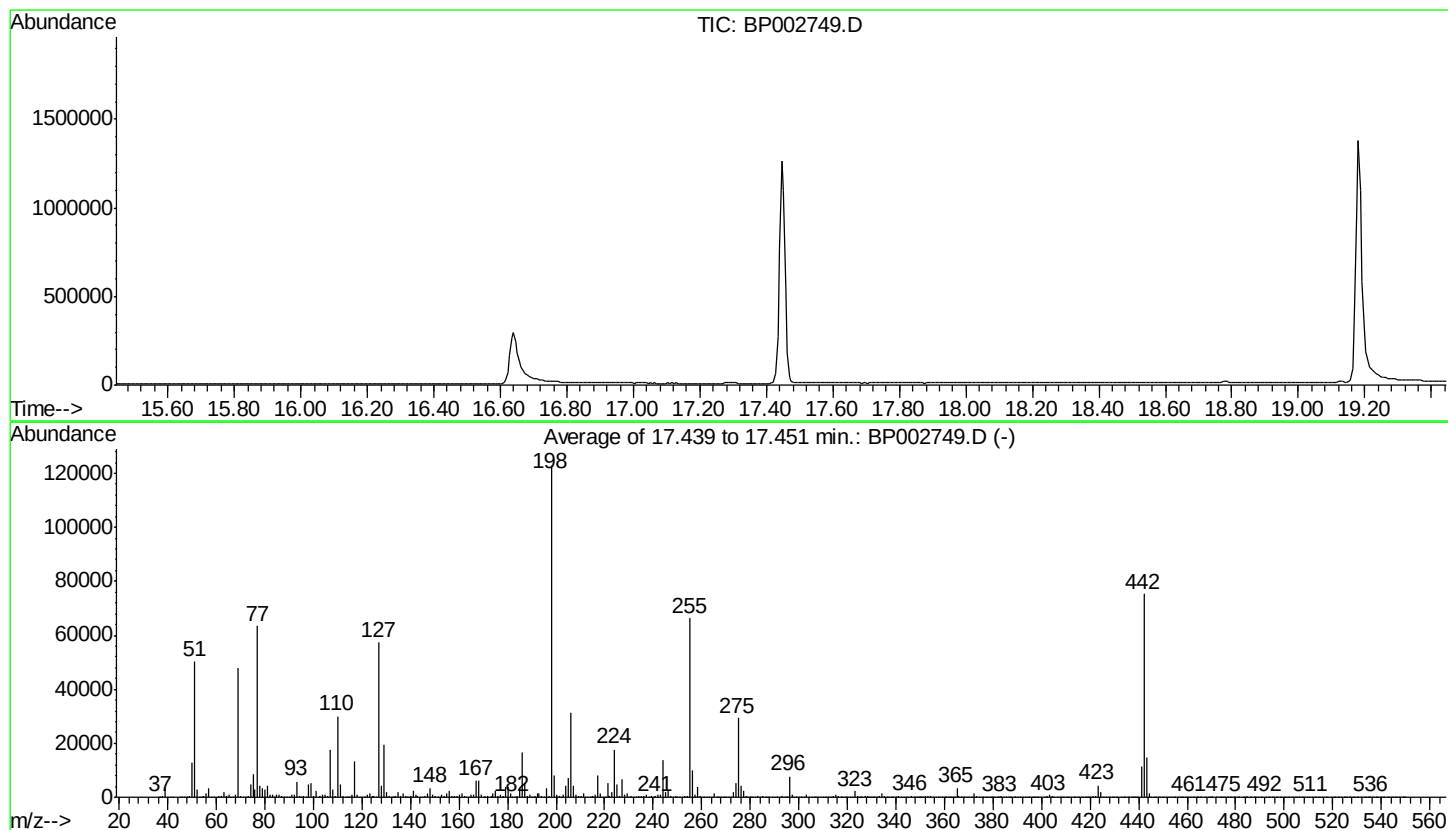

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	50074	PASS
68	69	0.00	2	1.8	878	PASS
69	198	0.00	100	39.0	47910	PASS
70	69	0.00	2	0.6	296	PASS
127	198	10	80	46.6	57269	PASS
197	198	0.00	2	0.5	560	PASS
198	198	100	100	100.0	122856	PASS
199	198	5	9	6.6	8096	PASS
275	198	10	60	23.8	29288	PASS
365	198	1	100	2.8	3498	PASS
441	198	0.01	100	9.4	11582	PASS
442	198	50	100	61.2	75237	PASS
443	442	15	24	19.4	14620	PASS