




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020984.D
Acq On : 16 Jul 2024 10:01
Operator : MA/JU
Sample : P3177-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BS6

Manual IntegrationsAPPROVED

Quant Time: Jul 16 22:54:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024

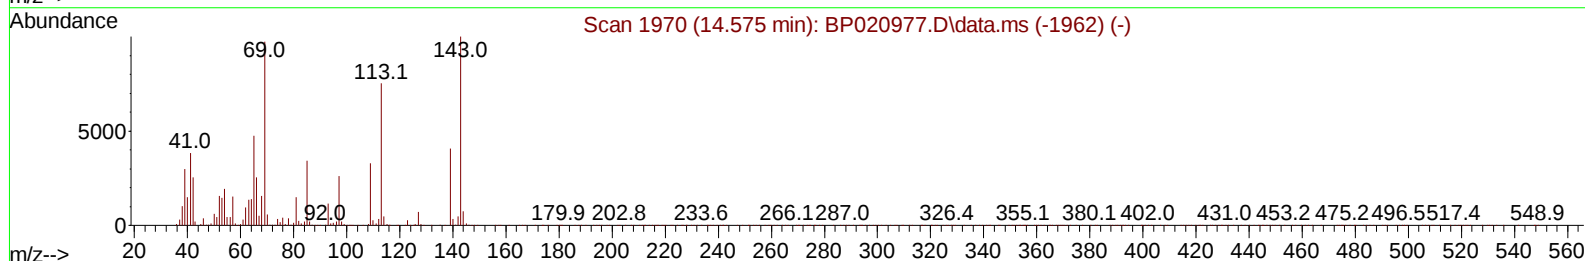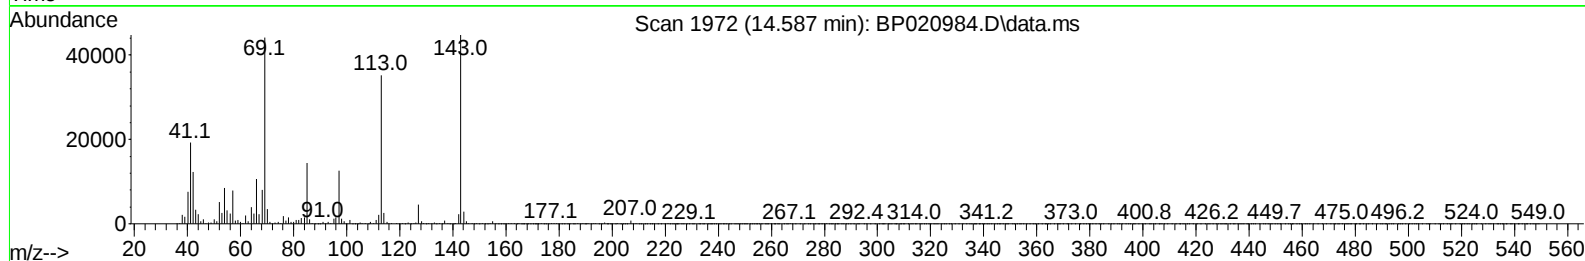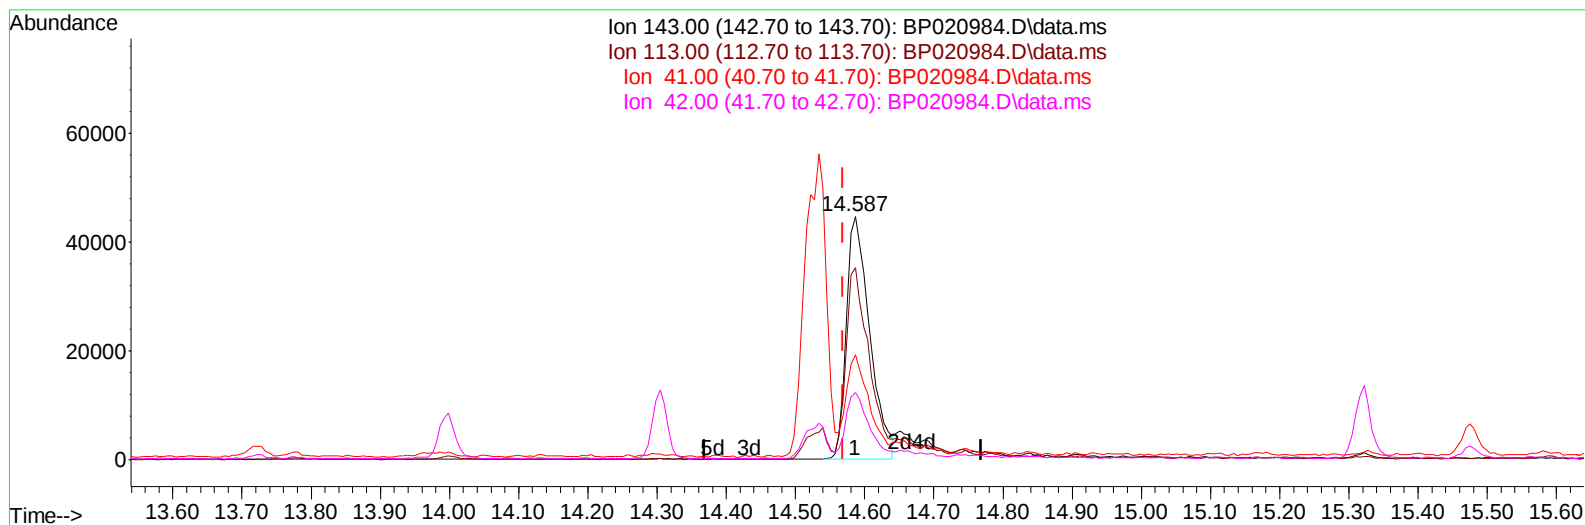

TIC: BP020984.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.018) 15.25 ng/u1

response 104393

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	78.77
41.00	37.90	42.98
42.00	27.10	27.58




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020984.D
Acq On : 16 Jul 2024 10:01
Operator : MA/JU
Sample : P3177-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BS6

Manual IntegrationsAPPROVED

Quant Time: Jul 16 22:54:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024

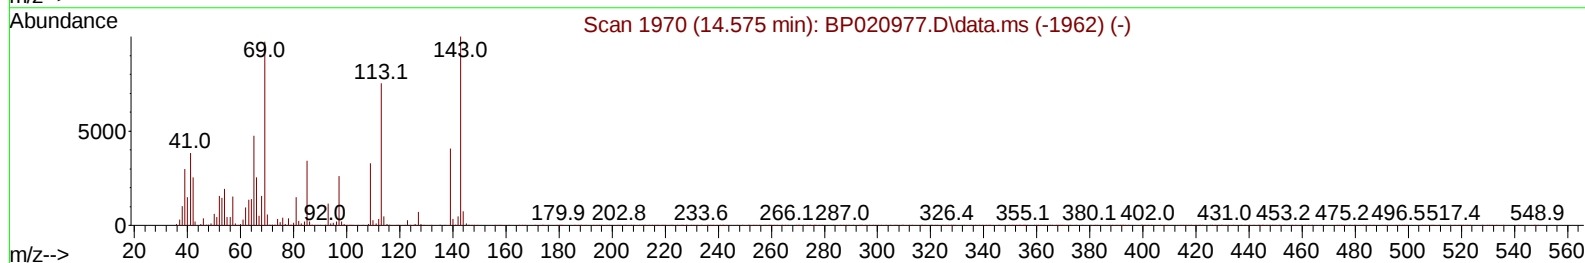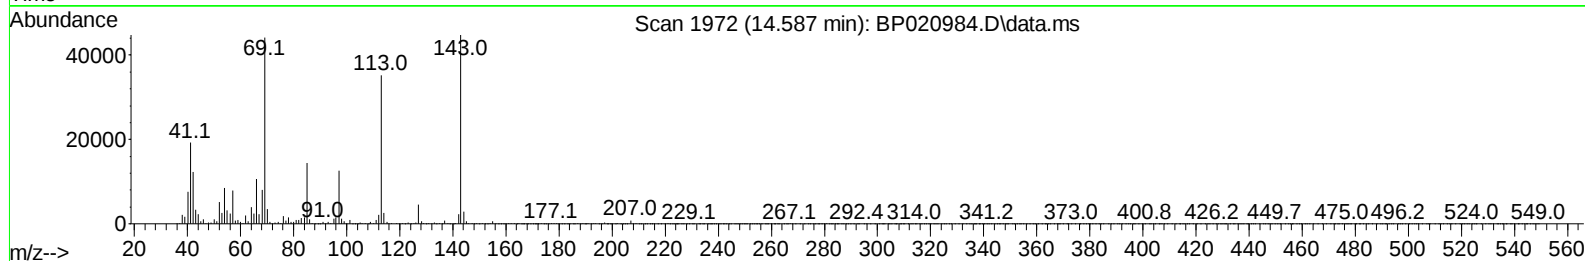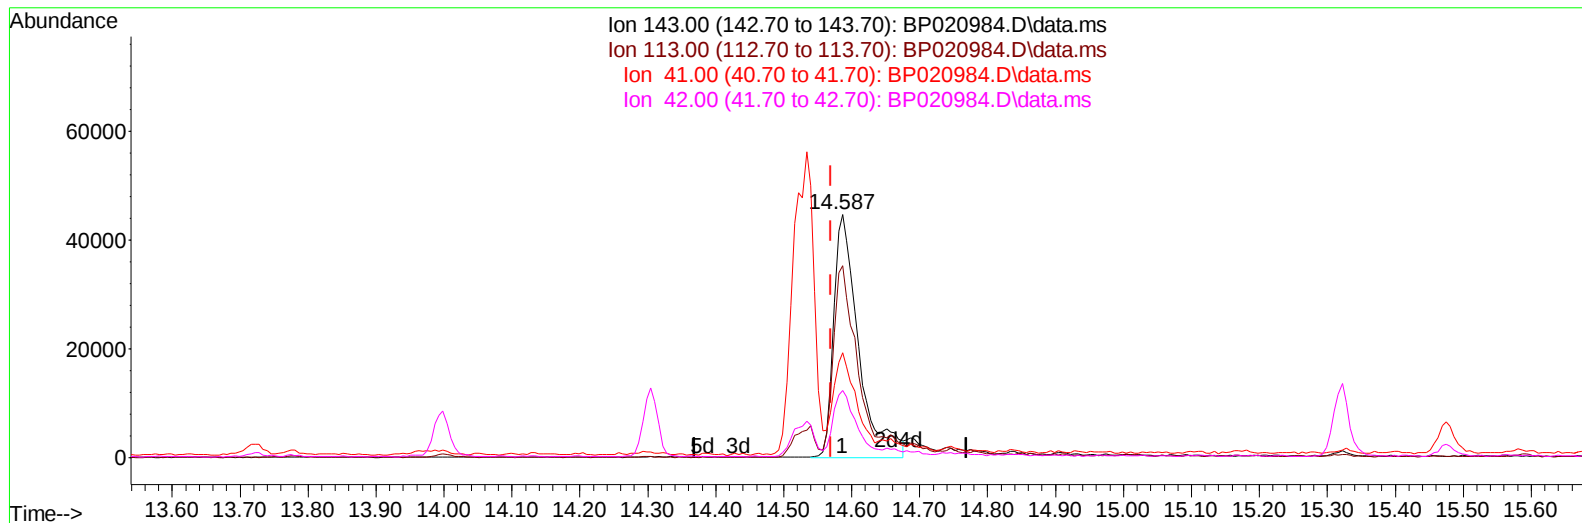

TIC: BP020984.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.018) 16.59 ng/ul m

response 113601

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	78.77
41.00	37.90	42.98
42.00	27.10	27.58

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
 Data File : BP020984.D
 Acq On : 16 Jul 2024 10:01
 Operator : MA/JU
 Sample : P3177-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BS6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/18/2024

Quant Time: Jul 16 23:06:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 15 12:22:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	243188	20.000	ng/ul	0.00
20) Naphthalene-d8	10.452	136	975966	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	662003	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.122	188	1345716	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1373797	20.000	ng/ul	0.00
88) Perylene-d12	24.839	264	1671836	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	17327	3.242	ng/uL	0.01
4) Pyridine-d5	3.670	84	241823	15.630	ng/ul	0.02
7) Phenol-d5	6.899	99	378357	19.083	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	226417	18.844	ng/ul	0.01
11) 2-Chlorophenol-d4	7.246	132	322994	19.773	ng/ul	0.01
15) 4-Methylphenol-d8	8.410	113	326444	19.824	ng/ul	0.02
21) Nitrobenzene-d5	8.852	128	155960	20.574	ng/ul	0.02
24) 2-Nitrophenol-d4	9.557	143	178727	20.600	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.099	165	323174	20.599	ng/ul	0.01
31) 4-Chloroaniline-d4	10.604	131	431616	20.767	ng/ul	0.02
46) Dimethylphthalate-d6	13.728	166	1063122	22.091	ng/ul	0.02
49) Acenaphthylene-d8	13.998	160	1175652	21.757	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	113601m	16.591	ng/ul	0.02
60) Fluorene-d10	15.322	176	900199	22.801	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	117345	14.412	ng/ul	0.01
73) Anthracene-d10	17.216	188	1375949	23.021	ng/ul	0.00
81) Pyrene-d10	19.598	212	1689691	19.894	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.621	264	1849882	22.435	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020984.D
Acq On : 16 Jul 2024 10:01
Operator : MA/JU
Sample : P3177-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BS6

Manual IntegrationsAPPROVED

Quant Time: Jul 16 23:06:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024

