




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020987.D
Acq On : 16 Jul 2024 12:10
Operator : MA/JU
Sample : P3177-18
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BY6

Manual IntegrationsAPPROVED

Quant Time: Jul 16 22:55:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024

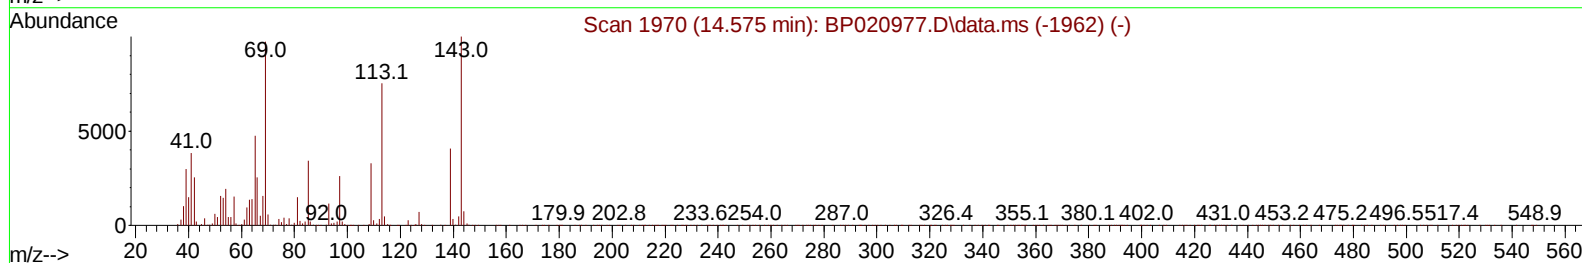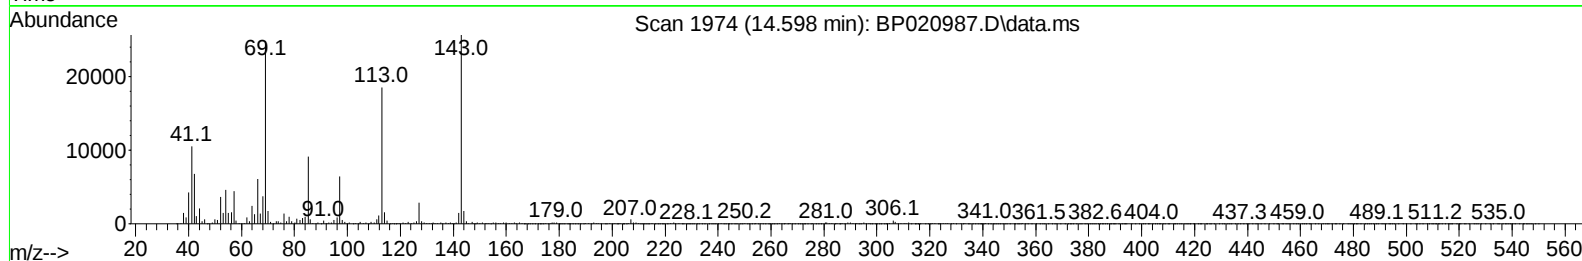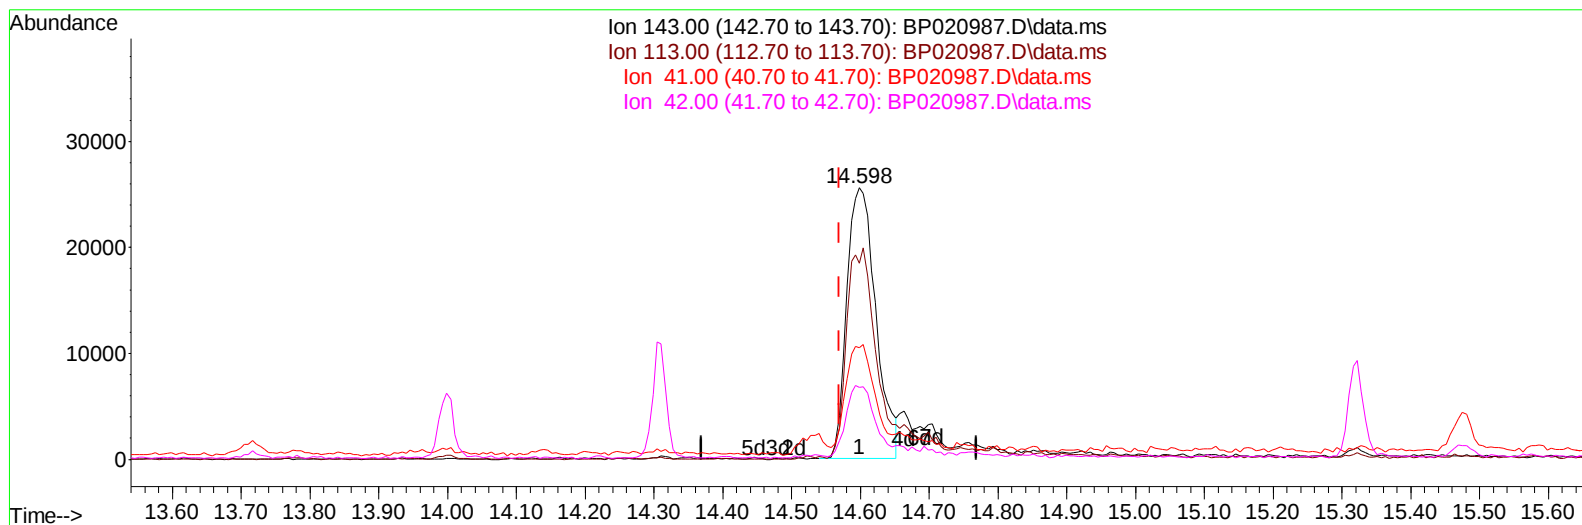

TIC: BP020987.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.598min (+ 0.029) 13.20 ng/u1

response 75309

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	72.30
41.00	37.90	41.08
42.00	27.10	26.51




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020987.D
Acq On : 16 Jul 2024 12:10
Operator : MA/JU
Sample : P3177-18
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BY6

Manual IntegrationsAPPROVED

Quant Time: Jul 16 22:55:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024

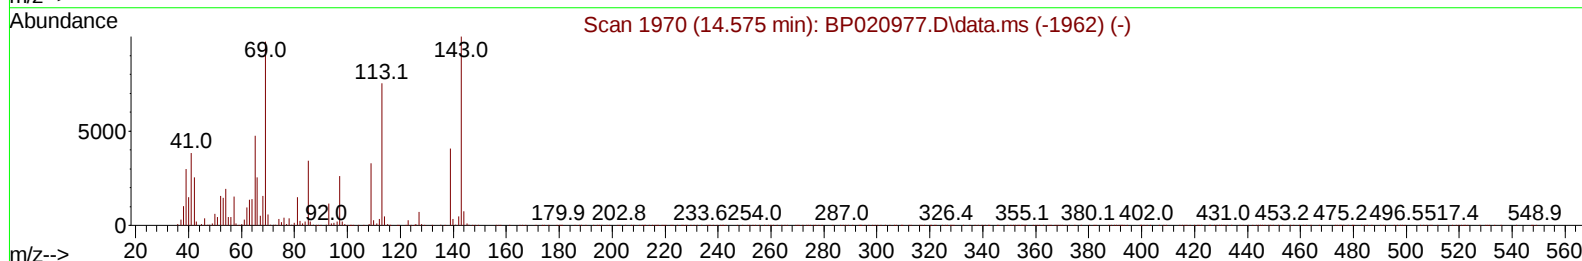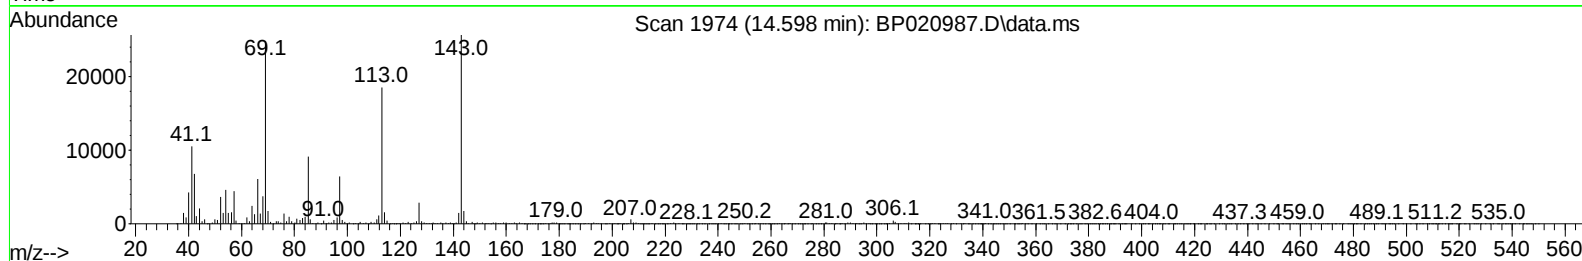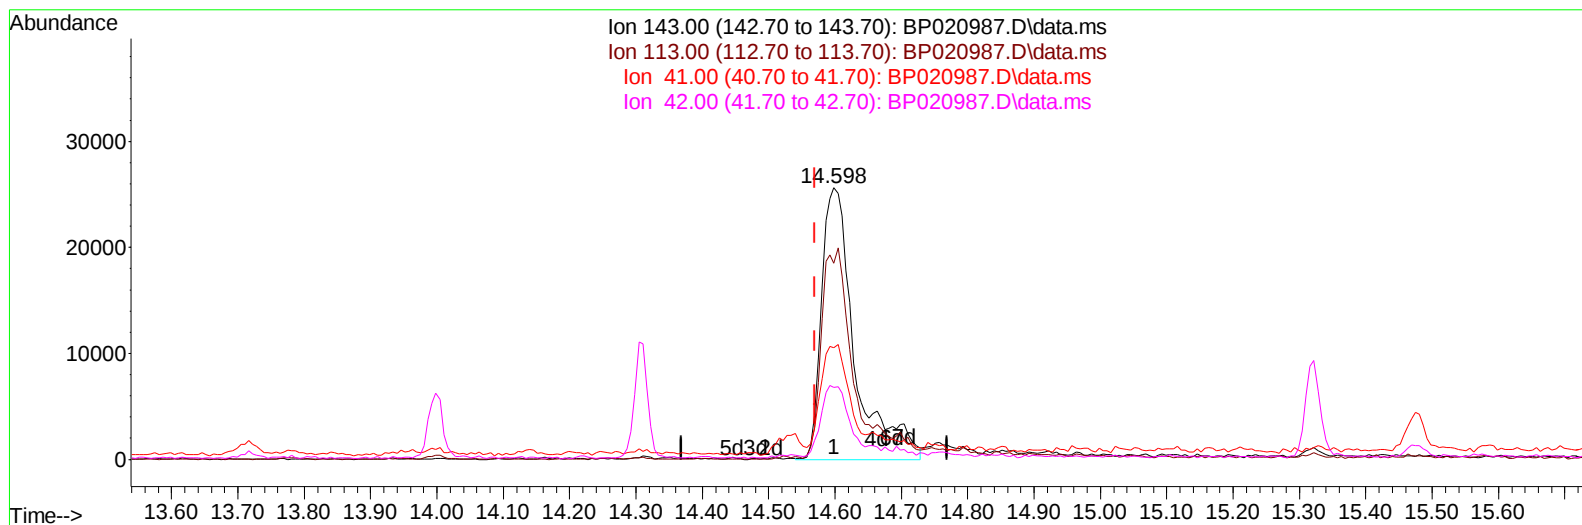

TIC: BP020987.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.598min (+ 0.029) 15.60 ng/ul m

response 89013

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	72.30
41.00	37.90	41.08
42.00	27.10	26.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
 Data File : BP020987.D
 Acq On : 16 Jul 2024 12:10
 Operator : MA/JU
 Sample : P3177-18
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BY6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/18/2024

Quant Time: Jul 16 23:13:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 15 12:22:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	251736	20.000	ng/ul	0.00
20) Naphthalene-d8	10.457	136	932968	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.310	164	551559	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	1130903	20.000	ng/ul	0.01
79) Chrysene-d12	21.557	240	1215811	20.000	ng/ul	0.00
88) Perylene-d12	24.863	264	1507909	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	15429	2.789	ng/uL	0.00
4) Pyridine-d5	3.658	84	211213	13.188	ng/ul	0.00
7) Phenol-d5	6.893	99	318025	15.496	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	197060	15.844	ng/ul	0.00
11) 2-Chlorophenol-d4	7.240	132	278899	16.494	ng/ul	0.00
15) 4-Methylphenol-d8	8.405	113	262060	15.374	ng/ul	0.01
21) Nitrobenzene-d5	8.846	128	128341	17.711	ng/ul	0.02
24) 2-Nitrophenol-d4	9.558	143	144177	17.383	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.099	165	246027	16.405	ng/ul	0.01
31) 4-Chloroaniline-d4	10.605	131	324902	16.353	ng/ul	0.02
46) Dimethylphthalate-d6	13.716	166	721928	18.005	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	829178	18.417	ng/ul	0.00
54) 4-Nitrophenol-d4	14.598	143	89013m	15.603	ng/ul	0.03
60) Fluorene-d10	15.322	176	620434	18.862	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	79340	11.595	ng/ul	0.01
73) Anthracene-d10	17.222	188	946973	18.853	ng/ul	0.00
81) Pyrene-d10	19.610	212	1206846	16.056	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.633	264	1389439	18.683	ng/ul	0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020987.D
Acq On : 16 Jul 2024 12:10
Operator : MA/JU
Sample : P3177-18
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BY6

Manual IntegrationsAPPROVED

Quant Time: Jul 16 23:13:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024

