

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
 Data File : BP020968.D
 Acq On : 15 Jul 2024 21:48
 Operator : MA/JU
 Sample : P3100-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BY0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/16/2024
 Supervised By :mohammad ahmed 07/18/2024

Quant Time: Jul 15 23:10:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 15 12:22:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	170366	20.000	ng/u1	0.01
20) Naphthalene-d8	10.457	136	661870	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.304	164	440366	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.122	188	956190	20.000	ng/u1	0.00
79) Chrysene-d12	21.563	240	963827	20.000	ng/u1	0.01
88) Perylene-d12	24.845	264	1170594	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	15838	4.230	ng/uL	0.00
4) Pyridine-d5	3.681	84	21111	1.948	ng/u1	0.03
7) Phenol-d5	6.905	99	335656	24.166	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.052	67	202654	24.076	ng/u1	0.02
11) 2-Chlorophenol-d4	7.252	132	286998	25.079	ng/u1	0.02
15) 4-Methylphenol-d8	8.416	113	257039	22.282	ng/u1	0.02
21) Nitrobenzene-d5	8.857	128	132040	25.685	ng/u1	0.03
24) 2-Nitrophenol-d4	9.557	143	153983	26.170	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	10.104	165	264071	24.820	ng/u1	0.02
31) 4-Chloroaniline-d4	10.610	131	232168	16.472	ng/u1	0.02
46) Dimethylphthalate-d6	13.728	166	896445	28.003	ng/u1	0.02
49) Acenaphthylene-d8	14.004	160	992638	27.615	ng/u1	0.00
54) 4-Nitrophenol-d4	14.581	143	110201	24.195	ng/u1	0.01
60) Fluorene-d10	15.322	176	796318	30.321	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	113321	19.587	ng/u1	0.02
73) Anthracene-d10	17.222	188	1287870	30.325	ng/u1	0.00
81) Pyrene-d10	19.610	212	1386556	23.269	ng/u1	0.01
92) Benzo(a)pyrene-d12	24.615	264	1058589	18.336	ng/u1	0.01
Target Compounds						
					Qvalue	
80) Fluoranthene	19.257	202	105071	1.460	ng/u1	99
82) Pyrene	19.633	202	84759	1.157	ng/u1	95
87) Chrysene	21.610	228	66597m	1.062	ng/u1	
90) Benzo(b)fluoranthene	23.804	252	88884	1.251	ng/u1#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020968.D
Acq On : 15 Jul 2024 21:48
Operator : MA/JU
Sample : P3100-14
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A4BY0

Quant Time: Jul 15 23:10:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/16/2024
Supervised By :mohammad ahmed 07/18/2024

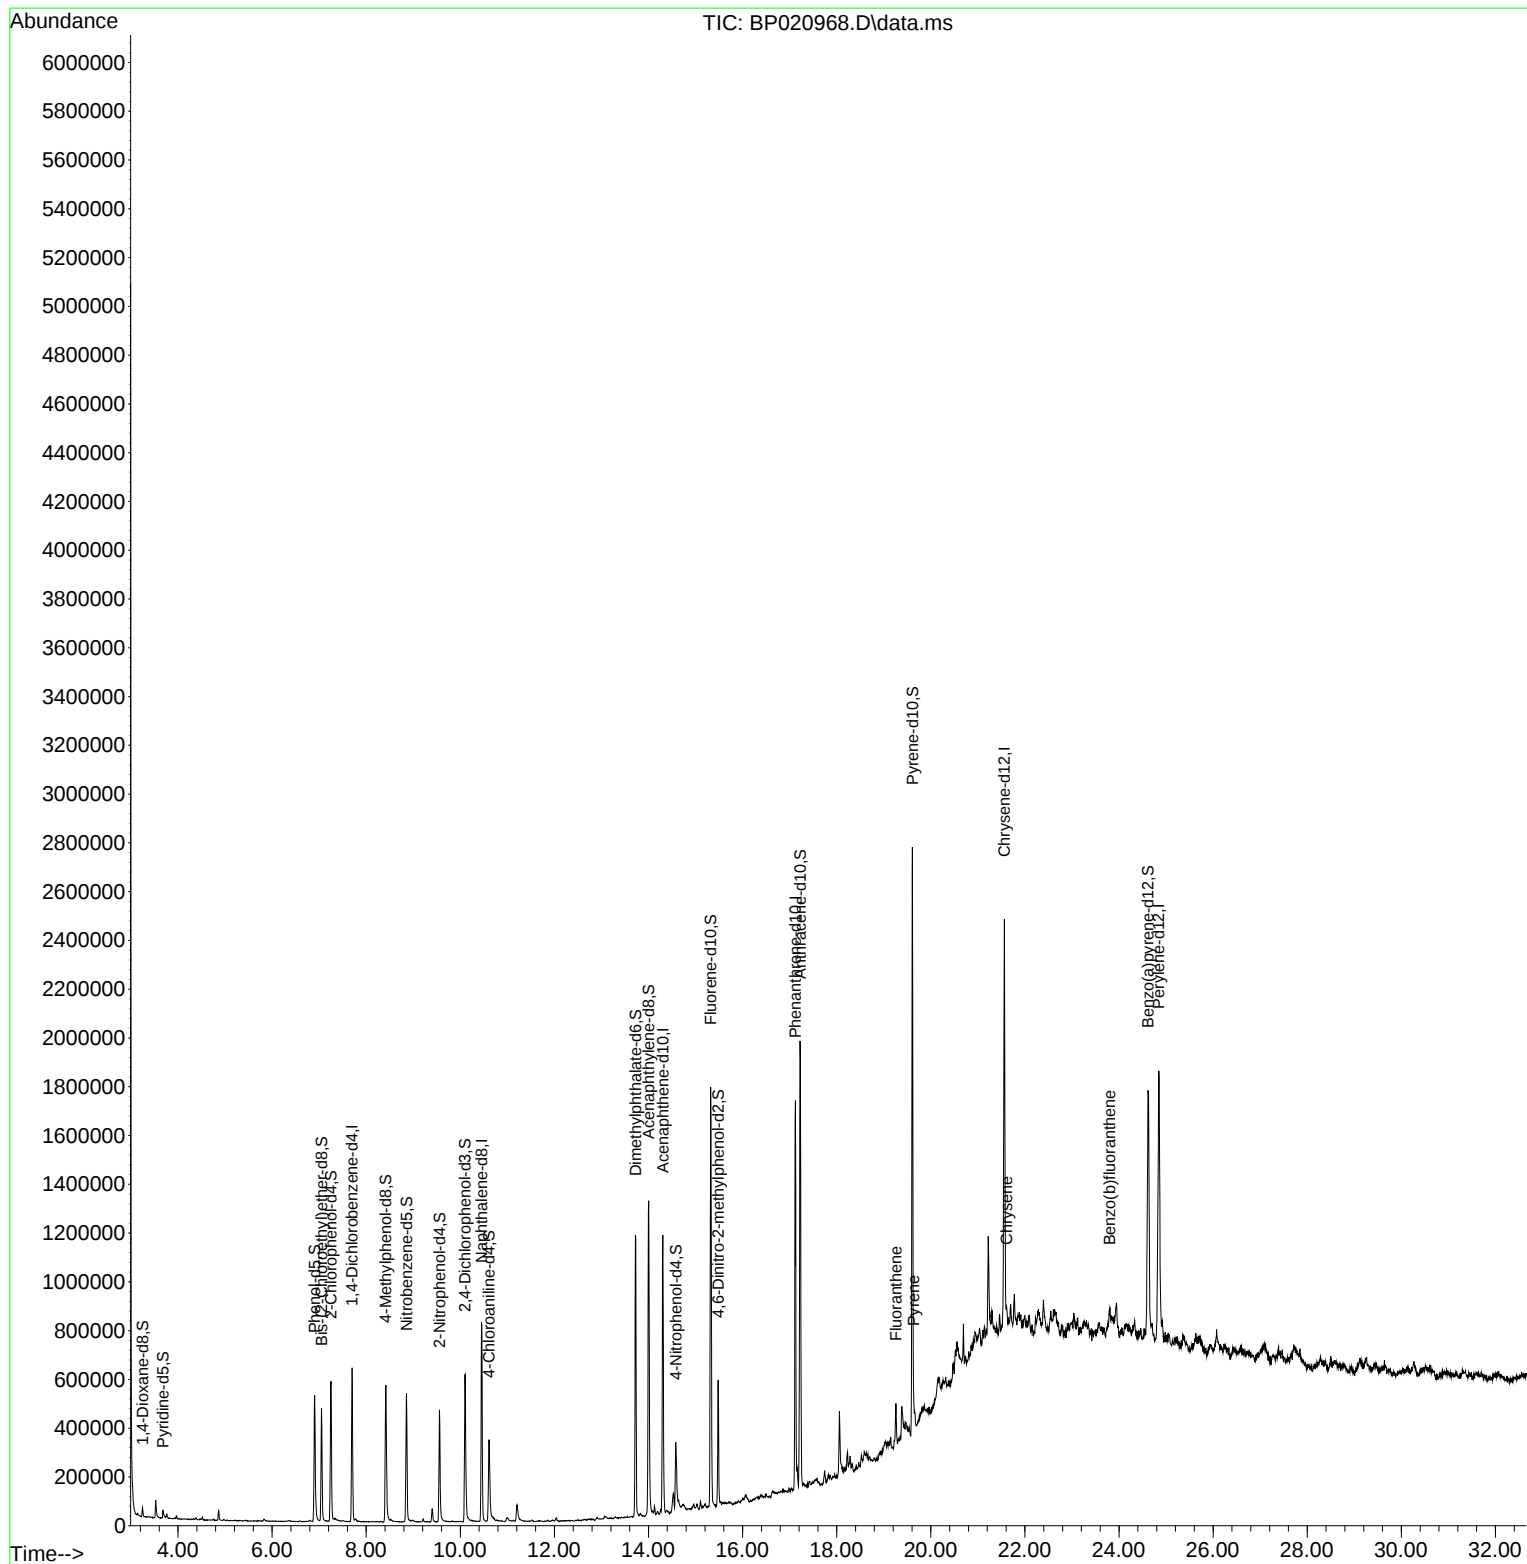

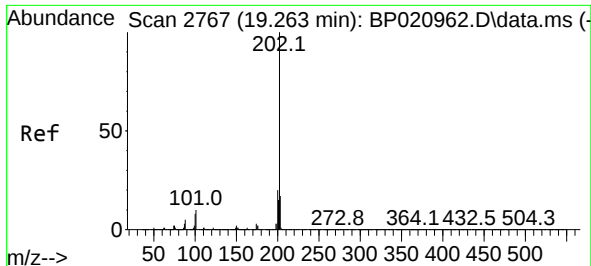

#80
Fluoranthene
Concen: 1.460 ng/ul
RT: 19.257 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP020968.D
Acq: 15 Jul 2024 21:48




Instrument :
BNA_P
ClientSampleId :
A4BY0

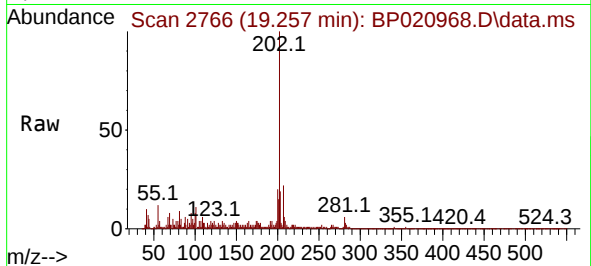

Tgt Ion:202 Resp: 10507
Ion Ratio Lower Upper
202 100
101 10.6 8.0 12.0
100 7.9 6.1 9.1




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/16/2024
Supervised By :mohammad ahmed 07/18/2024

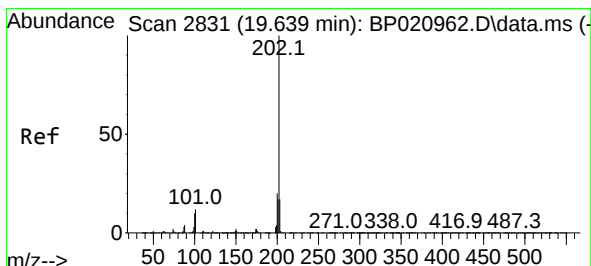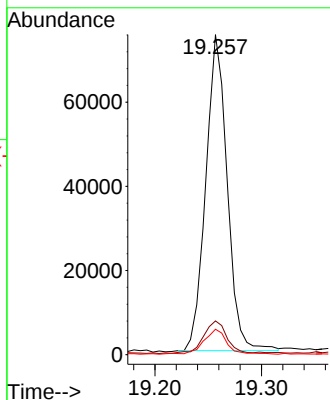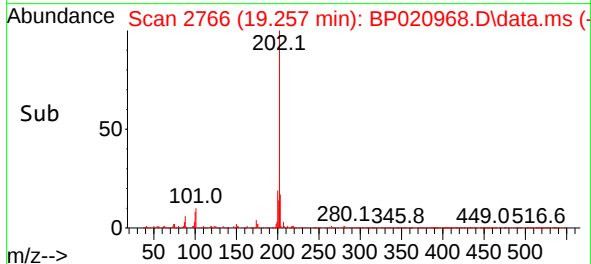

#82
Pyrene
Concen: 1.157 ng/ul
RT: 19.633 min Scan# 2830
Delta R.T. 0.006 min
Lab File: BP020968.D
Acq: 15 Jul 2024 21:48

Tgt Ion:202 Resp: 84759
Ion Ratio Lower Upper
202 100
101 13.6 9.4 14.2
100 11.6 7.8 11.6

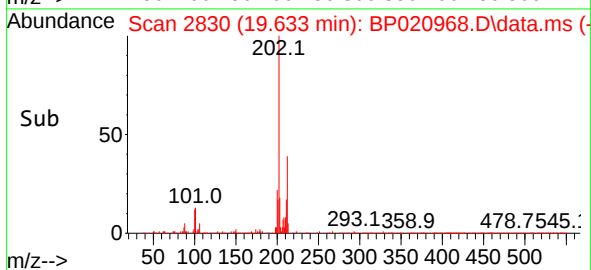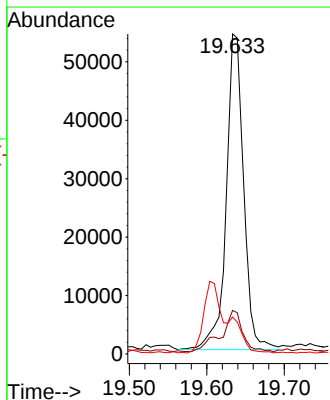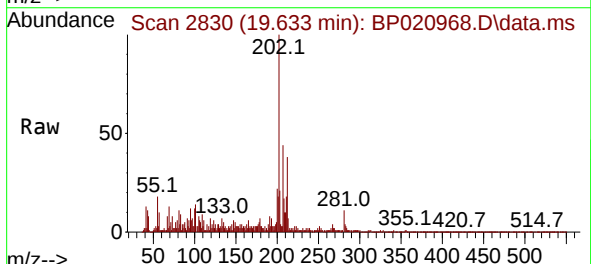

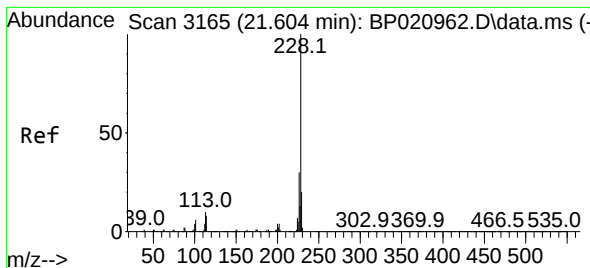

#87

Chrysene

Concen: 1.062 ng/ul m

RT: 21.610 min Scan# 3166

Delta R.T. 0.012 min

Lab File: BP020968.D

Acq: 15 Jul 2024 21:48

Instrument :

BNA_P

ClientSampleId :

A4BY0





Tgt Ion:	228	Resp:	6659
Ion Ratio	Lower	Upper	
228	100		
226	34.4	23.6	35.4
229	31.8	15.5	23.3

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/16/2024

Supervised By :mohammad ahmed 07/18/2024

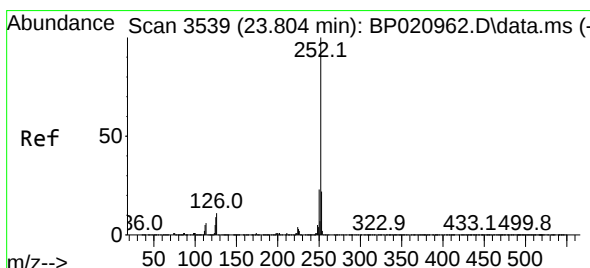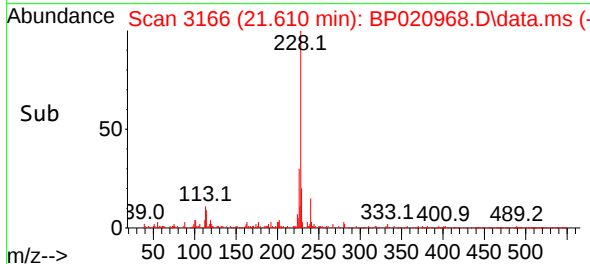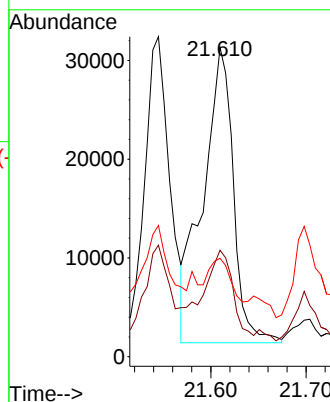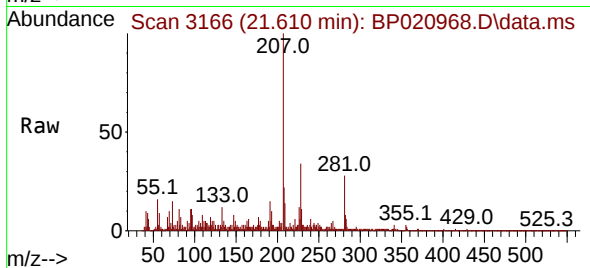

#90

Benzo(b)fluoranthene

Concen: 1.251 ng/ul

RT: 23.804 min Scan# 3539

Delta R.T. 0.023 min

Lab File: BP020968.D

Acq: 15 Jul 2024 21:48

Tgt Ion:	252	Resp:	88884
Ion Ratio	Lower	Upper	
252	100		
253	31.3	17.1	25.7#
125	17.4	7.0	10.4#

