

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
 Data File : BP021000.D
 Acq On : 16 Jul 2024 21:38
 Operator : MA/JU
 Sample : P3178-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BY4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/18/2024

Quant Time: Jul 16 23:43:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 15 12:22:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	193252	20.000	ng/u1	0.00
20) Naphthalene-d8	10.457	136	778562	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.316	164	504351	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.122	188	1047708	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	1090217	20.000	ng/u1	0.00
88) Perylene-d12	24.851	264	1309619	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	15504	3.651	ng/uL	0.00
4) Pyridine-d5	3.663	84	215569	17.534	ng/u1	0.01
7) Phenol-d5	6.899	99	339768	21.565	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	204761	21.445	ng/u1	0.00
11) 2-Chlorophenol-d4	7.246	132	281308	21.671	ng/u1	0.01
15) 4-Methylphenol-d8	8.404	113	283148	21.638	ng/u1	0.01
21) Nitrobenzene-d5	8.840	128	138047	22.828	ng/u1	0.01
24) 2-Nitrophenol-d4	9.551	143	155480	22.464	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.098	165	277679	22.187	ng/u1	0.01
31) 4-Chloroaniline-d4	10.604	131	378695	22.840	ng/u1	0.02
46) Dimethylphthalate-d6	13.716	166	882928	24.082	ng/u1	0.00
49) Acenaphthylene-d8	14.004	160	1004107	24.390	ng/u1	0.00
54) 4-Nitrophenol-d4	14.581	143	112388m	21.545	ng/u1	0.01
60) Fluorene-d10	15.322	176	773909	25.730	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	98968	15.612	ng/u1	0.00
73) Anthracene-d10	17.222	188	1209948	26.001	ng/u1	0.00
81) Pyrene-d10	19.598	212	1490398	22.112	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.621	264	1626916	25.188	ng/u1	0.02
Target Compounds						
					Qvalue	
80) Fluoranthene	19.251	202	98297	1.208	ng/u1	99
82) Pyrene	19.633	202	98071	1.184	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP021000.D
Acq On : 16 Jul 2024 21:38
Operator : MA/JU
Sample : P3178-16
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A4BY4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024


Quant Time: Jul 16 23:43:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 15 12:22:22 2024
Response via : Initial Calibration

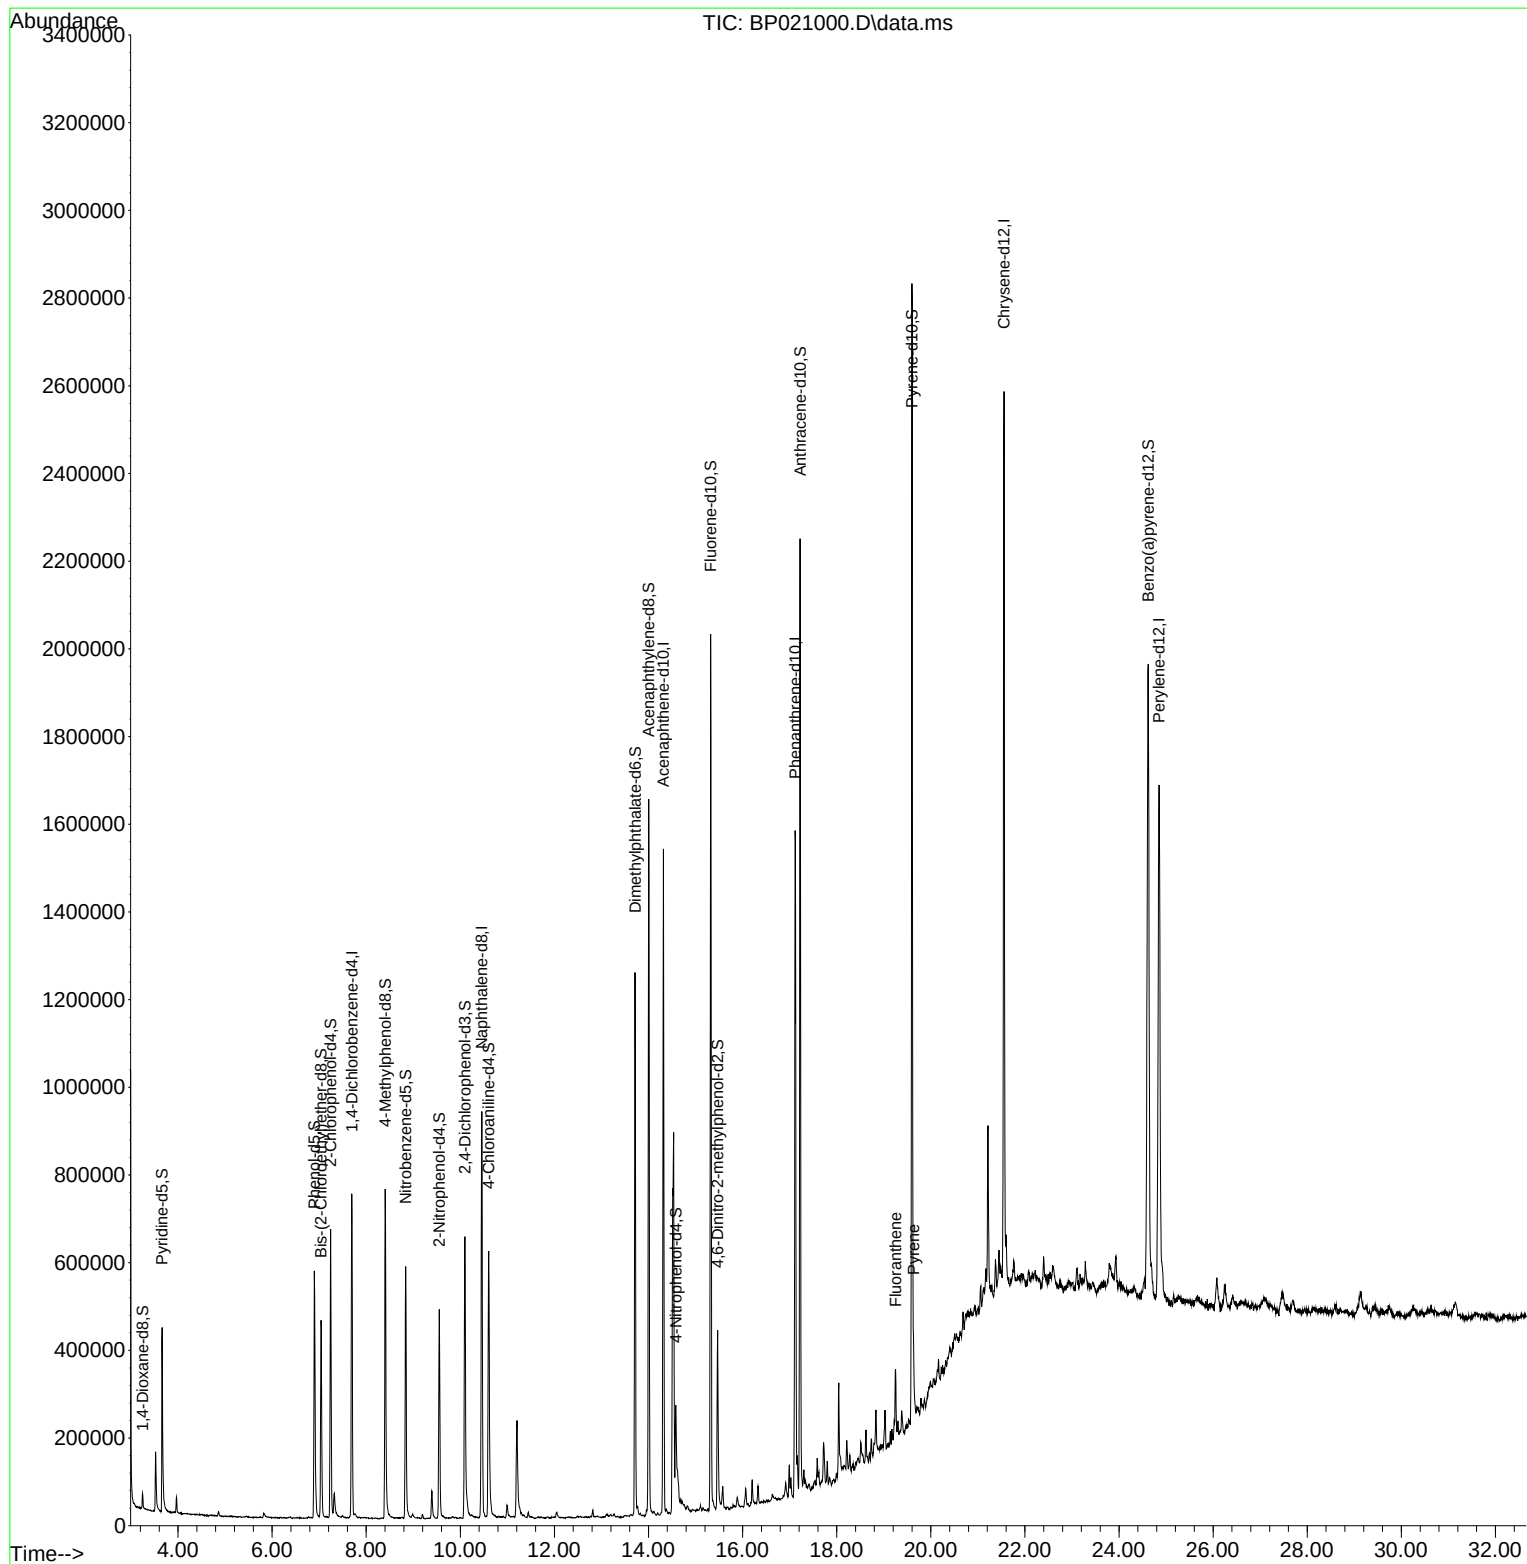

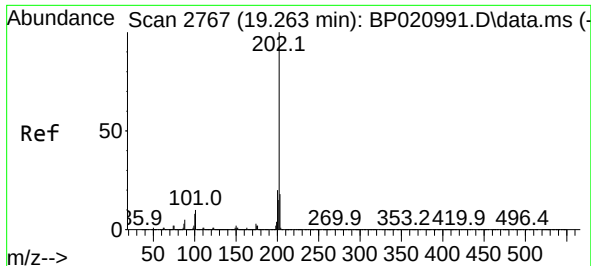

#80
Fluoranthene
Concen: 1.208 ng/ul
RT: 19.251 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP021000.D
Acq: 16 Jul 2024 21:38




Instrument :
BNA_P
ClientSampleId :
A4BY4

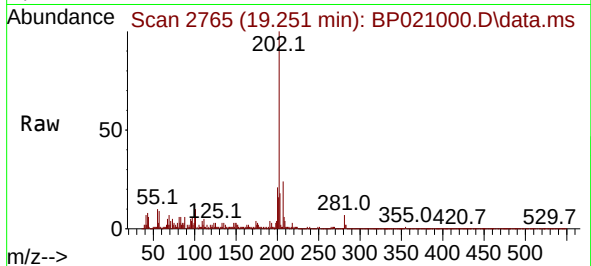

Tgt Ion:202 Resp: 9829
Ion Ratio Lower Upper
202 100
101 10.4 8.0 12.0
100 8.0 6.1 9.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/18/2024

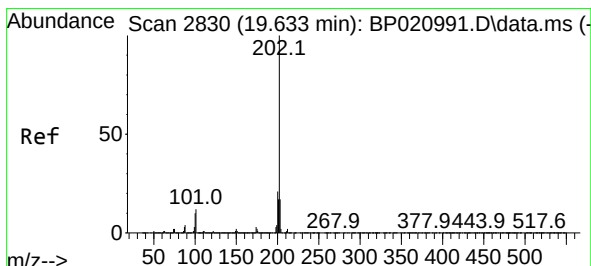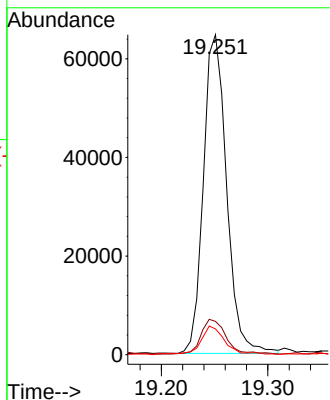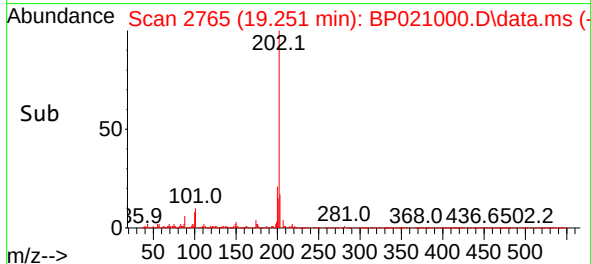

#82
Pyrene
Concen: 1.184 ng/ul
RT: 19.633 min Scan# 2830
Delta R.T. 0.006 min
Lab File: BP021000.D
Acq: 16 Jul 2024 21:38

Tgt Ion:202 Resp: 98071
Ion Ratio Lower Upper
202 100
101 10.7 9.4 14.2
100 9.2 7.8 11.6

