

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
 Data File : BP020963.D
 Acq On : 15 Jul 2024 18:08
 Operator : MA/JU
 Sample : PB162022BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	54	rVB	54067	73025	1.81%	0.175%
2	3.664	111	115	140	rVB	625350	930288	23.04%	2.230%
3	3.970	163	167	172	rBV	15643	20018	0.50%	0.048%
4	6.905	659	666	678	rBV	616750	1125472	27.88%	2.698%
5	7.046	683	690	703	rVB	572564	884630	21.91%	2.121%
6	7.246	717	724	739	rBV	725036	1192876	29.55%	2.860%
7	7.699	794	801	810	rBV	646459	1032296	25.57%	2.475%
8	8.416	916	923	936	rBV	891184	1425325	35.31%	3.417%
9	8.846	987	996	1008	rBV	719914	1118222	27.70%	2.681%
10	9.557	1109	1117	1128	rBV	546216	966183	23.93%	2.317%
11	10.093	1201	1208	1218	rBV	759564	1378663	34.15%	3.305%
12	10.252	1232	1235	1239	rBV6	2992	4608	0.11%	0.011%
13	10.452	1261	1269	1285	rVB	800029	1431741	35.47%	3.433%
14	10.604	1288	1295	1318	rBV	735669	1440552	35.68%	3.454%
15	12.063	1534	1543	1551	rBV4	9257	29103	0.72%	0.070%
16	13.275	1744	1749	1752	rBV6	3031	5363	0.13%	0.013%
17	13.728	1820	1826	1836	rBV	1481217	2054441	50.89%	4.926%
18	13.804	1836	1839	1847	rVB5	5068	10239	0.25%	0.025%
19	14.016	1865	1875	1887	rBV	1422314	2509233	62.16%	6.016%
20	14.322	1918	1927	1942	rBV	964637	1858911	46.05%	4.457%
21	14.581	1965	1971	1980	rBV	273992	611827	15.16%	1.467%
22	14.740	1996	1998	2002	rVB4	6153	5700	0.14%	0.014%
23	15.334	2091	2099	2110	rBV	2014747	3015804	74.71%	7.231%
24	15.481	2117	2124	2134	rBV	567766	860892	21.33%	2.064%
25	16.116	2228	2232	2239	rVB8	5511	9678	0.24%	0.023%
26	17.116	2396	2402	2413	rBV	1453604	2108896	52.24%	5.056%
27	17.228	2413	2421	2436	rVV2	1751332	3203457	79.35%	7.681%
28	18.057	2558	2562	2571	rBV5	25103	56238	1.39%	0.135%
29	19.151	2744	2748	2752	rVB3	30141	38871	0.96%	0.093%
30	19.604	2819	2825	2838	rBV	2419933	3693183	91.49%	8.855%
31	21.563	3152	3158	3168	rVB	1342921	2205968	54.64%	5.289%
32	24.639	3672	3681	3691	rVB2	1641159	4036908	100.00%	9.679%
33	24.845	3708	3716	3728	rBV2	844131	2369561	58.70%	5.681%




Sum of corrected areas: 41708172

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020963.D
Acq On : 15 Jul 2024 18:08
Operator : MA/JU
Sample : PB162022BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

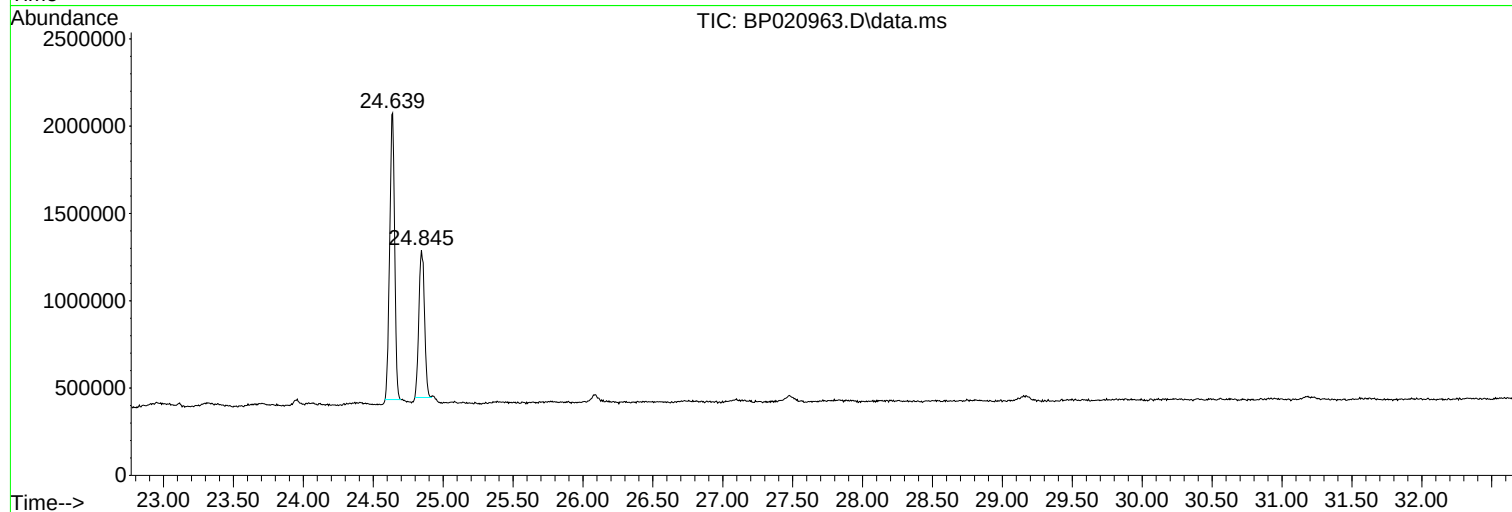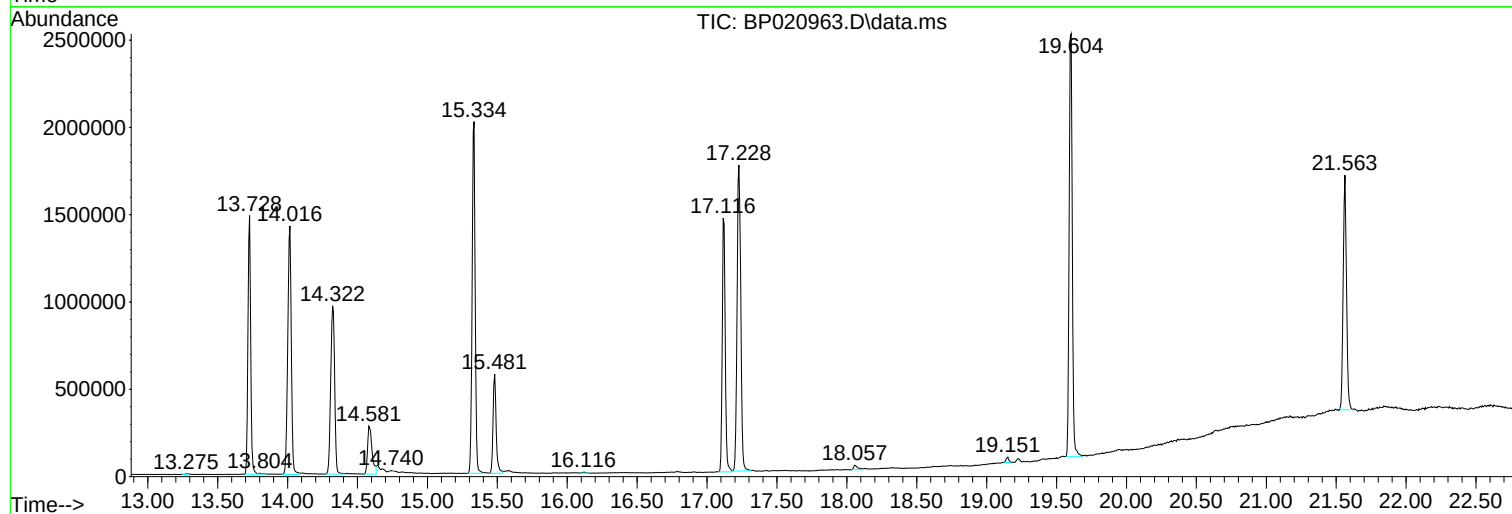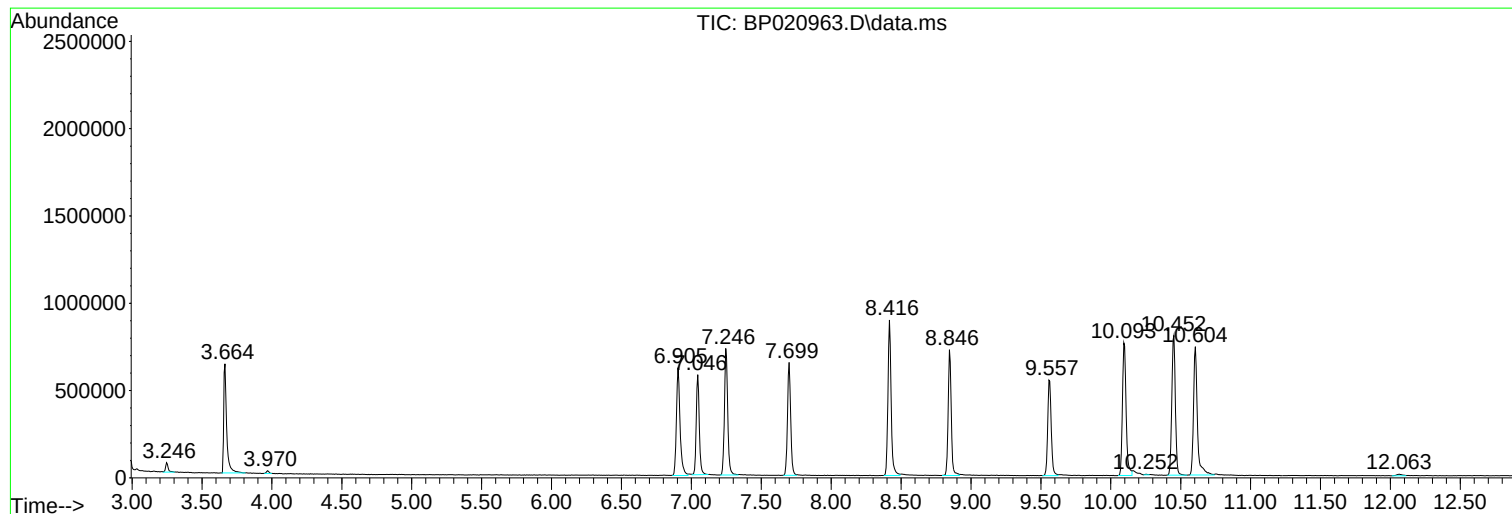

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020963.D
Acq On : 15 Jul 2024 18:08
Operator : MA/JU
Sample : PB162022BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020963.D
Acq On : 15 Jul 2024 18:08
Operator : MA/JU
Sample : PB162022BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc