

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
 Data File : BP020992.D
 Acq On : 16 Jul 2024 15:48
 Operator : MA/JU
 Sample : PB162047BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	50	rBV	57652	71148	1.74%	0.131%
2	3.652	111	113	134	rBV	744481	1108431	27.17%	2.044%
3	3.958	162	165	170	rVB	19449	25819	0.63%	0.048%
4	6.893	657	664	680	rBV	823756	1463341	35.87%	2.698%
5	7.040	683	689	708	rVB	702434	1153441	28.27%	2.127%
6	7.240	715	723	738	rBV	880878	1488140	36.48%	2.744%
7	7.693	792	800	810	rBV	1011893	1639127	40.18%	3.022%
8	8.404	913	921	945	rBV	1000376	1883658	46.17%	3.473%
9	8.563	945	948	956	rVB10	2982	7534	0.18%	0.014%
10	8.846	987	996	1012	rBV	764838	1510970	37.04%	2.786%
11	9.551	1107	1116	1124	rBV	732287	1295972	31.77%	2.389%
12	10.093	1200	1208	1227	rBV	940273	1952930	47.87%	3.601%
13	10.457	1262	1270	1281	rBV	1441186	2489317	61.02%	4.590%
14	10.598	1286	1294	1314	rBV	944629	1935206	47.43%	3.568%
15	10.828	1331	1333	1339	rVB7	2863	4274	0.10%	0.008%
16	12.045	1535	1540	1552	rBV2	14336	31701	0.78%	0.058%
17	13.716	1817	1824	1840	rBV	1683066	2739116	67.14%	5.050%
18	13.998	1866	1872	1885	rBV	2298047	3279839	80.39%	6.047%
19	14.316	1919	1926	1944	rBV	2359461	3219734	78.92%	5.936%
20	14.581	1964	1971	1975	rBV2	236101	496765	12.18%	0.916%
21	14.698	1990	1991	1998	rVB6	14788	23151	0.57%	0.043%
22	14.786	2005	2006	2011	rVB5	5201	6736	0.17%	0.012%
23	14.845	2014	2016	2023	rVB7	4025	7409	0.18%	0.014%
24	15.322	2090	2097	2114	rBV	2558049	3824349	93.74%	7.051%
25	15.475	2114	2123	2135	rVV	510371	927387	22.73%	1.710%
26	15.569	2135	2139	2145	rVB	16226	25293	0.62%	0.047%
27	16.128	2230	2234	2237	rBV6	6302	8171	0.20%	0.015%
28	16.792	2344	2347	2350	rBV4	4414	5043	0.12%	0.009%
29	16.898	2363	2365	2371	rBV3	5095	6788	0.17%	0.013%
30	17.128	2396	2404	2414	rBV	2081211	3113802	76.32%	5.741%
31	17.227	2414	2421	2438	rVV	2431166	3534127	86.63%	6.516%
32	17.804	2516	2519	2524	rVB6	7670	9868	0.24%	0.018%
33	18.057	2557	2562	2565	rBV6	14193	27558	0.68%	0.051%
34	19.151	2744	2748	2755	rBV4	27106	46044	1.13%	0.085%
35	19.233	2759	2762	2767	rVV2	21231	33682	0.83%	0.062%
36	19.610	2820	2826	2836	rBV	2530328	3813037	93.46%	7.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020992.D
Acq On : 16 Jul 2024 15:48
Operator : MA/JU
Sample : PB162047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK047

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	21.568	3153	3159	3172	rVB	2045886	3183606	78.04%	5.870%
38	24.645	3673	3682	3697	rVB2	1476339	4079710	100.00%	7.522%
39	24.880	3713	3722	3742	rVB	1222877	3764040	92.26%	6.940%




Sum of corrected areas: 54236264

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020992.D
Acq On : 16 Jul 2024 15:48
Operator : MA/JU
Sample : PB162047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

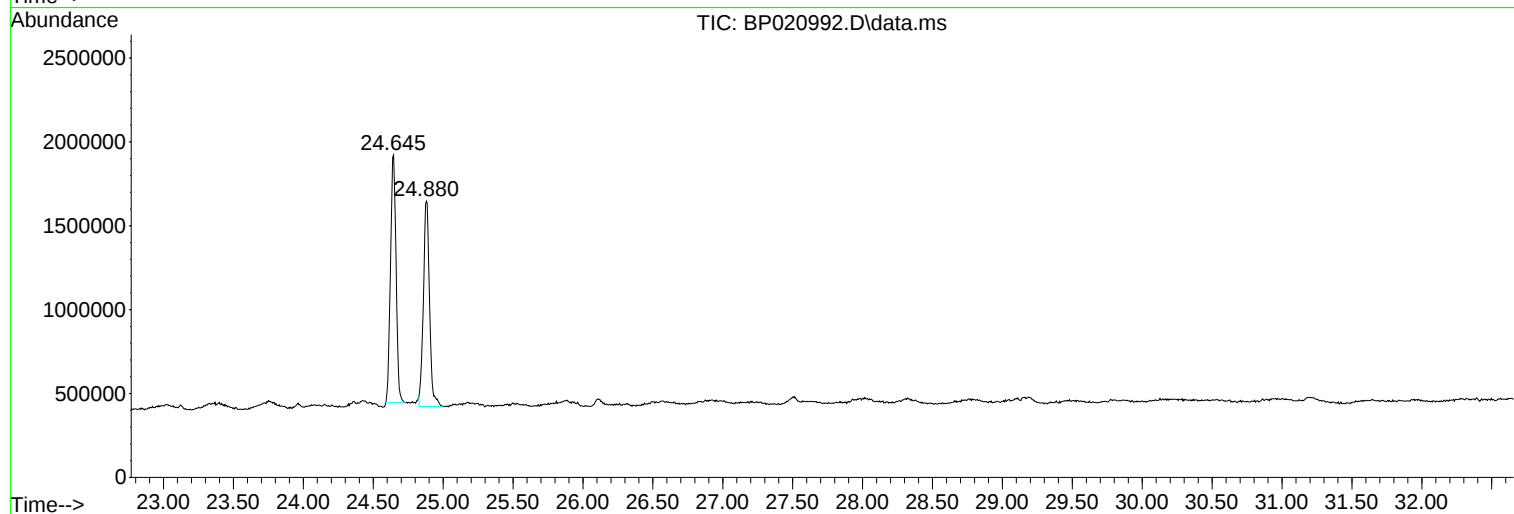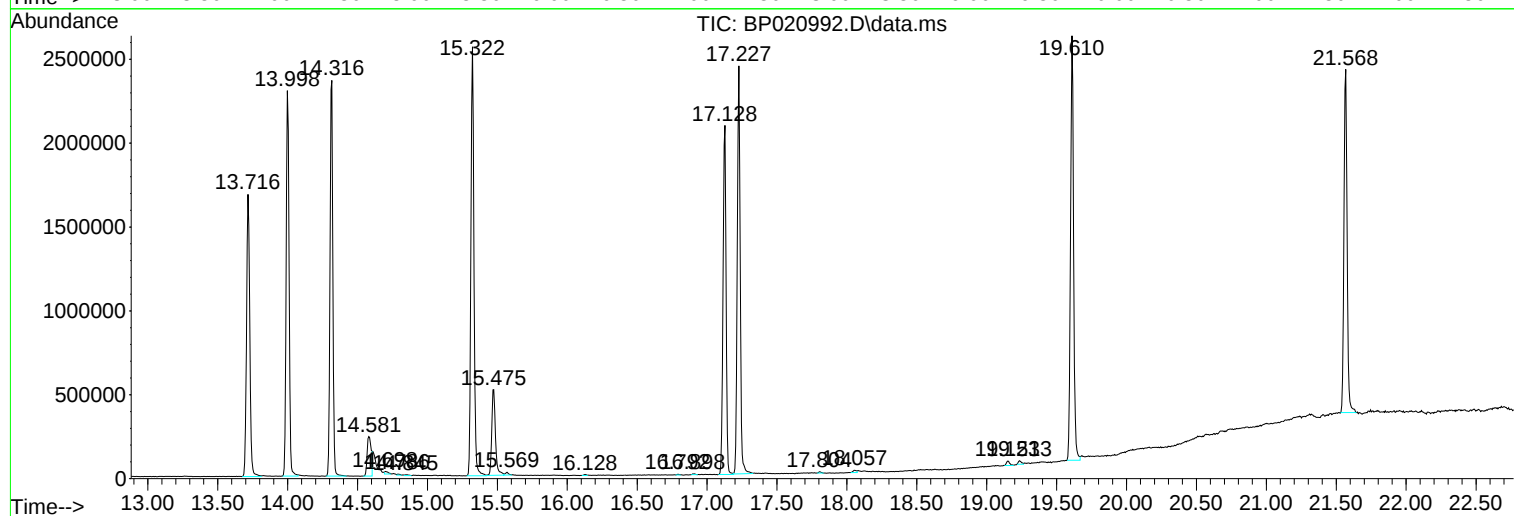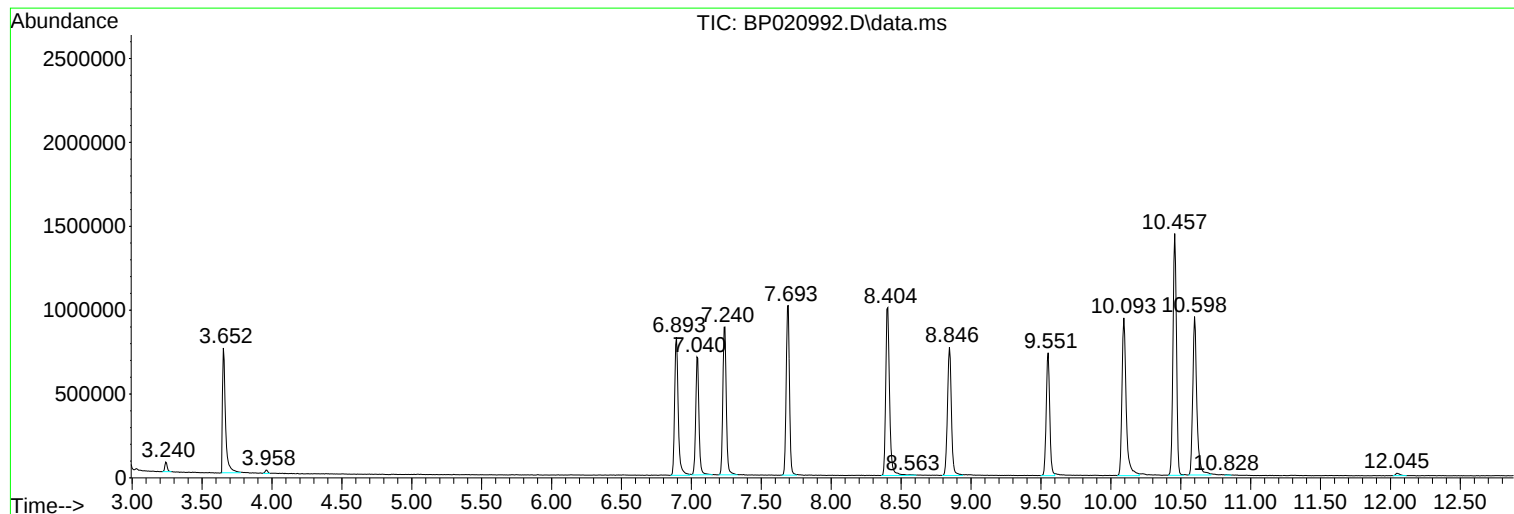

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020992.D
Acq On : 16 Jul 2024 15:48
Operator : MA/JU
Sample : PB162047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071524\
Data File : BP020992.D
Acq On : 16 Jul 2024 15:48
Operator : MA/JU
Sample : PB162047BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc