
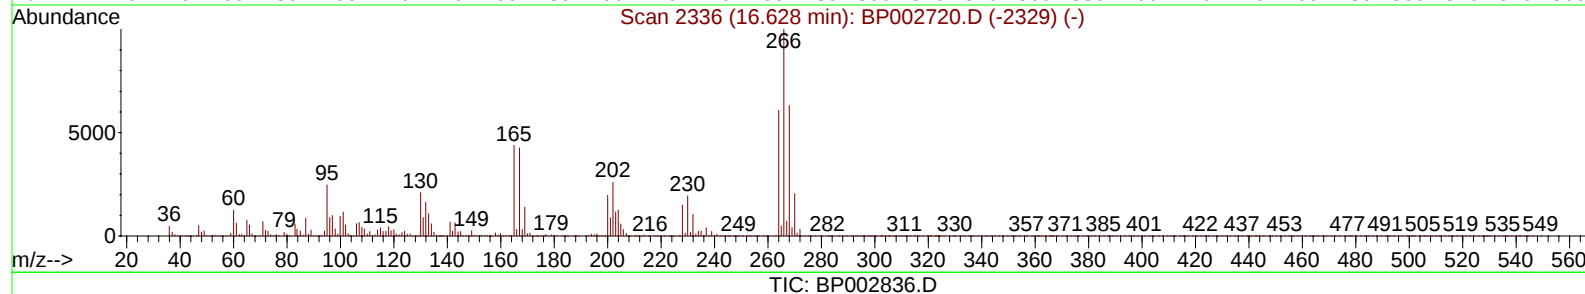
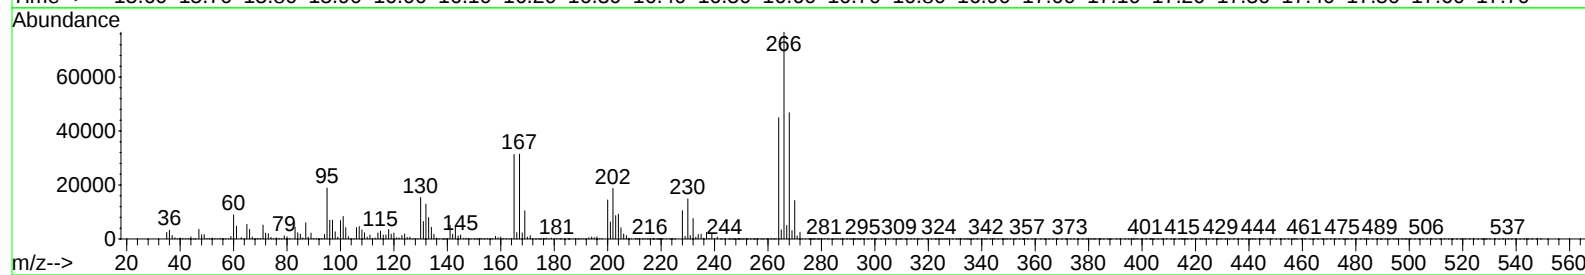


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072320\
Data File : BP002836.D
Acq On : 23 Jul 2020 12:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 18:59:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

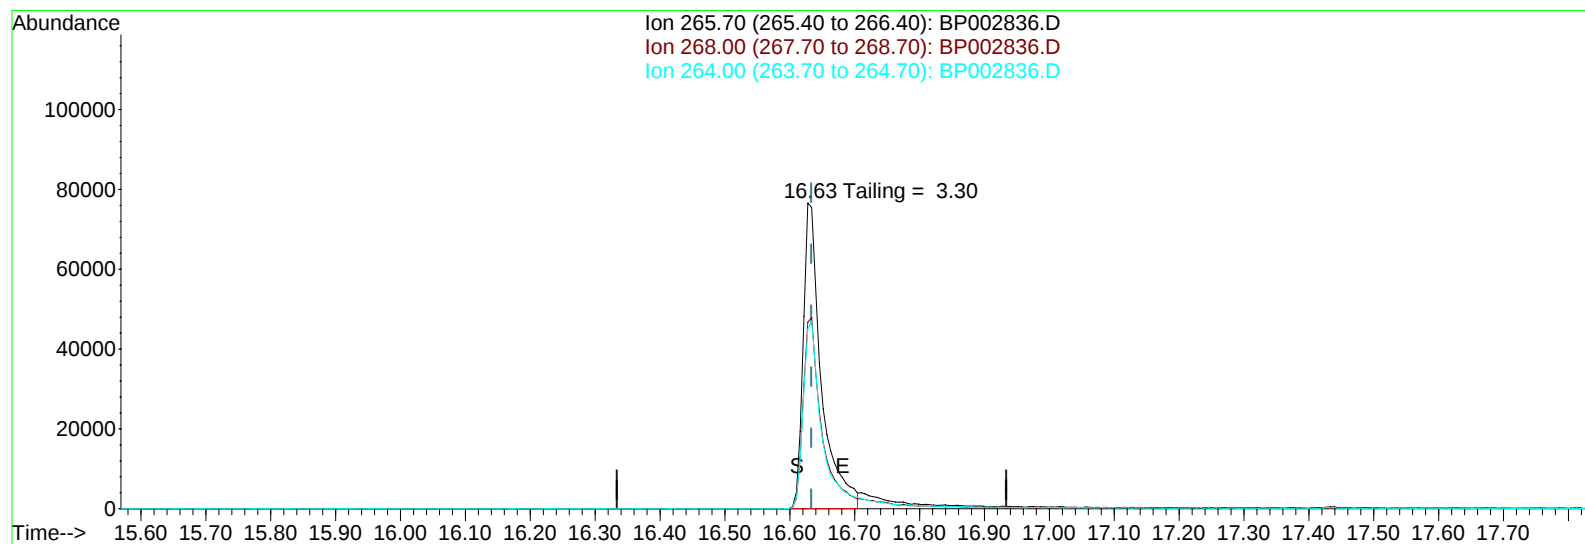

(70) Pentachlorophenol (C)




16.628min (-0.006) 57918.52ng

response 164099

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	61.04
264.00	60.70	58.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072320\
 Data File : BP002836.D
 Acq On : 23 Jul 2020 12:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 18:59:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

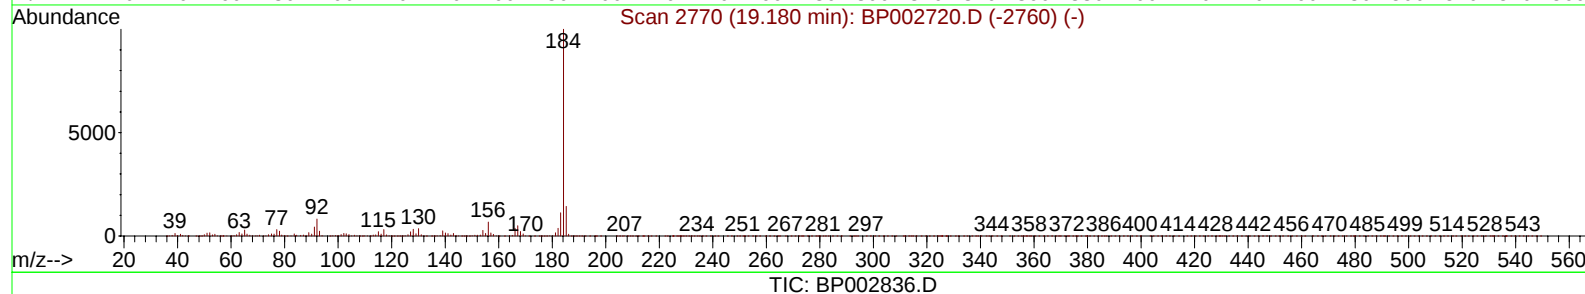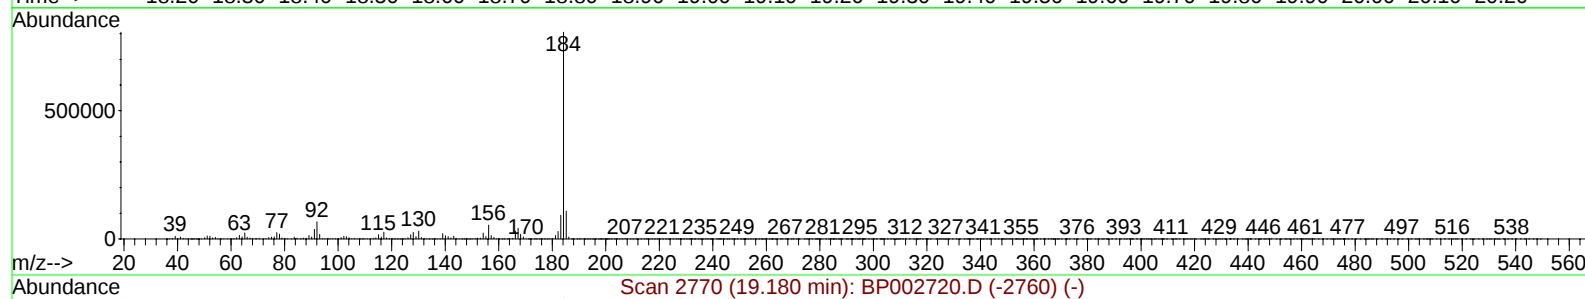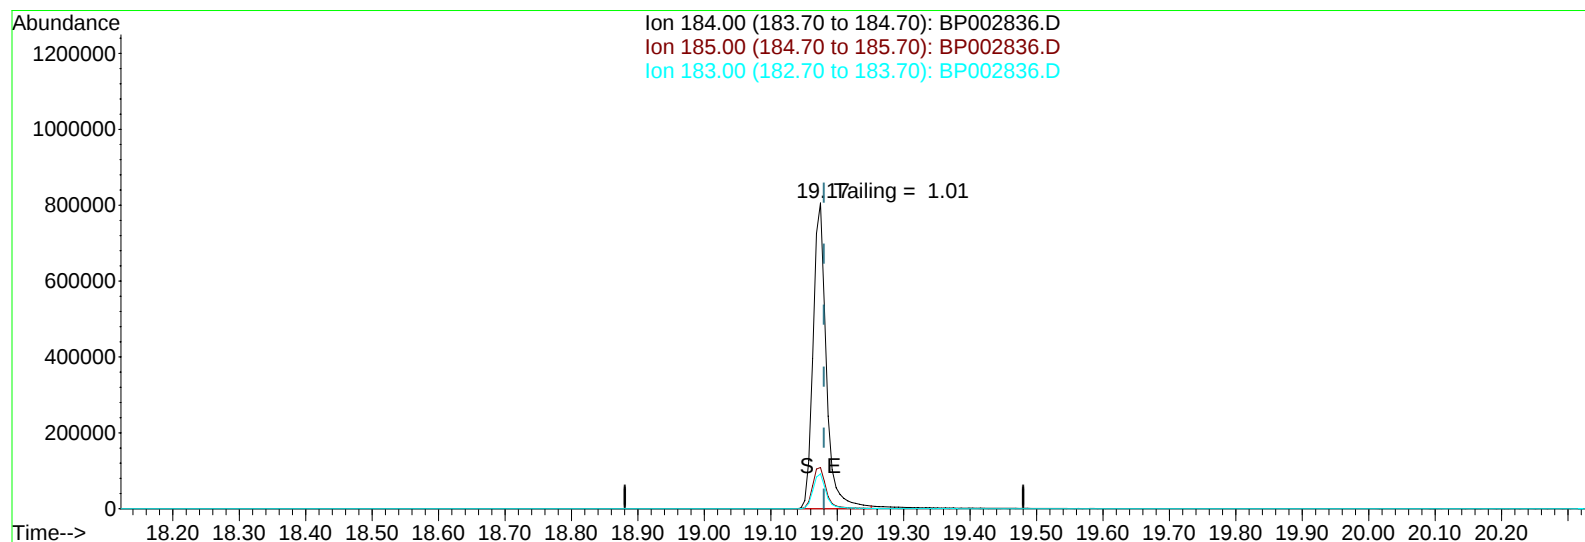

(77) Benzidine

19.175min (-0.006) 64526.57ng

response 1137184

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	13.49
183.00	11.20	11.43
0.00	0.00	0.00