

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072320\
Data File : BP002838.D
Acq On : 23 Jul 2020 13:48
Operator : CG/JU
Sample : PB130378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130378BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.175	382	389	414	rBV	2315219	3620850	53.40%	10.534%
2	6.752	650	657	683	rBV	2121485	3707020	54.68%	10.785%
3	7.546	785	792	804	rBV	507729	810467	11.95%	2.358%
4	8.693	979	987	1015	rBV	1414265	2468180	36.40%	7.181%
5	10.316	1252	1263	1283	rBV	600486	1116420	16.47%	3.248%
6	12.816	1680	1688	1709	rBV	2931839	4931547	72.74%	14.348%
7	14.198	1916	1923	1939	rBV	904365	1490786	21.99%	4.337%
8	15.704	2172	2179	2203	rBV	2066212	3597209	53.06%	10.465%
9	16.963	2386	2393	2410	rBV	1187987	1820349	26.85%	5.296%
10	19.551	2827	2833	2851	rBV2	4862318	6780048	100.00%	19.725%
11	21.075	3087	3092	3105	rBV	1609190	2088410	30.80%	6.076%
12	23.263	3457	3464	3476	rBV2	992648	1940816	28.63%	5.646%


Sum of corrected areas: 34372102

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072320\
Data File : BP002838.D
Acq On : 23 Jul 2020 13:48
Operator : CG/JU
Sample : PB130378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130378BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

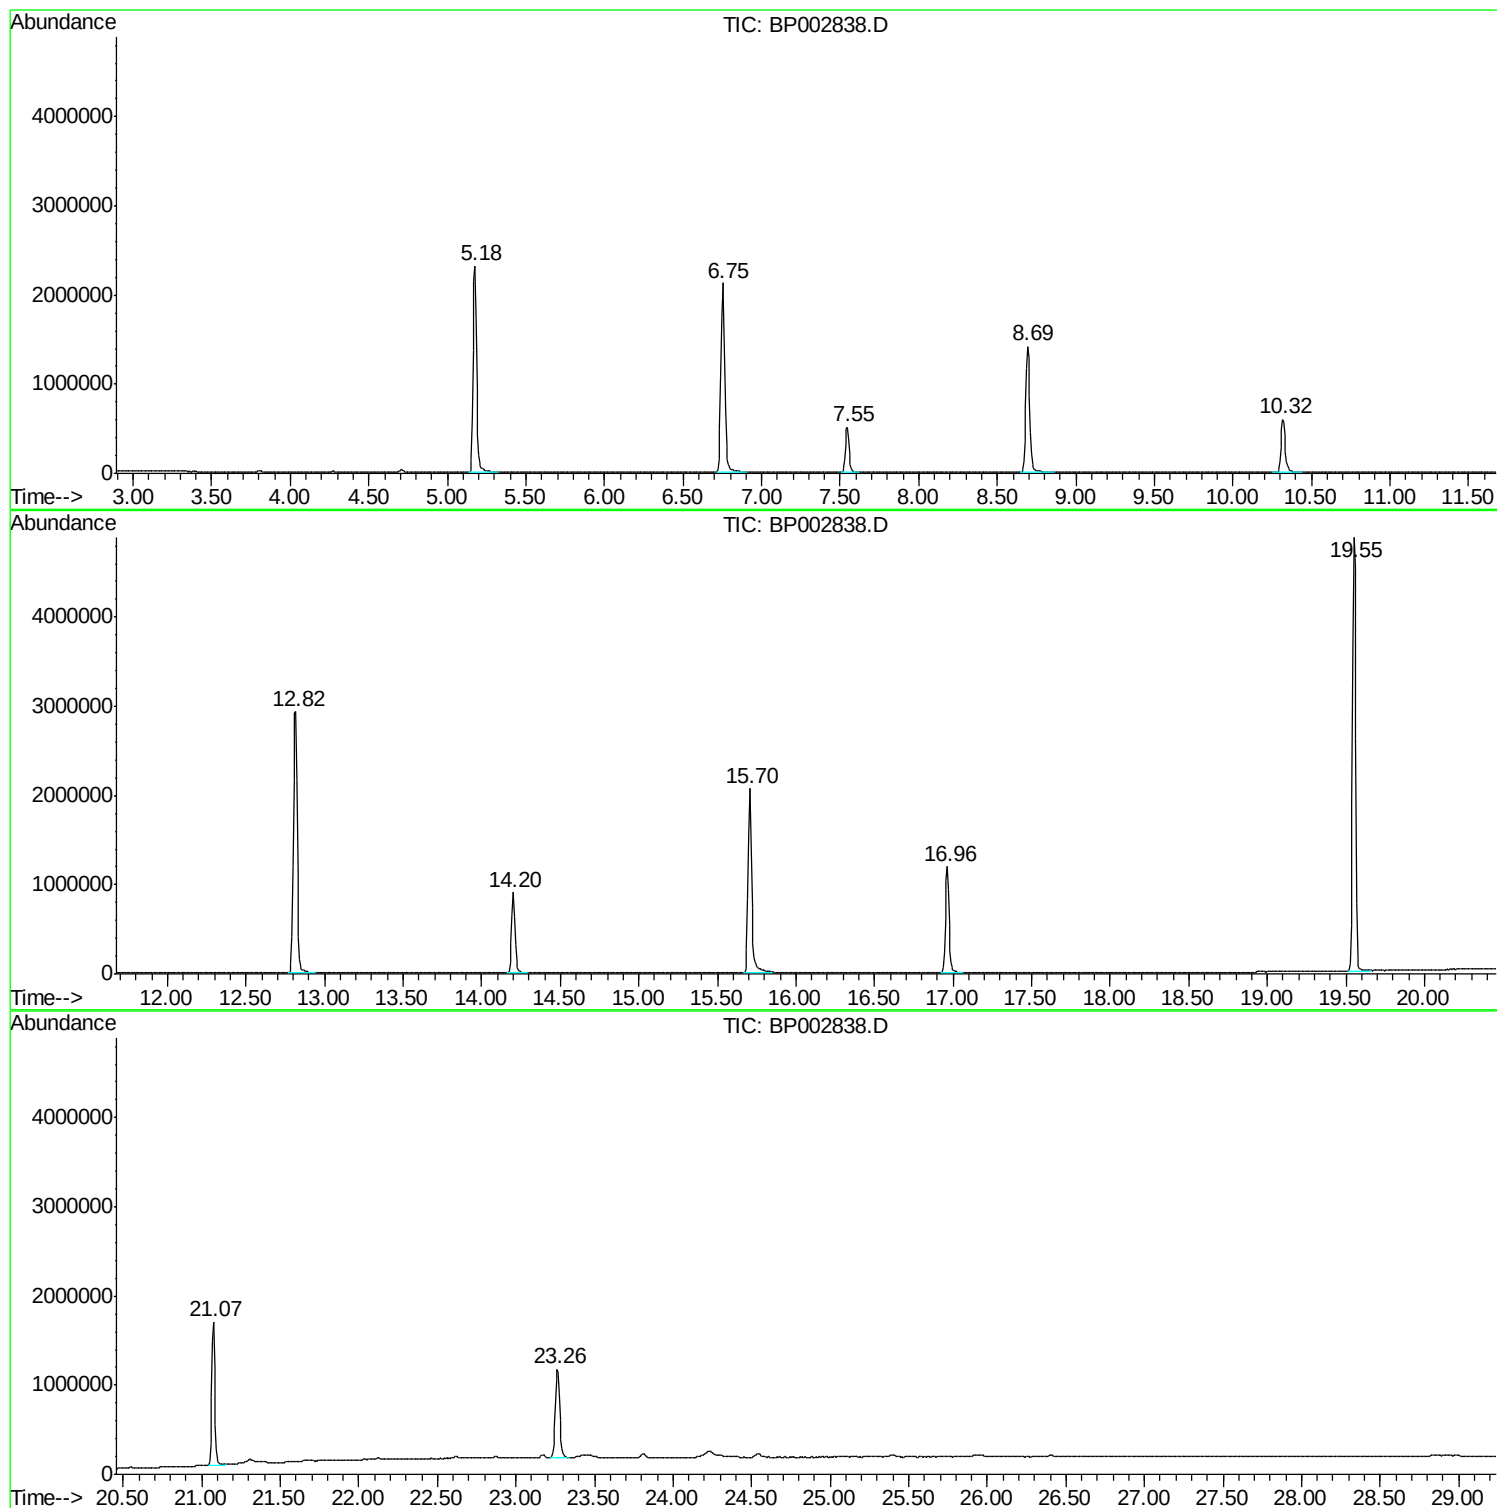

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP072320\
Data File : BP002838.D
Acq On : 23 Jul 2020 13:48
Operator : CG/JU
Sample : PB130378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130378BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP072320\
Data File : BP002838.D
Acq On : 23 Jul 2020 13:48
Operator : CG/JU
Sample : PB130378BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130378BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc