


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP072320\
 Data File : BP002836.D
 Acq On : 23 Jul 2020 12:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:54:03 2020

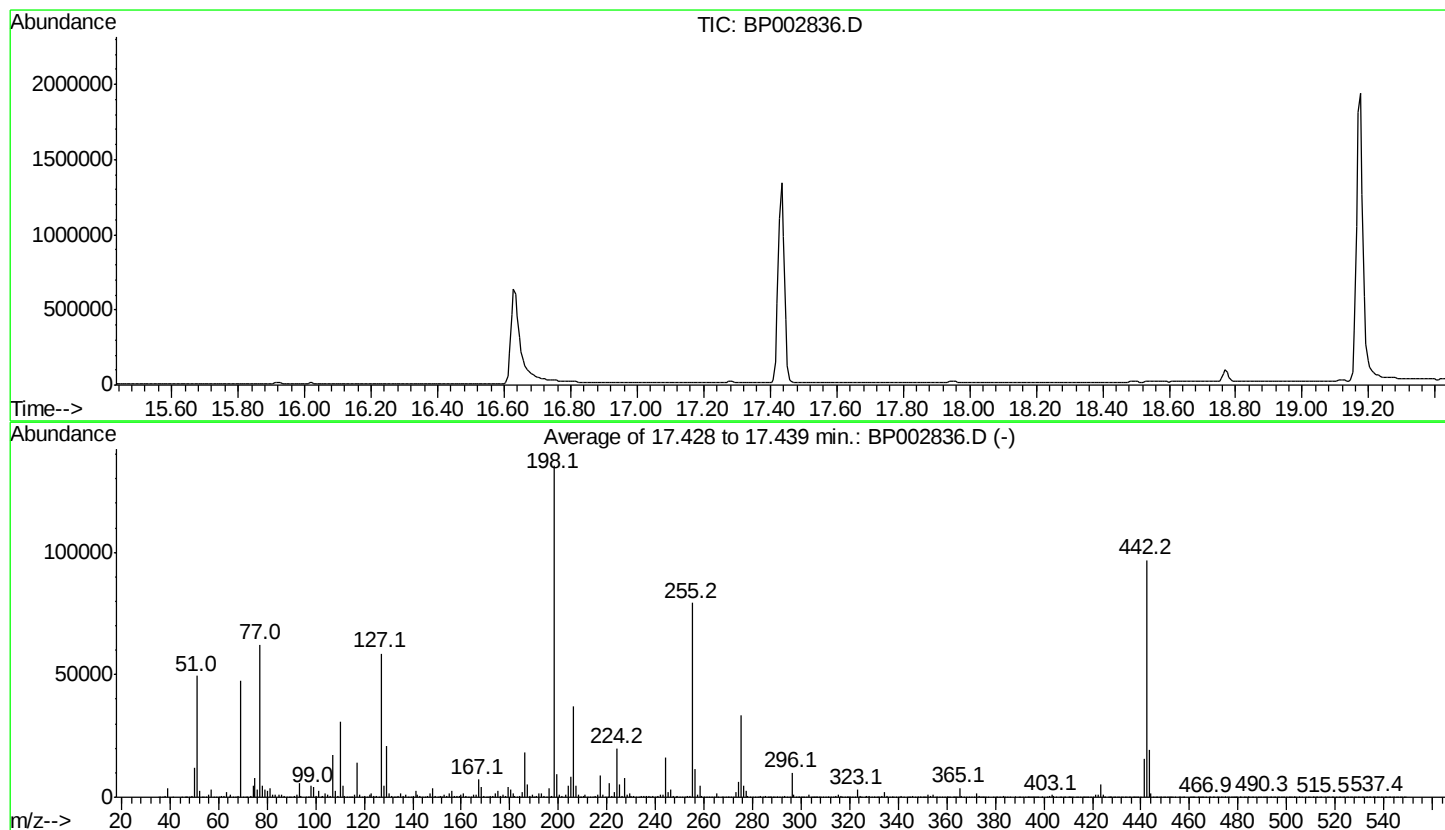

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	49605	PASS
68	69	0.00	2	1.4	650	PASS
69	198	0.00	100	35.3	47722	PASS
70	69	0.00	2	0.4	213	PASS
127	198	10	80	43.3	58671	PASS
197	198	0.00	2	0.3	363	PASS
198	198	100	100	100.0	135379	PASS
199	198	5	9	6.8	9192	PASS
275	198	10	60	24.8	33611	PASS
365	198	1	100	2.8	3840	PASS
441	198	0.01	100	11.6	15705	PASS
442	198	50	100	71.5	96785	PASS
443	442	15	24	19.7	19107	PASS