

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006390.D
 Acq On : 28 Jul 2021 15:14
 Operator : CG/JU
 Sample : M3107-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGD00

Quant Time: Jul 28 15:48:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 28 15:07:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	351688	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.569	136	1498542	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.410	164	848081	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.163	188	1613294	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	1378950	20.000	ng/ul	0.00
88) Perylene-d12	23.610	264	1184568	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	21344	2.265	ng/uL	0.00
4) Pyridine-d5	3.705	84	239678	8.569	ng/ul	0.00
7) Phenol-d5	6.958	99	389474	11.791	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	267285	13.005	ng/ul	0.00
11) 2-Chlorophenol-d4	7.317	132	308428	12.569	ng/ul	-0.01
15) 4-Methylphenol-d8	8.487	113	316134	12.171	ng/ul	-0.01
21) Nitrobenzene-d5	8.940	128	149928	13.437	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.658	143	146159	13.719	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	255375	12.232	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.710	131	404705	11.775	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	886300	14.684	ng/ul	-0.01
49) Acenaphthylene-d8	14.104	160	1024746	13.819	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	119837	9.999	ng/ul	0.00
60) Fluorene-d10	15.404	176	714194	14.075	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.522	200	85529	9.510	ng/ul	-0.01
73) Anthracene-d10	17.263	188	1078910	14.815	ng/ul	0.00
81) Pyrene-d10	19.504	212	1161143	16.371	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.457	264	768417	12.765	ng/ul	0.00
Target Compounds						
80) Fluoranthene	19.181	202	110438	1.264	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006390.D
Acq On : 28 Jul 2021 15:14
Operator : CG/JU
Sample : M3107-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGD00

Quant Time: Jul 28 15:48:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 28 15:07:59 2021
Response via : Initial Calibration

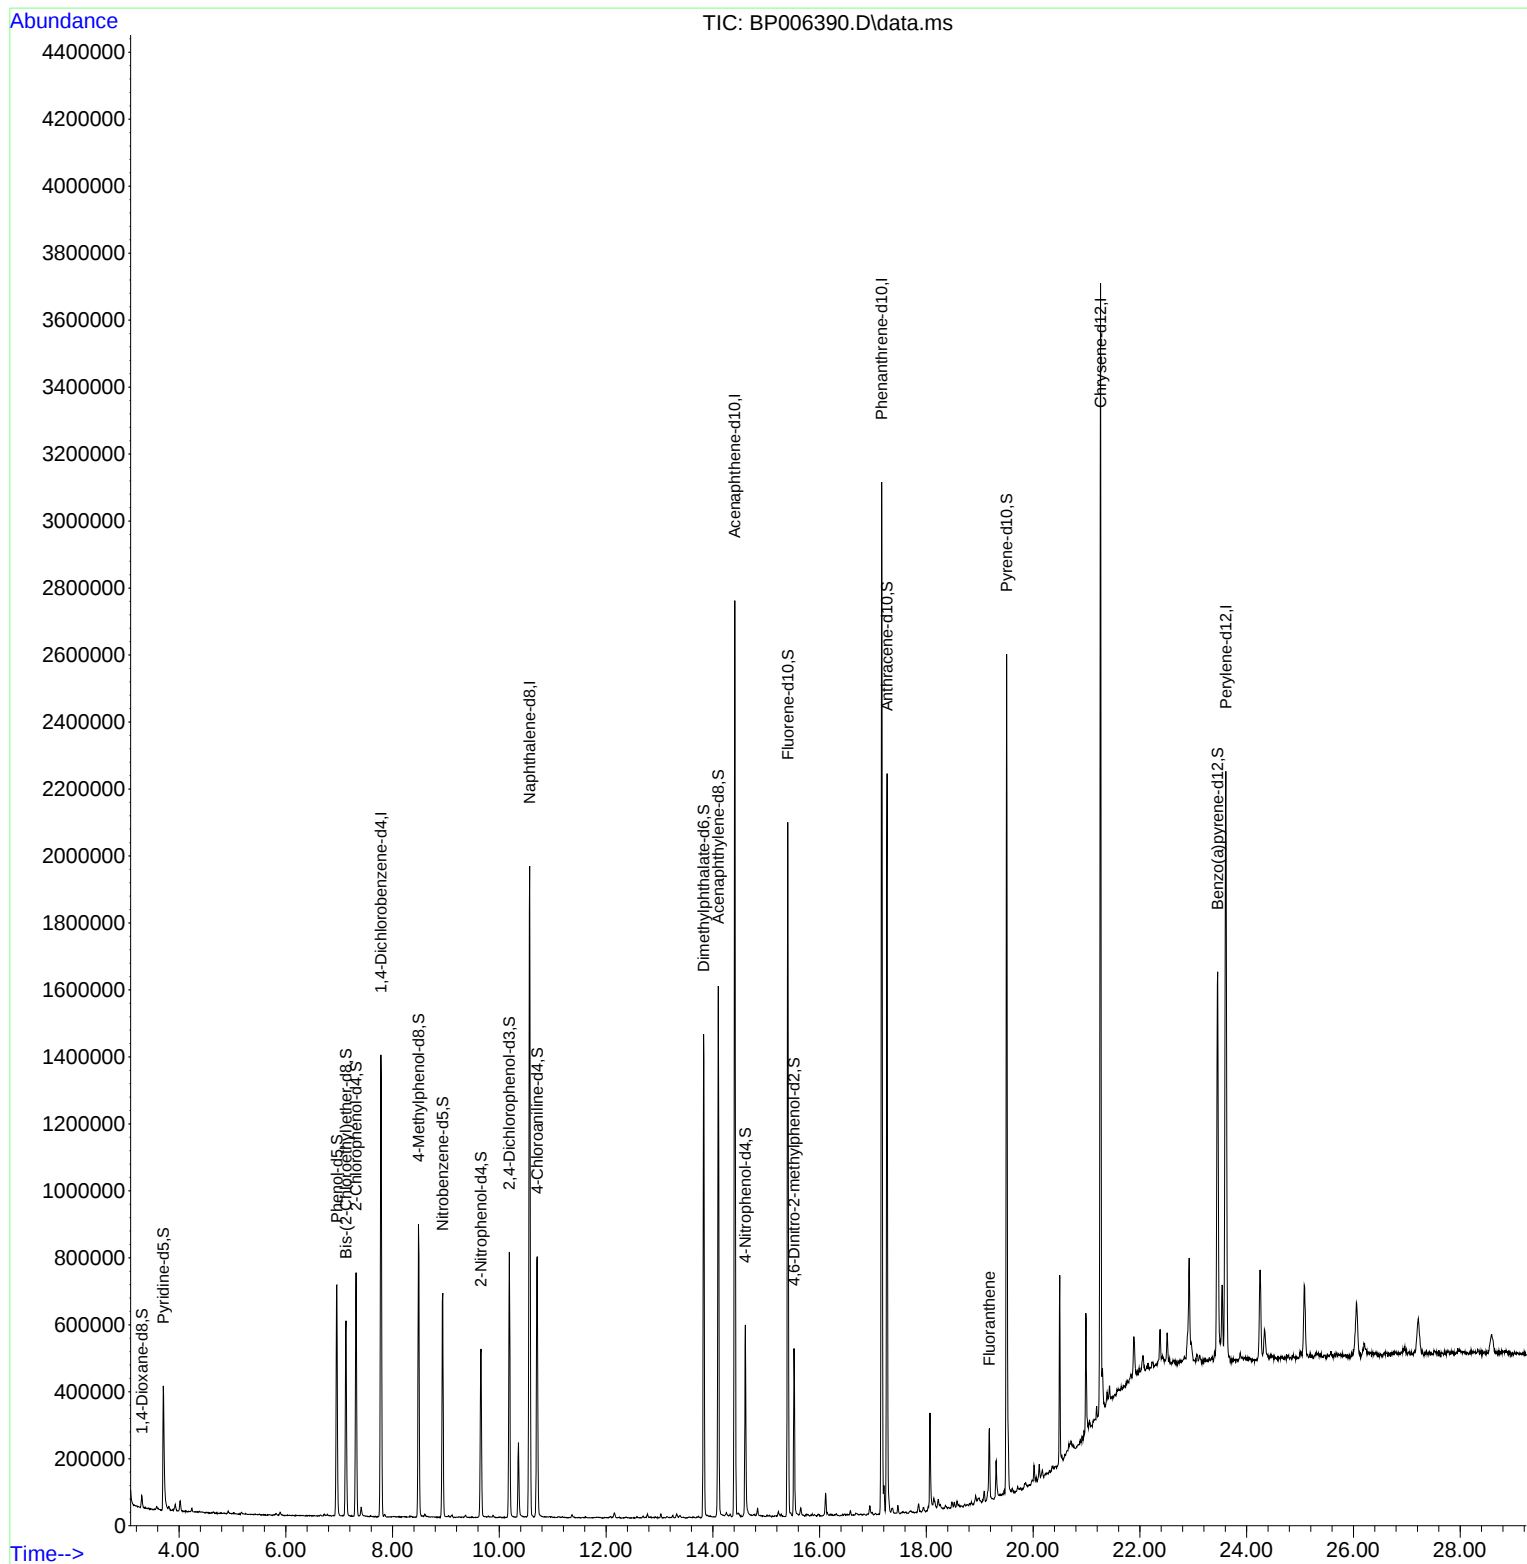

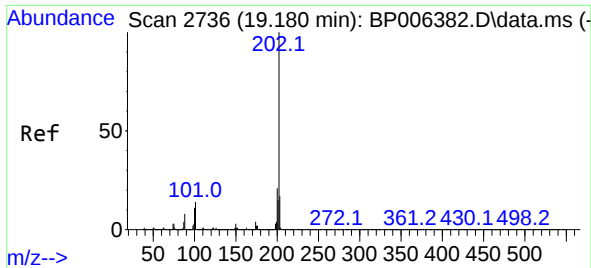

#80
Fluoranthene
Concen: 1.264 ng/ul
RT: 19.181 min Scan# 2736
Delta R.T. -0.006 min
Lab File: BP006390.D
Acq: 28 Jul 2021 15:14

Instrument :
BNA_P
ClientSampleId :
BGD00

Tgt Ion:202 Resp: 110438
Ion Ratio Lower Upper
202 100
101 13.4 11.0 16.6
100 11.0 8.8 13.2

