

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006396.D
 Acq On : 28 Jul 2021 18:39
 Operator : CG/JU
 Sample : M3107-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEM6

Quant Time: Jul 29 01:06:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	334928	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.563	136	1429163	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.410	164	820405	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.163	188	1558446	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	1380539	20.000	ng/ul	0.00
88) Perylene-d12	23.604	264	1222874	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	17114	1.907	ng/uL	0.00
4) Pyridine-d5	3.711	84	118501	4.449	ng/ul	0.00
7) Phenol-d5	6.952	99	286026	9.093	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.128	67	196719	10.051	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	225564	9.652	ng/ul	-0.01
15) 4-Methylphenol-d8	8.487	113	229519	9.278	ng/ul	-0.01
21) Nitrobenzene-d5	8.934	128	106349	9.994	ng/ul	-0.02
24) 2-Nitrophenol-d4	9.657	143	97011	9.548	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	182954	9.189	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.704	131	280842	8.568	ng/ul	-0.01
46) Dimethylphthalate-d6	13.828	166	602046	10.311	ng/ul	-0.01
49) Acenaphthylene-d8	14.098	160	716150	9.983	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.610	143	60578	5.225	ng/ul	0.00
60) Fluorene-d10	15.404	176	508623	10.362	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.522	200	34605	3.983	ng/ul	-0.01
73) Anthracene-d10	17.257	188	741679	10.543	ng/ul	-0.01
81) Pyrene-d10	19.504	212	837383	11.793	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.451	264	609852	9.814	ng/ul	-0.01
Target Compounds						
					Qvalue	
80) Fluoranthene	19.174	202	113204	1.294	ng/ul	100
82) Pyrene	19.527	202	99896	1.100	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006396.D
Acq On : 28 Jul 2021 18:39
Operator : CG/JU
Sample : M3107-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEM6

Quant Time: Jul 29 01:06:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 04:29:12 2021
Response via : Initial Calibration




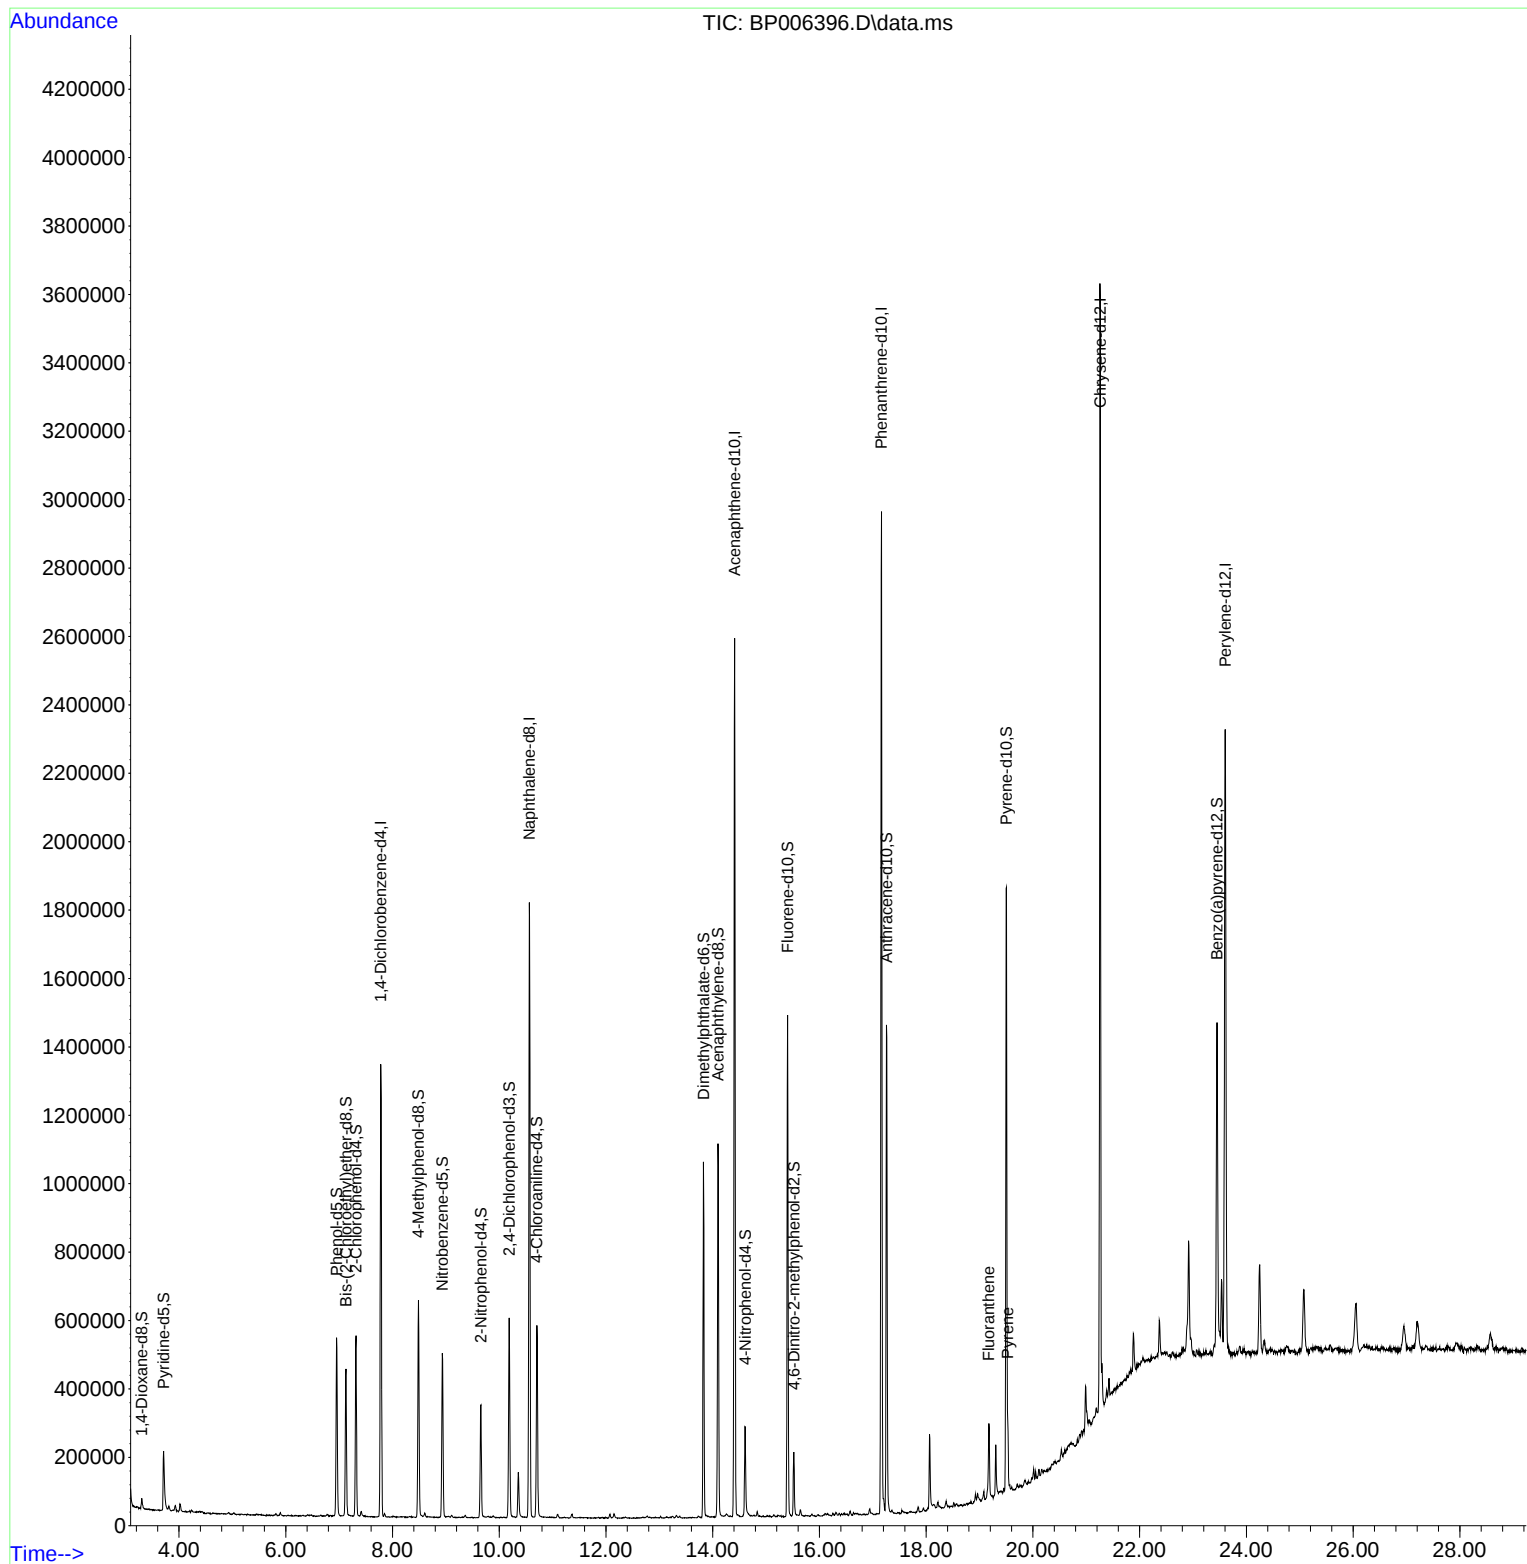


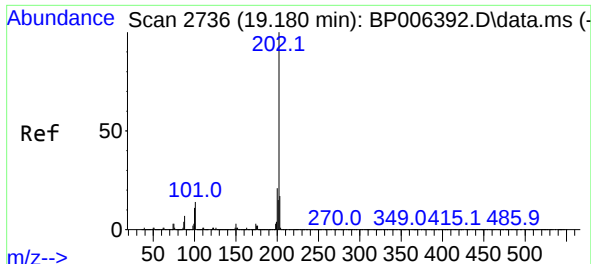

#80
Fluoranthene
Concen: 1.294 ng/ul
RT: 19.174 min Scan# 2735
Delta R.T. -0.012 min
Lab File: BP006396.D
Acq: 28 Jul 2021 18:39

Instrument :
BNA_P
ClientSampled :
BGEM6

Tgt Ion:202	Resp:	113204
Ion Ratio	Lower	Upper
202	100	
101	13.9	11.0 16.6
100	10.9	8.8 13.2

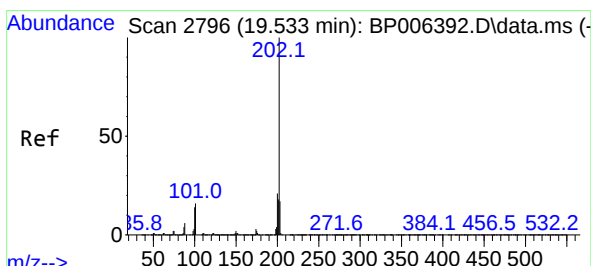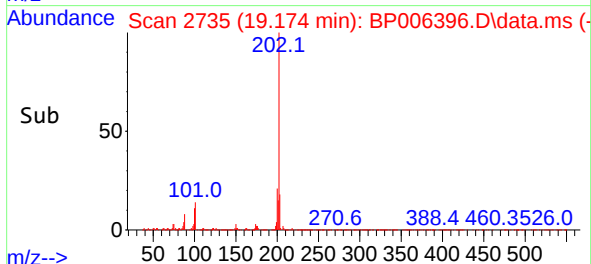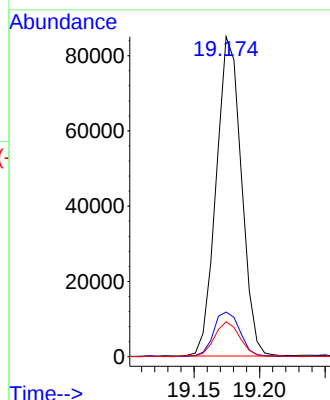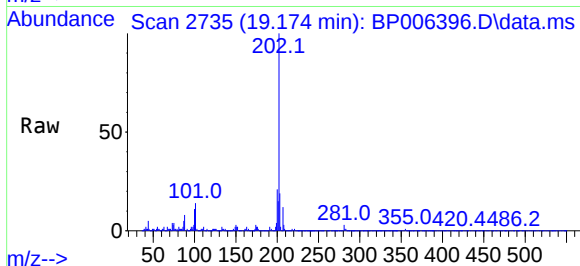

#82
Pyrene
Concen: 1.100 ng/ul
RT: 19.527 min Scan# 2795
Delta R.T. -0.012 min
Lab File: BP006396.D
Acq: 28 Jul 2021 18:39

Tgt Ion:202	Resp:	99896
Ion Ratio	Lower	Upper
202	100	
101	17.1	13.0 19.4
100	14.6	11.0 16.4

