

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006406.D
 Acq On : 29 Jul 2021 00:20
 Operator : CG/JU
 Sample : M3122-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEM7

Quant Time: Jul 29 01:09:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	354011	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.563	136	1569676	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.410	164	923018	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.157	188	1798798	20.000	ng/ul	-0.01
79) Chrysene-d12	21.251	240	1627648	20.000	ng/ul	-0.02
88) Perylene-d12	23.598	264	1441299	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	50937	5.371	ng/uL	0.00
4) Pyridine-d5	3.705	84	288709	10.254	ng/ul	0.00
7) Phenol-d5	6.952	99	250301	7.528	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.122	67	769712	37.207	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.316	132	695188	28.144	ng/ul	-0.01
15) 4-Methylphenol-d8	8.487	113	473188	18.098	ng/ul	-0.01
21) Nitrobenzene-d5	8.934	128	455835	39.001	ng/ul	-0.02
24) 2-Nitrophenol-d4	9.652	143	441584	39.569	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.187	165	699910	32.005	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.704	131	1126215	31.281	ng/ul	-0.01
46) Dimethylphthalate-d6	13.828	166	2650380	40.345	ng/ul	-0.01
49) Acenaphthylene-d8	14.098	160	3209848	39.770	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.604	143	87266	6.690	ng/ul	-0.01
60) Fluorene-d10	15.404	176	2282363	41.328	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.522	200	351932	35.095	ng/ul	-0.01
73) Anthracene-d10	17.263	188	3774495	46.484	ng/ul	0.00
81) Pyrene-d10	19.498	212	4116126	49.167	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.451	264	3402661	46.457	ng/ul	-0.01
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.934	77	22480	1.239	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006406.D
Acq On : 29 Jul 2021 00:20
Operator : CG/JU
Sample : M3122-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEM7

Quant Time: Jul 29 01:09:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 04:29:12 2021
Response via : Initial Calibration

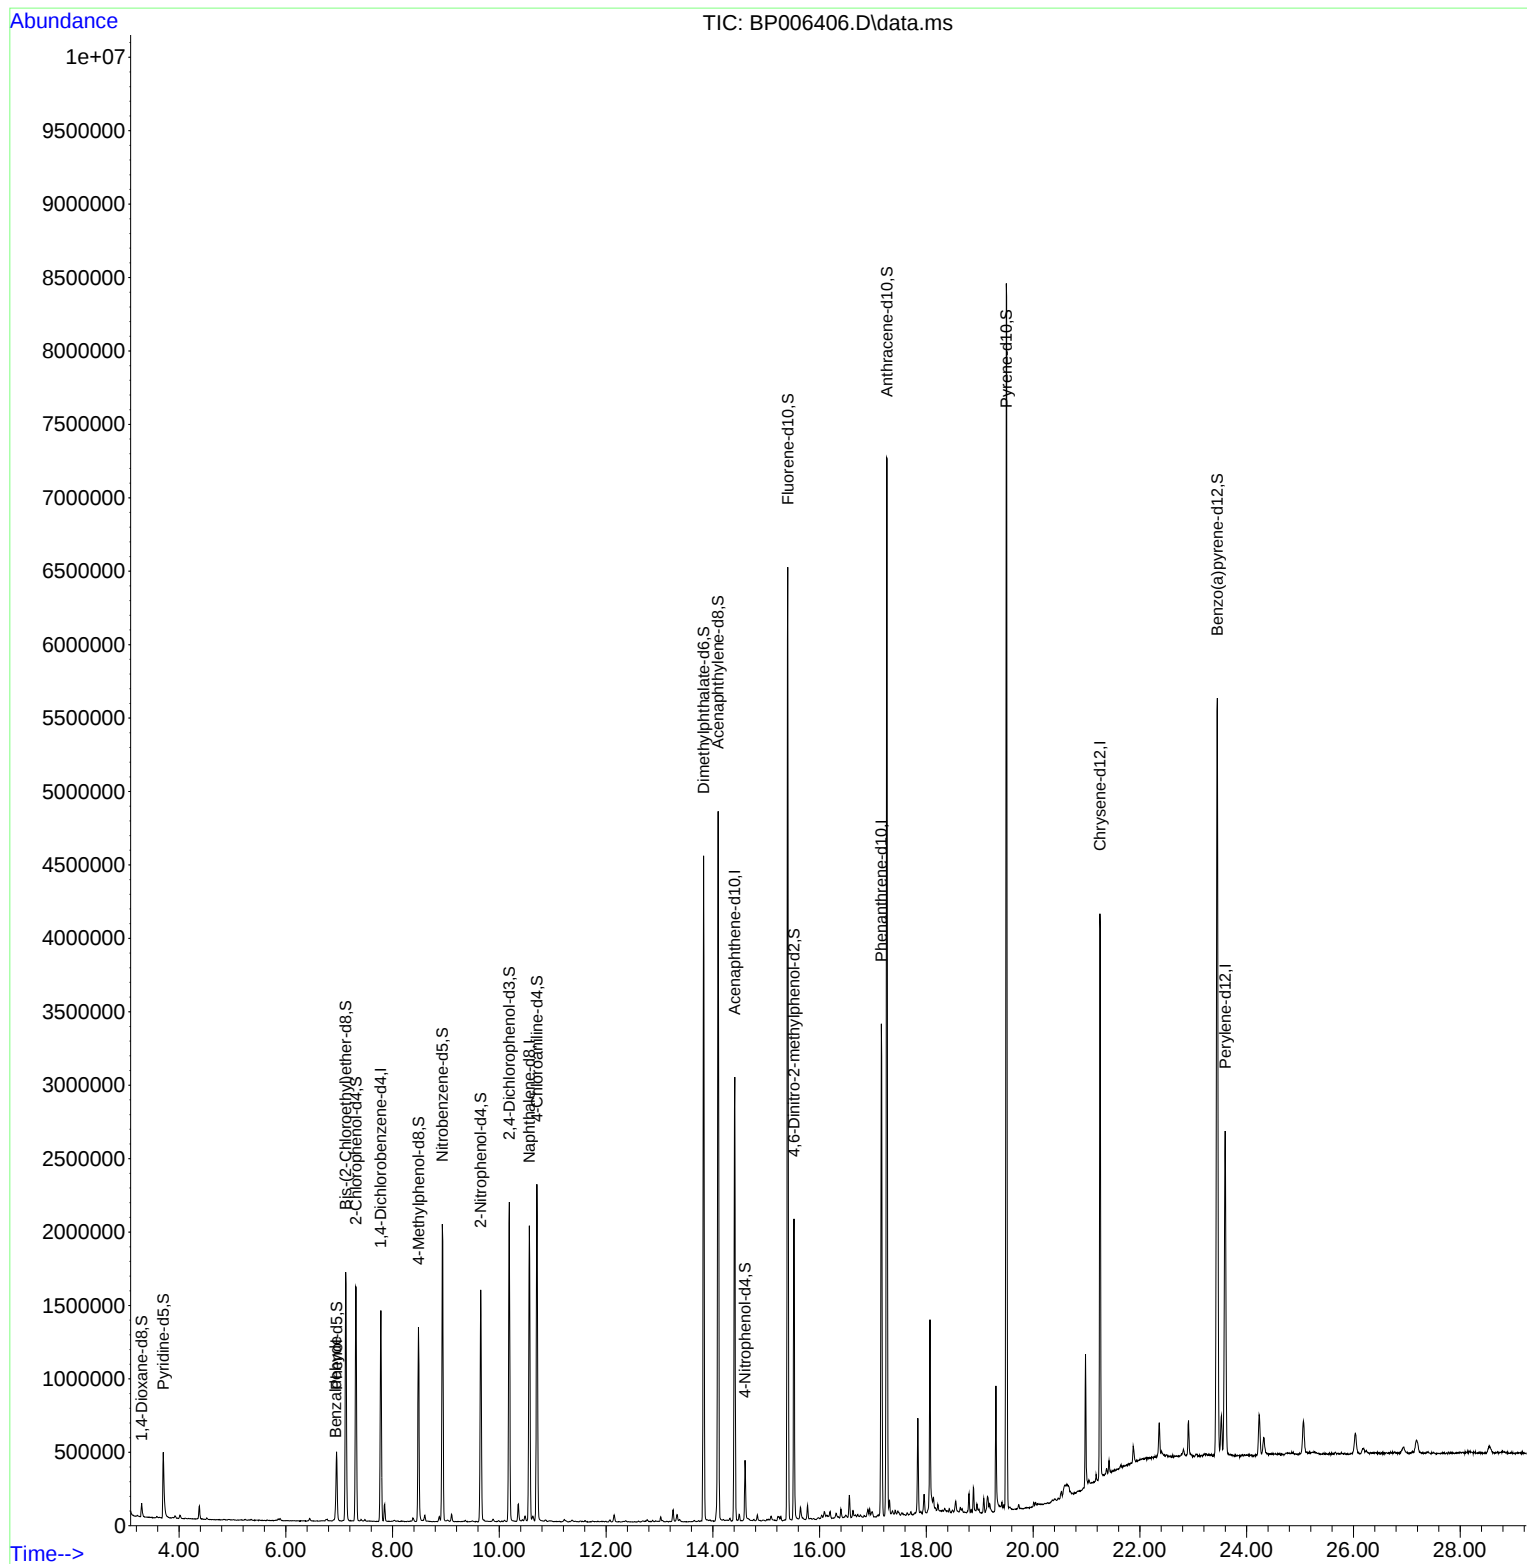

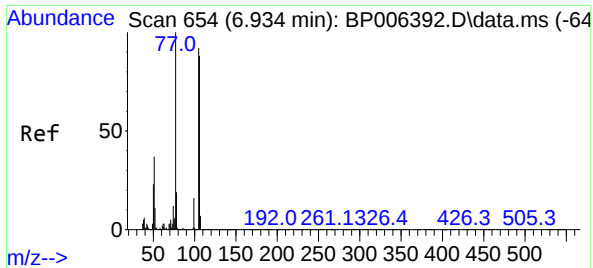

#6
Benzaldehyde
Concen: 1.239 ng/ul
RT: 6.934 min Scan# 654
Delta R.T. -0.012 min
Lab File: BP006406.D
Acq: 29 Jul 2021 00:20

Instrument :
BNA_P
ClientSampleId :
BGEM7

Tgt Ion: 77 Resp: 22480

Ion	Ratio	Lower	Upper
77	100		
105	87.5	74.5	111.7
106	79.8	71.0	106.4

