

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006407.D
 Acq On : 29 Jul 2021 00:54
 Operator : CG/JU
 Sample : M3124-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0061

Quant Time: Jul 29 01:56:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 29 01:09:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	367014	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.563	136	1611667	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.404	164	950245	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.157	188	1830920	20.000	ng/ul	-0.01
79) Chrysene-d12	21.257	240	1721181	20.000	ng/ul	-0.01
88) Perylene-d12	23.598	264	1576762	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	45414	4.619	ng/uL	0.00
4) Pyridine-d5	3.705	84	304370	10.428	ng/ul	0.00
7) Phenol-d5	6.952	99	247050	7.167	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.122	67	762632	35.558	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.316	132	691140	26.989	ng/ul	-0.01
15) 4-Methylphenol-d8	8.487	113	486143	17.934	ng/ul	-0.01
21) Nitrobenzene-d5	8.934	128	455902	37.990	ng/ul	-0.02
24) 2-Nitrophenol-d4	9.651	143	451096	39.368	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.187	165	721720	32.143	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.704	131	1104225	29.871	ng/ul	-0.01
46) Dimethylphthalate-d6	13.828	166	2767704	40.924	ng/ul	-0.01
49) Acenaphthylene-d8	14.098	160	3283327	39.515	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.604	143	90647	6.750	ng/ul	-0.01
60) Fluorene-d10	15.404	176	2259773	39.746	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.522	200	358974	35.169	ng/ul	-0.01
73) Anthracene-d10	17.257	188	3633238	43.959	ng/ul	-0.01
81) Pyrene-d10	19.498	212	4030168	45.524	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.445	264	3541367	44.197	ng/ul	-0.02
Target Compounds						
16) Acetophenone	8.604	105	43286	1.038	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006407.D
Acq On : 29 Jul 2021 00:54
Operator : CG/JU
Sample : M3124-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0061

Quant Time: Jul 29 01:56:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 29 01:09:55 2021
Response via : Initial Calibration

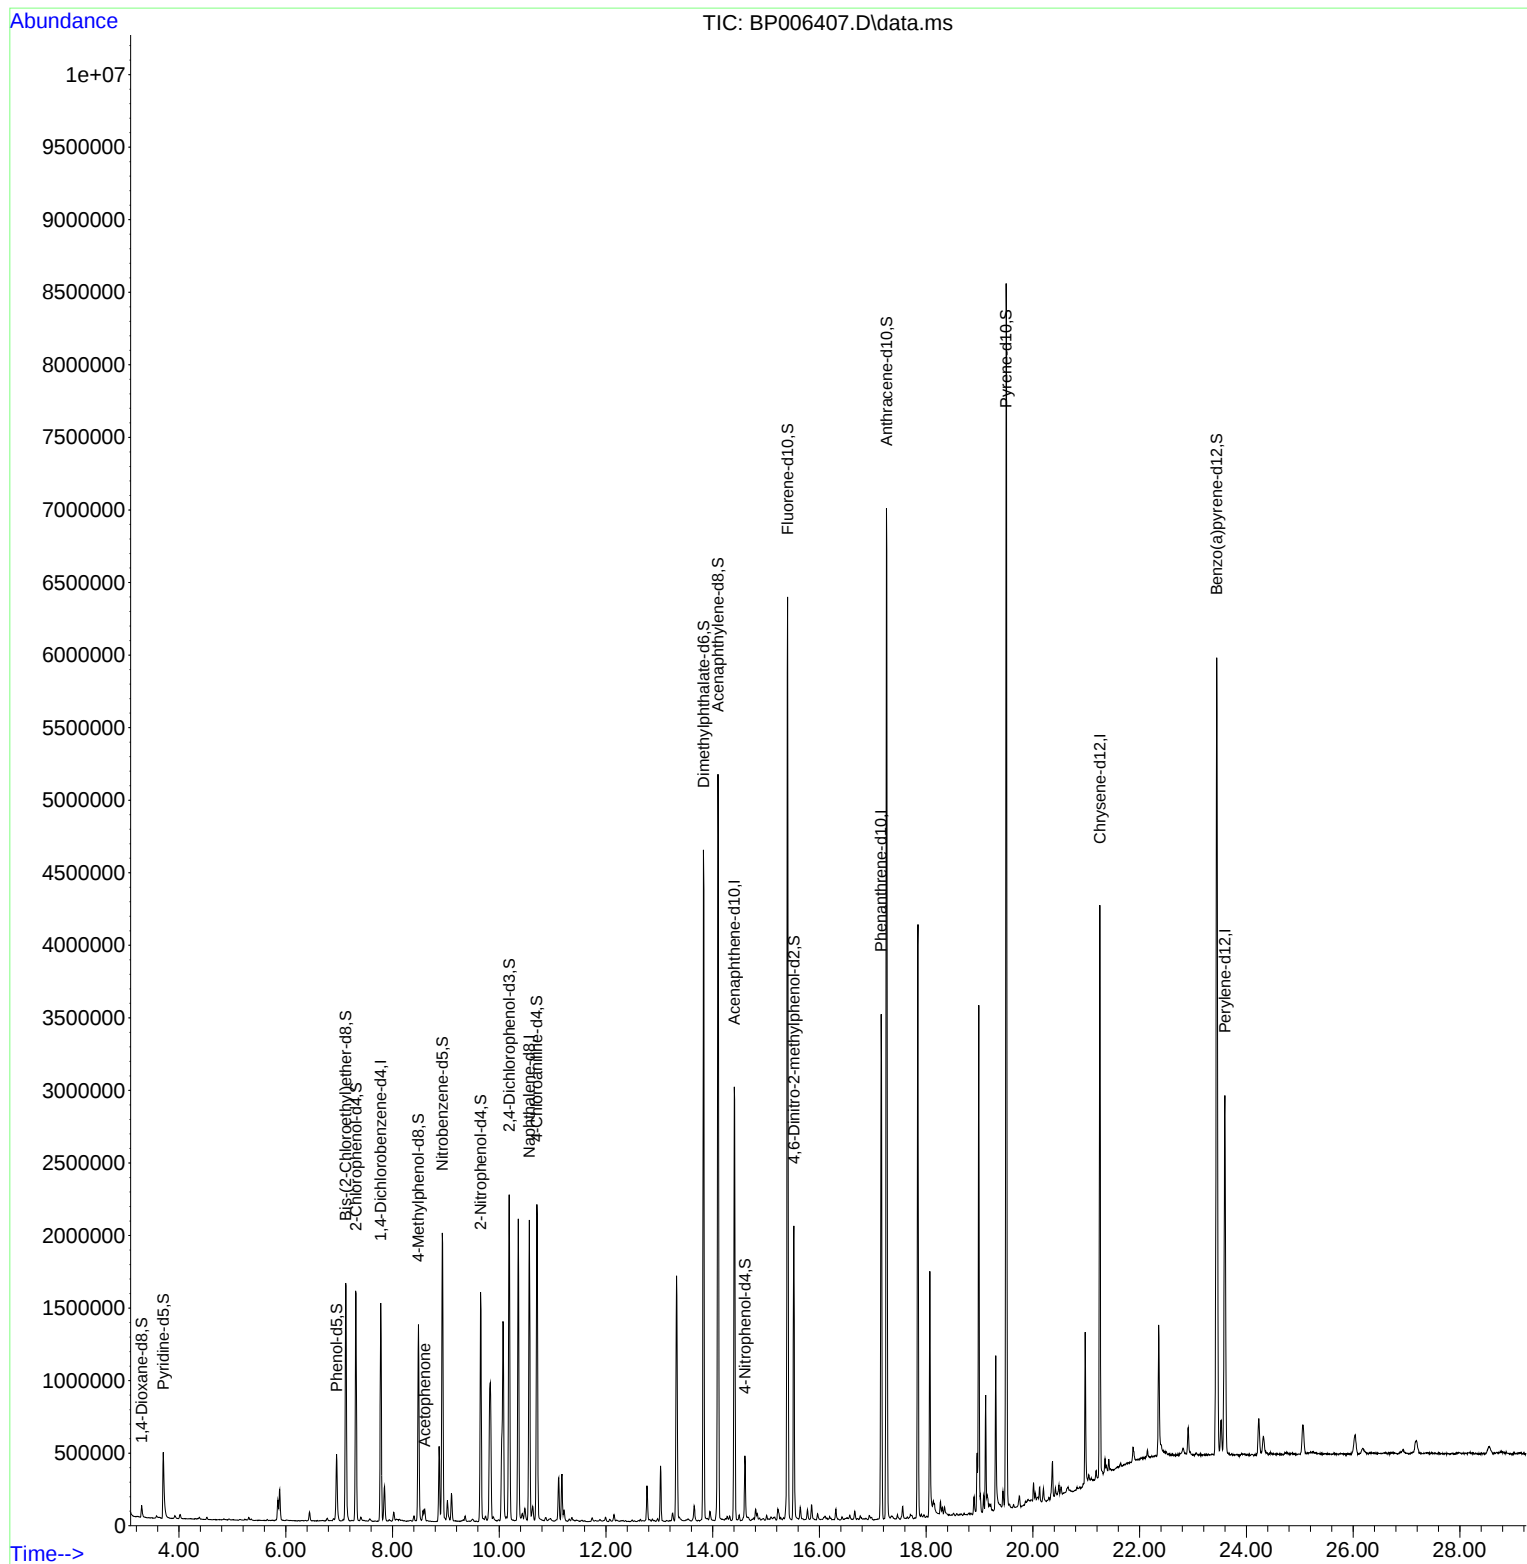

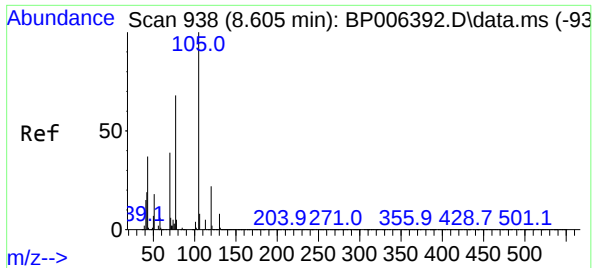

#16
 Acetophenone
 Concen: 1.038 ng/ul
 RT: 8.604 min Scan# 938
 Delta R.T. -0.012 min
 Lab File: BP006407.D
 Acq: 29 Jul 2021 00:54

Instrument :
 BNA_P
 ClientSampleId :
 C0061

Tgt Ion:	105	Resp:	43286
Ion	Ratio	Lower	Upper
105	100		
77	84.1	65.0	97.4
51	27.3	17.9	26.9#

