

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006394.D
 Acq On : 28 Jul 2021 17:31
 Operator : CG/JU
 Sample : PB137941BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK941

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006394.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	44	rBV	122496	177704	1.74%	0.157%
2	3.699	100	104	130	rBV	1498576	2632601	25.73%	2.331%
3	4.016	153	158	166	rVB	67393	109508	1.07%	0.097%
4	6.958	650	658	666	rBV	2035475	3230475	31.57%	2.860%
5	7.128	680	687	701	rVB	1691100	2600375	25.41%	2.302%
6	7.316	712	719	732	rVB	2138467	3308191	32.33%	2.929%
7	7.781	790	798	807	rBV	1519221	2372262	23.18%	2.100%
8	8.487	911	918	931	rBV	2599604	4078707	39.86%	3.611%
9	8.940	986	995	1004	rBV	1948306	3174609	31.02%	2.811%
10	9.651	1107	1116	1134	rBV	1593406	2604021	25.45%	2.306%
11	10.187	1198	1207	1221	rBV	2391492	3950904	38.61%	3.498%
12	10.563	1263	1271	1281	rVB	2123763	3529900	34.49%	3.125%
13	10.704	1287	1295	1308	rBV	2448402	4198328	41.03%	3.717%
14	12.151	1533	1541	1551	rBV	44933	82580	0.81%	0.073%
15	12.363	1572	1577	1584	rVB10	7299	14429	0.14%	0.013%
16	13.140	1704	1709	1714	rBV8	6063	10945	0.11%	0.010%
17	13.375	1746	1749	1758	rVB3	9773	18403	0.18%	0.016%
18	13.828	1820	1826	1834	rBV	4067085	5889601	57.55%	5.215%
19	14.104	1865	1873	1887	rBV	4736661	6980081	68.21%	6.180%
20	14.410	1917	1925	1936	rBV	3210701	4615612	45.10%	4.087%
21	14.610	1952	1959	1982	rBV	2104005	3036725	29.67%	2.689%
22	14.775	1982	1987	1991	rVB7	5937	13574	0.13%	0.012%
23	15.404	2087	2094	2107	rBV	6125952	8436608	82.44%	7.470%
24	15.522	2107	2114	2129	rVV	1805894	2418411	23.63%	2.141%
25	15.645	2130	2135	2141	rVB	70791	109800	1.07%	0.097%
26	16.081	2204	2209	2217	rBV	10563	22473	0.22%	0.020%
27	16.839	2333	2338	2343	rVB8	8889	14397	0.14%	0.013%
28	16.945	2350	2356	2363	rBV2	22546	40163	0.39%	0.036%
29	17.163	2386	2393	2403	rBV	3732234	5252262	51.32%	4.650%
30	17.263	2403	2410	2423	rBV2	6420913	9252960	90.42%	8.192%
31	17.539	2451	2457	2463	rBV3	13174	24196	0.24%	0.021%
32	17.839	2505	2508	2514	rVB8	8880	13028	0.13%	0.012%
33	18.063	2541	2546	2557	rBV2	58696	114847	1.12%	0.102%
34	18.580	2630	2634	2636	rBV5	10181	12635	0.12%	0.011%
35	19.080	2714	2719	2724	rBV2	85259	116186	1.14%	0.103%
36	19.145	2726	2730	2737	rBV	82832	117906	1.15%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006394.D
Acq On : 28 Jul 2021 17:31
Operator : CG/JU
Sample : PB137941BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Title : SVOA CALIBRATION

37	19.304	2753	2757	2761	rBV5	43378	57715	0.56%	0.051%
38	19.504	2785	2791	2799	rBV	8036670	10233549	100.00%	9.061%
39	21.257	3084	3089	3097	rBV	4279469	5471989	53.47%	4.845%
40	23.451	3455	3462	3470	rBV2	4842905	9209250	89.99%	8.154%
41	23.533	3473	3476	3480	rVV	235214	348456	3.41%	0.309%
42	23.604	3481	3488	3497	rVB2	2641321	5049738	49.34%	4.471%




Sum of corrected areas: 112946104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006394.D
Acq On : 28 Jul 2021 17:31
Operator : CG/JU
Sample : PB137941BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

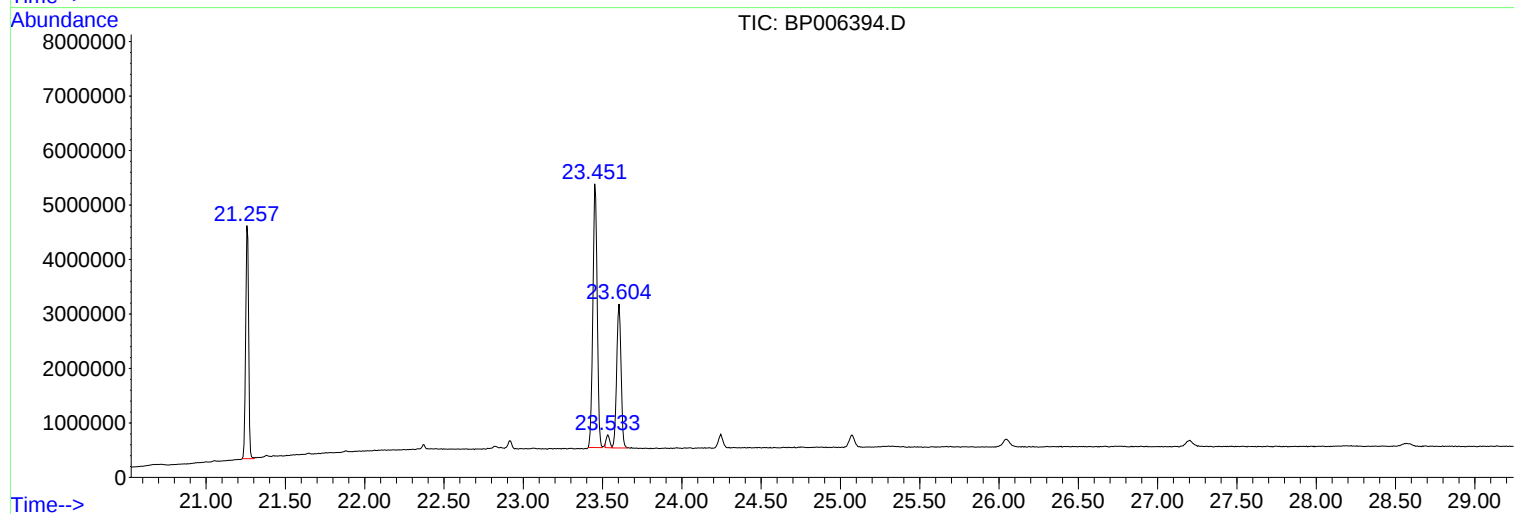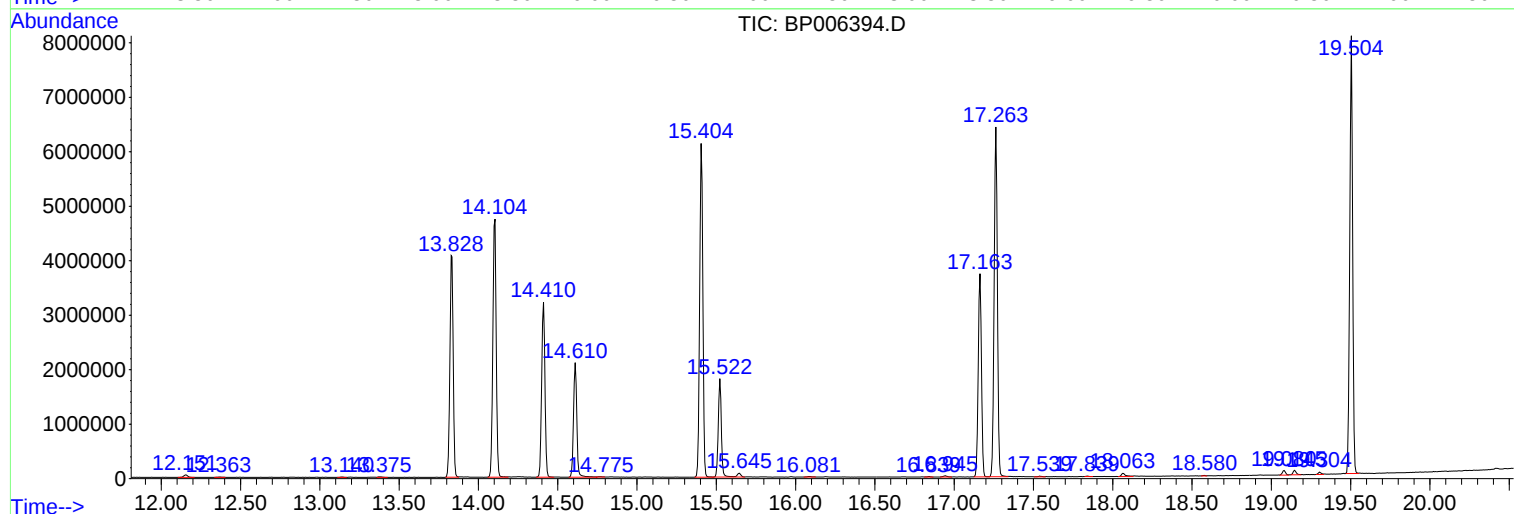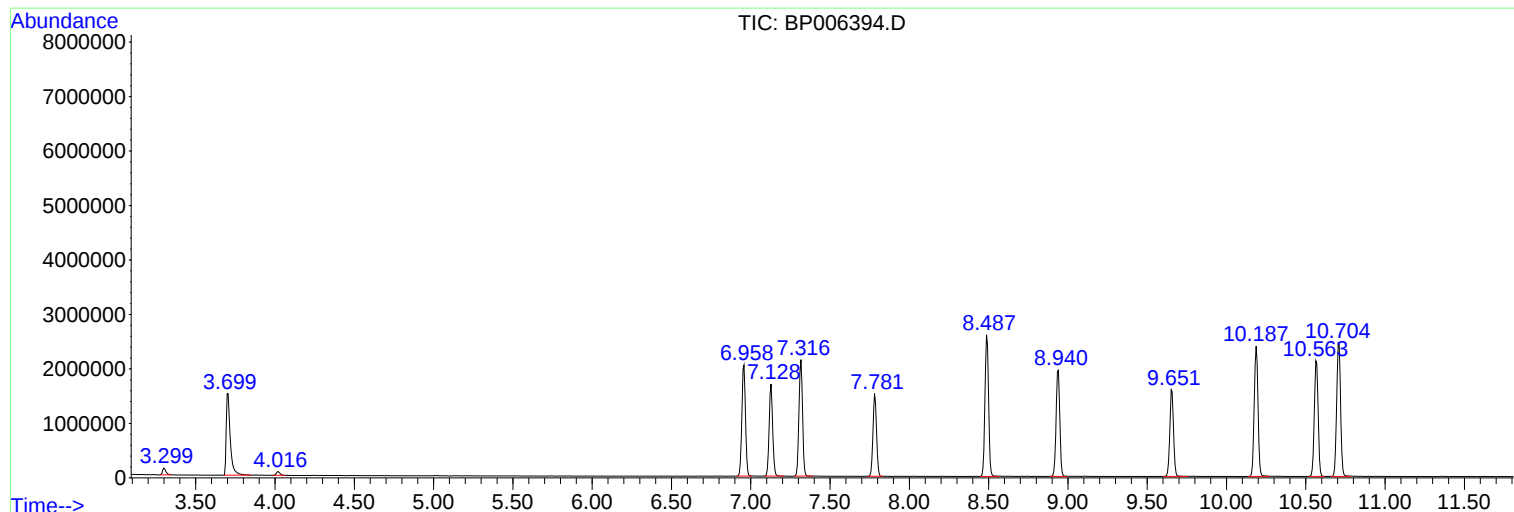

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006394.D
Acq On : 28 Jul 2021 17:31
Operator : CG/JU
Sample : PB137941BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006394.D
Acq On : 28 Jul 2021 17:31
Operator : CG/JU
Sample : PB137941BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK941

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
