

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006399.D
 Acq On : 28 Jul 2021 20:21
 Operator : CG/JU
 Sample : M3107-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGD10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006399.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	43	rVB	30645	43941	1.01%	0.096%
2	3.705	101	105	119	rBV	241723	449397	10.36%	0.977%
3	3.811	119	123	130	rVV2	32428	51186	1.18%	0.111%
4	3.876	132	134	138	rVV4	6573	8549	0.20%	0.019%
5	3.928	139	143	151	rVV	14902	28281	0.65%	0.062%
6	4.017	154	158	164	rBV2	19730	29492	0.68%	0.064%
7	4.234	192	195	204	rVB4	15069	25152	0.58%	0.055%
8	4.381	216	220	227	rVB	44171	66702	1.54%	0.145%
9	4.564	249	251	256	rVB5	6360	8128	0.19%	0.018%
10	4.640	260	264	269	rVV5	6690	9226	0.21%	0.020%
11	4.723	276	278	282	rVB5	4077	4792	0.11%	0.010%
12	4.923	310	312	317	rVB3	7285	10044	0.23%	0.022%
13	5.028	327	330	335	rVB7	6252	8513	0.20%	0.019%
14	5.817	461	464	469	rVB5	4925	7067	0.16%	0.015%
15	5.899	475	478	483	rVB4	9169	14616	0.34%	0.032%
16	6.411	561	565	568	rBV6	5160	7888	0.18%	0.017%
17	6.775	620	627	634	rBV5	13856	27883	0.64%	0.061%
18	6.952	650	657	670	rVV	575843	915696	21.12%	1.992%
19	7.081	673	679	680	rBV6	2990	5045	0.12%	0.011%
20	7.128	680	687	697	rVB	493009	794660	18.33%	1.728%
21	7.317	711	719	729	rVB	589701	936520	21.60%	2.037%
22	7.417	729	736	743	rBV3	20414	37309	0.86%	0.081%
23	7.781	789	798	806	rBV	1198465	1877099	43.29%	4.083%
24	7.846	806	809	815	rVB6	6212	11021	0.25%	0.024%
25	8.105	848	853	857	rBV7	3758	7537	0.17%	0.016%
26	8.487	910	918	931	rBV	517540	826134	19.05%	1.797%
27	8.605	931	938	944	rVB4	8745	18696	0.43%	0.041%
28	8.934	987	994	1007	rBV	579713	981233	22.63%	2.134%
29	9.105	1019	1023	1033	rVB2	51076	80952	1.87%	0.176%
30	9.363	1063	1067	1072	rVB5	5106	8988	0.21%	0.020%
31	9.652	1105	1116	1124	rBV	425917	699978	16.14%	1.522%
32	9.875	1152	1154	1161	rVB8	5781	9047	0.21%	0.020%
33	10.187	1198	1207	1221	rBV	641698	1053727	24.30%	2.292%
34	10.358	1230	1236	1246	rBV	146821	242310	5.59%	0.527%
35	10.563	1263	1271	1279	rBV	1630118	2761891	63.70%	6.007%
36	10.705	1286	1295	1312	rVB	622799	1063808	24.53%	2.314%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006399.D
 Acq On : 28 Jul 2021 20:21
 Operator : CG/JU
 Sample : M3107-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGD10

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	11.093	1360	1361	1368	rVB6	4850	5986	0.14%	0.013%
38	11.363	1402	1407	1412	rBV5	13411	22553	0.52%	0.049%
39	11.993	1511	1514	1519	rVB7	3947	7295	0.17%	0.016%
40	12.075	1524	1528	1533	rVV3	10774	16750	0.39%	0.036%
41	12.152	1533	1541	1552	rVB2	14578	33057	0.76%	0.072%
42	12.322	1567	1570	1575	rBV6	3479	5235	0.12%	0.011%
43	12.363	1575	1577	1584	rVB7	3767	5468	0.13%	0.012%
44	12.522	1600	1604	1609	rBV7	2790	4566	0.11%	0.010%
45	12.769	1642	1646	1650	rBV6	5401	6802	0.16%	0.015%
46	13.028	1686	1690	1694	rBV4	6412	9929	0.23%	0.022%
47	13.069	1694	1697	1703	rVB8	3099	5559	0.13%	0.012%
48	13.140	1703	1709	1713	rVB9	4519	8834	0.20%	0.019%
49	13.204	1713	1720	1722	rBV7	3180	5728	0.13%	0.012%
50	13.252	1724	1728	1729	rBV3	5089	4862	0.11%	0.011%
51	13.316	1734	1739	1745	rVB6	8369	15845	0.37%	0.034%
52	13.381	1745	1750	1758	rBV6	5485	10955	0.25%	0.024%
53	13.828	1819	1826	1837	rBV	1282181	1753035	40.43%	3.813%
54	13.946	1845	1846	1851	rVB5	3512	4543	0.10%	0.010%
55	14.099	1862	1872	1883	rBV	1297196	1888338	43.55%	4.107%
56	14.257	1894	1899	1907	rVB10	4521	9505	0.22%	0.021%
57	14.322	1907	1910	1913	rVB5	4442	6027	0.14%	0.013%
58	14.410	1917	1925	1932	rBV	2432267	3556054	82.01%	7.734%
59	14.604	1950	1958	1971	rBV	444675	686764	15.84%	1.494%
60	14.769	1982	1986	1991	rVV7	7548	11288	0.26%	0.025%
61	14.834	1991	1997	2003	rVB5	15265	24012	0.55%	0.052%
62	15.228	2060	2064	2065	rBV4	4213	5880	0.14%	0.013%
63	15.240	2065	2066	2069	rVV2	6189	4541	0.10%	0.010%
64	15.281	2069	2073	2077	rVB7	3990	6183	0.14%	0.013%
65	15.404	2087	2094	2102	rBV	1769311	2494522	57.53%	5.426%
66	15.522	2107	2114	2125	rBV	387893	542209	12.50%	1.179%
67	15.646	2131	2135	2142	rVB3	20947	30225	0.70%	0.066%
68	15.863	2166	2172	2174	rVB7	3947	6700	0.15%	0.015%
69	15.963	2184	2189	2195	rVB10	4656	9233	0.21%	0.020%
70	16.104	2204	2213	2217	rBV10	6545	18177	0.42%	0.040%
71	16.304	2243	2247	2251	rVB7	3903	6409	0.15%	0.014%
72	16.428	2264	2268	2271	rBV5	5593	7984	0.18%	0.017%
73	16.569	2289	2292	2297	rBV4	11091	15328	0.35%	0.033%
74	16.710	2312	2316	2324	rVB	30352	39123	0.90%	0.085%
75	16.945	2350	2356	2360	rBV3	16273	28363	0.65%	0.062%
76	17.045	2370	2373	2375	rBV4	3088	4718	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
 Data File : BP006399.D
 Acq On : 28 Jul 2021 20:21
 Operator : CG/JU
 Sample : M3107-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGD10

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

77	17.163	2386	2393	2398	rBV	2829512	4048658	93.37%	8.806%
78	17.204	2398	2400	2403	rVV	60066	66353	1.53%	0.144%
79	17.257	2403	2409	2419	rVV2	1739602	2436736	56.20%	5.300%
80	17.357	2422	2426	2434	rVB2	13608	28115	0.65%	0.061%
81	17.516	2451	2453	2455	rBV3	4161	5141	0.12%	0.011%
82	17.557	2455	2460	2465	rVB7	8539	19673	0.45%	0.043%
83	17.851	2505	2510	2515	rVB4	20545	31033	0.72%	0.067%
84	17.945	2521	2526	2530	rBV7	19030	30705	0.71%	0.067%
85	18.028	2538	2540	2542	rBV3	4020	4578	0.11%	0.010%
86	18.063	2542	2546	2554	rBV	256082	356716	8.23%	0.776%
87	18.216	2569	2572	2576	rVB3	7123	9525	0.22%	0.021%
88	18.522	2620	2624	2626	rBV4	12321	13912	0.32%	0.030%
89	18.551	2626	2629	2633	rBV5	9973	16720	0.39%	0.036%
90	18.922	2688	2692	2697	rBV4	40626	56017	1.29%	0.122%
91	19.081	2715	2719	2723	rVB5	25510	32131	0.74%	0.070%
92	19.139	2726	2729	2730	rVV3	30896	28683	0.66%	0.062%
93	19.175	2731	2735	2745	rVB	138131	229712	5.30%	0.500%
94	19.304	2753	2757	2764	rBV	150478	195407	4.51%	0.425%
95	19.498	2785	2790	2799	rBV	2266078	3013824	69.51%	6.555%
96	20.986	3039	3043	3048	rBV4	127558	190217	4.39%	0.414%
97	21.257	3084	3089	3094	rBV	3661903	4336024	100.00%	9.431%
98	23.445	3455	3461	3468	rBV2	1210421	2264216	52.22%	4.925%
99	23.598	3480	3487	3501	rVB2	2104983	4102468	94.61%	8.923%




Sum of corrected areas: 45977657

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006399.D
Acq On : 28 Jul 2021 20:21
Operator : CG/JU
Sample : M3107-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGD10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

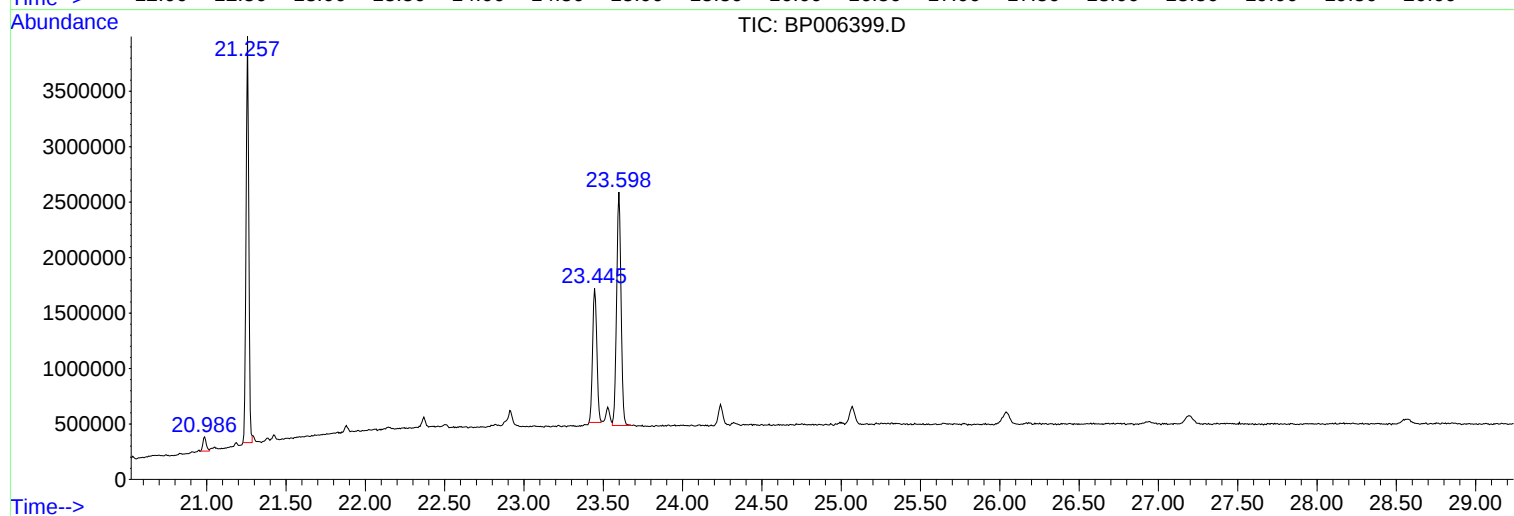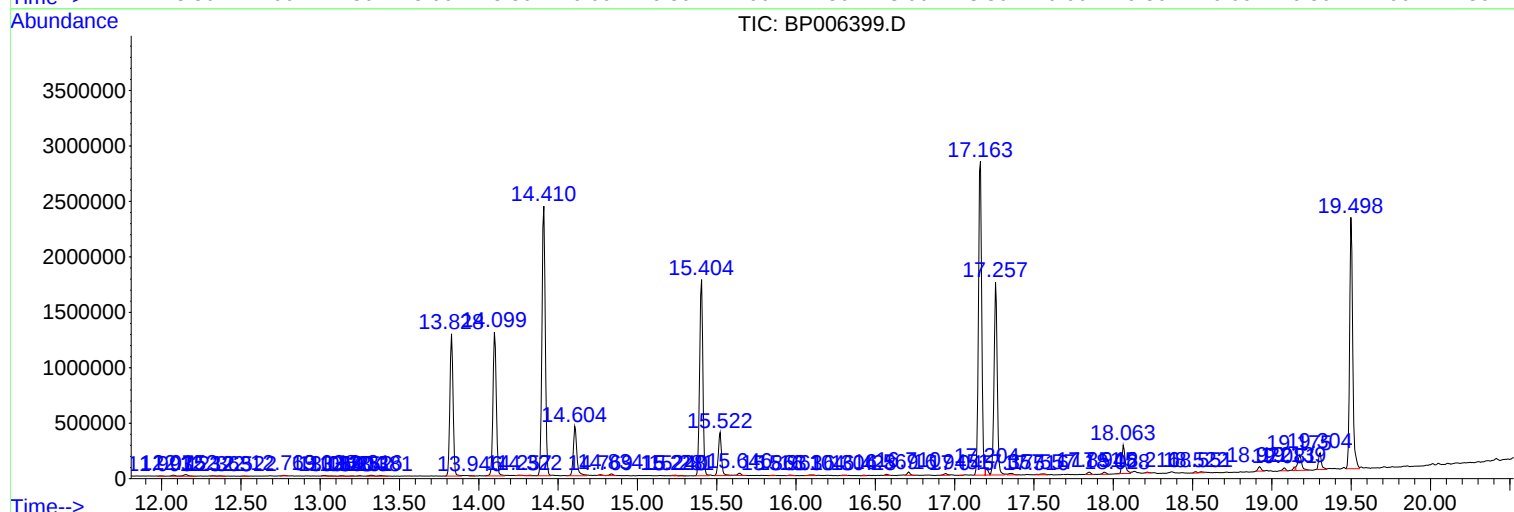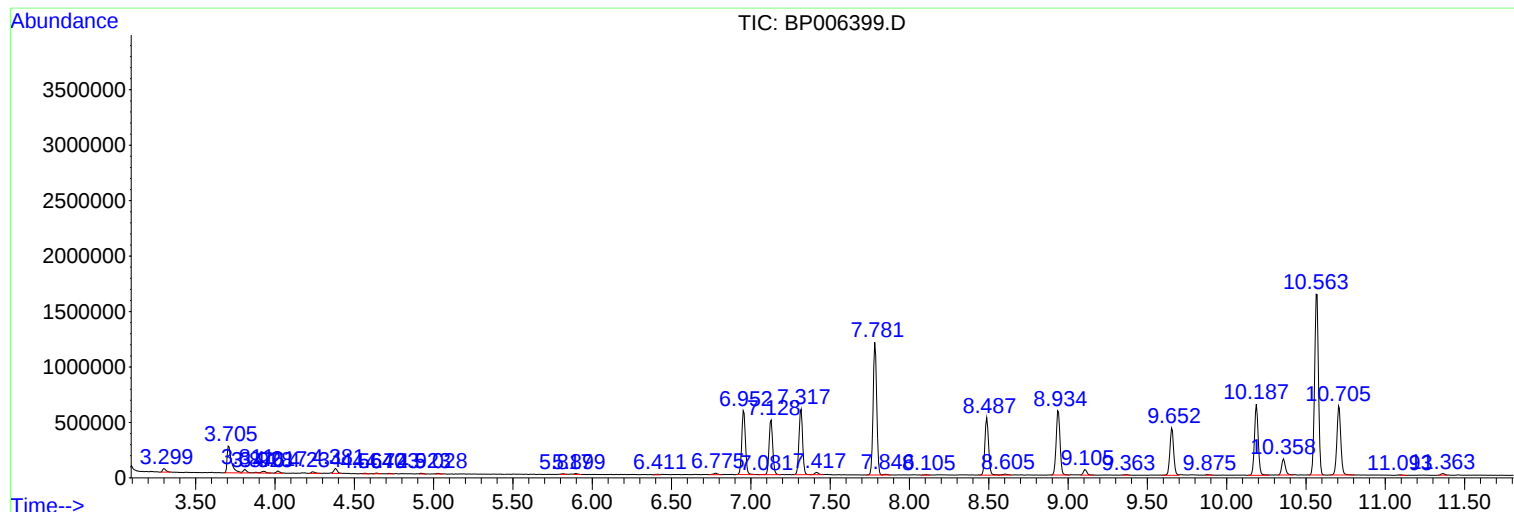

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006399.D
Acq On : 28 Jul 2021 20:21
Operator : CG/JU
Sample : M3107-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGD10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072821\
Data File : BP006399.D
Acq On : 28 Jul 2021 20:21
Operator : CG/JU
Sample : M3107-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGD10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
