

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073021\
 Data File : BP006442.D
 Acq On : 30 Jul 2021 17:17
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTDICC1.6

Quant Time: Jul 30 18:04:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270-SIM-BP073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 30 17:01:25 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.759	152	3105	0.400	ng	#-0.03
7) Naphthalene-d8	10.546	136	11560	0.400	ng	0.00
13) Acenaphthene-d10	14.390	164	6064	0.400	ng	0.00
19) Phenanthrene-d10	17.136	188	11570	0.400	ng	0.00
29) Chrysene-d12	21.253	240	10633	0.400	ng	0.00
35) Perylene-d12	23.589	264	9575	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.357	112	14750	1.766	ng	0.00
5) Phenol-d6	6.941	99	20148	1.907	ng	0.00
8) Nitrobenzene-d5	8.913	82	19358	2.501	ng	0.00
11) 2-Methylnaphthalene-d10	12.144	152	26849	1.476	ng	0.00
14) 2,4,6-Tribromophenol	15.880	330	4456	1.811	ng	0.00
15) 2-Fluorobiphenyl	13.025	172	38949	1.686	ng	0.00
27) Fluoranthene-d10	19.140	212	53221	1.626	ng	0.00
31) Terphenyl-d14	19.729	244	35197	1.301	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.299	88	5348	4.926	ng	# 100
3) n-Nitrosodimethylamine	3.615	42	6686	3.139	ng	# 91
6) bis(2-Chloroethyl)ether	7.204	93	17459	2.105	ng	# 46
9) Naphthalene	10.588	128	54073	1.802	ng	98
10) Hexachlorobutadiene	10.898	225	8910	1.535	ng	# 98
12) 2-Methylnaphthalene	12.216	142	35064	1.726	ng	99
16) Acenaphthylene	14.101	152	46437	1.685	ng	100
17) Acenaphthene	14.453	154	33801	1.970	ng	97
18) Fluorene	15.446	166	39954	1.853	ng	98
20) 4,6-Dinitro-2-methylph...	15.529	198	4358	5.059	ng	# 88
21) 4-Bromophenyl-phenylether	16.342	248	11859	1.724	ng	96
22) Hexachlorobenzene	16.441	284	12922	1.926	ng	98
23) Atrazine	16.620	200	10080	1.628	ng	97
24) Pentachlorophenol	16.798	266	5935	2.415	ng	99
25) Phenanthrene	17.175	178	63497	1.990	ng	100
26) Anthracene	17.275	178	56679	1.836	ng	100
28) Fluoranthene	19.164	202	72639	1.991	ng	100
30) Pyrene	19.522	202	72962	2.007	ng	100
32) Benzo(a)anthracene	21.236	228	68343	1.893	ng	99
33) Chrysene	21.288	228	67876	1.980	ng	99
34) Bis(2-ethylhexyl)phtha...	21.167	149	46416	2.244	ng	98
36) Indeno(1,2,3-cd)pyrene	25.998	276	75313	2.156	ng	99
37) Benzo(b)fluoranthene	22.873	252	69060	2.129	ng	# 92
38) Benzo(k)fluoranthene	22.922	252	68829	2.153	ng	# 91
39) Benzo(a)pyrene	23.481	252	59340	2.025	ng	# 88
40) Dibenzo(a,h)anthracene	26.019	278	63476	2.157	ng	96
41) Benzo(g,h,i)perylene	26.735	276	65073	2.193	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073021\
Data File : BP006442.D
Acq On : 30 Jul 2021 17:17
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6

Quant Time: Jul 30 18:04:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270-SIM-BP073021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 17:01:25 2021
Response via : Initial Calibration




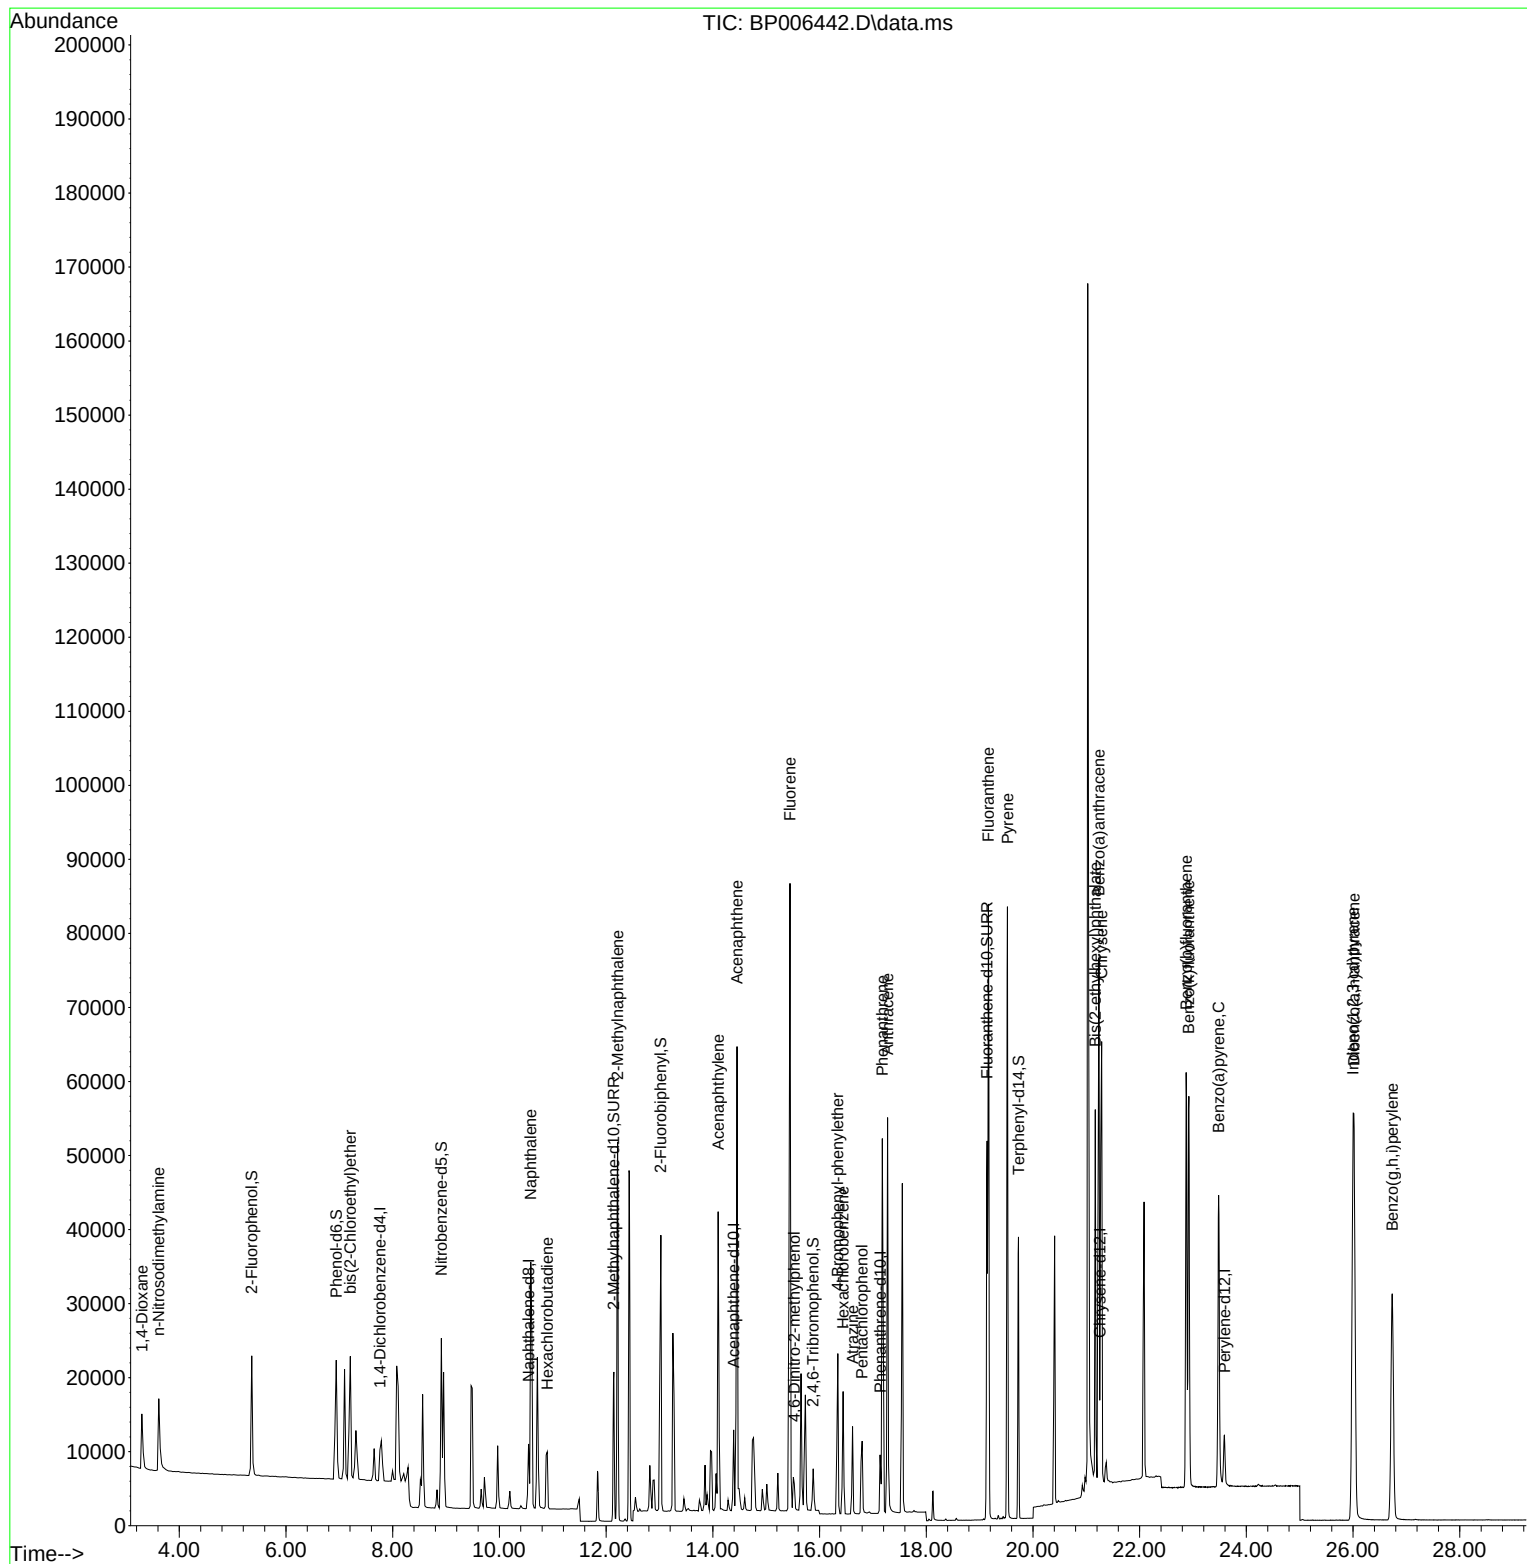




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.759 min Scan# 178
 Delta R.T. -0.026 min
 Lab File: BP006442.D
 Acq: 30 Jul 2021 17:17




Instrument :
 BNA_P
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:152 Resp: 3105
 Ion Ratio Lower Upper
 152 100
 150 175.7 105.7 158.5#
 115 96.8 41.6 62.4#

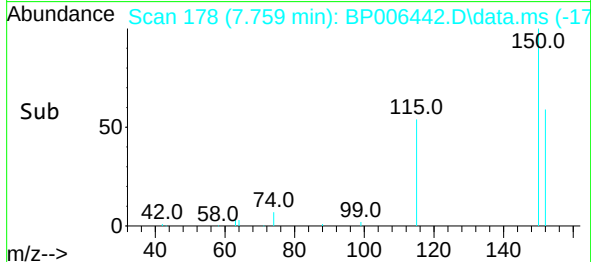

#2
 1,4-Dioxane
 Concen: 4.926 ng
 RT: 3.299 min Scan# 9
 Delta R.T. -0.026 min
 Lab File: BP006442.D
 Acq: 30 Jul 2021 17:17

Tgt Ion: 88 Resp: 5348
 Ion Ratio Lower Upper
 88 100
 43 47.4 0.0 0.0#
 58 121.3 0.0 0.0#


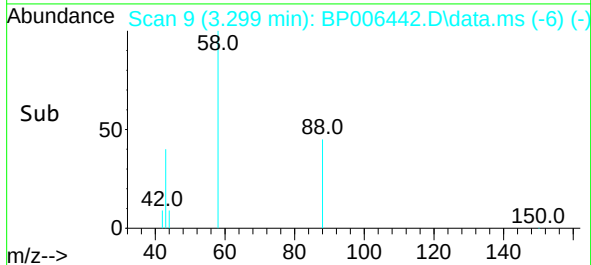




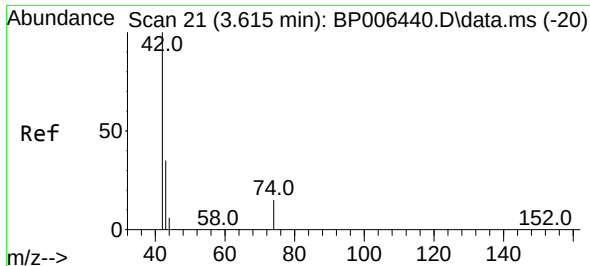

#3
n-Nitrosodimethylamine
Concen: 3.139 ng
RT: 3.615 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 6686
Ion Ratio Lower Upper
42 100
74 151.7 0.0 0.0#
44 6.0 7.4 11.0#

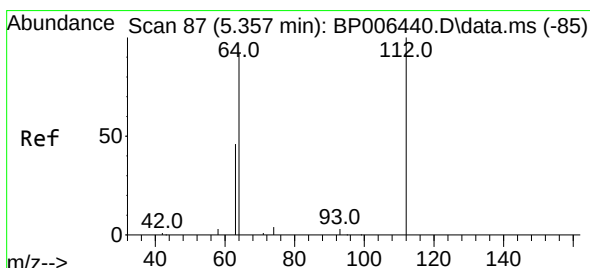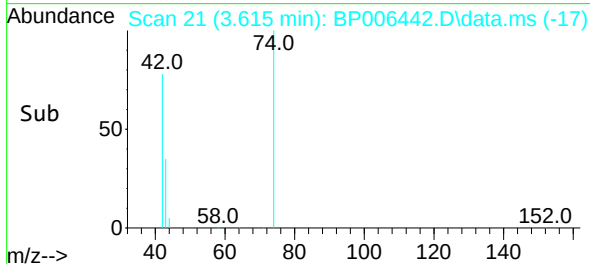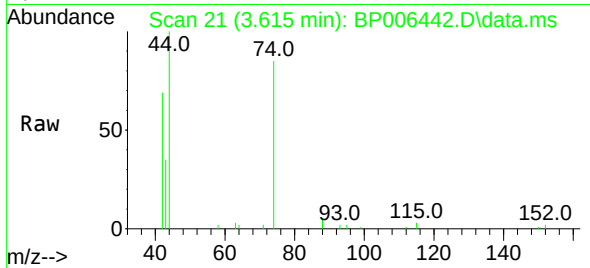

#4
2-Fluorophenol
Concen: 1.766 ng
RT: 5.357 min Scan# 87
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion: 112 Resp: 14750
Ion Ratio Lower Upper
112 100
64 62.2 58.7 88.1
63 30.7 29.8 44.8


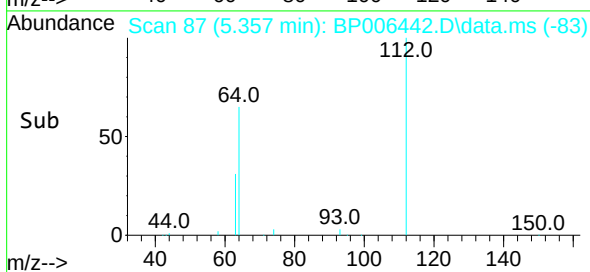

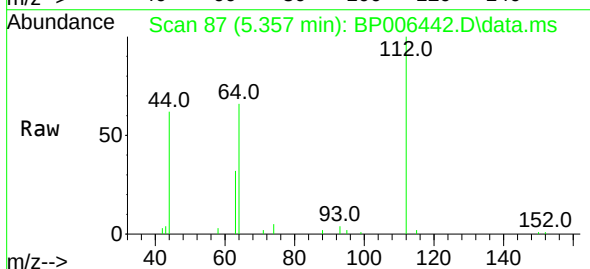




#5
Phenol-d6
Concen: 1.907 ng
RT: 6.941 min Scan# 147
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 20148
Ion Ratio Lower Upper
99 100
42 0.0 0.0 0.0
71 30.6 25.0 37.4

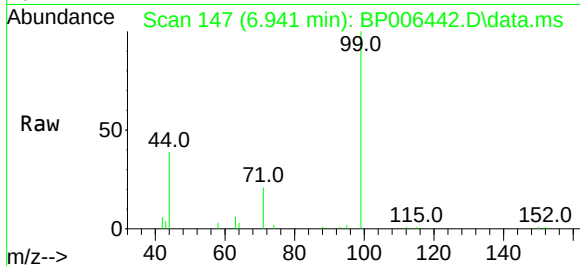

#6
bis(2-Chloroethyl)ether
Concen: 2.105 ng
RT: 7.204 min Scan# 157
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion: 93 Resp: 17459
Ion Ratio Lower Upper
93 100
63 0.0 51.4 77.0#
95 34.3 27.2 40.8




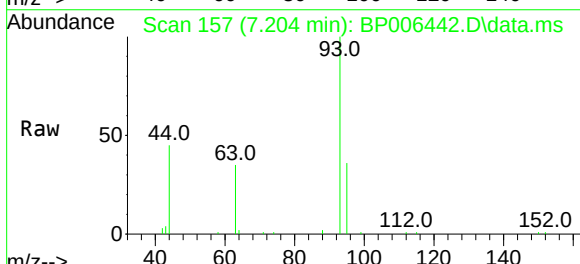




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.546 min Scan# 307
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	11560
Ion	Ratio	Lower	Upper
136	100		
137	11.8	9.2	13.8
54	7.2	6.2	9.2
68	7.0	6.1	9.1

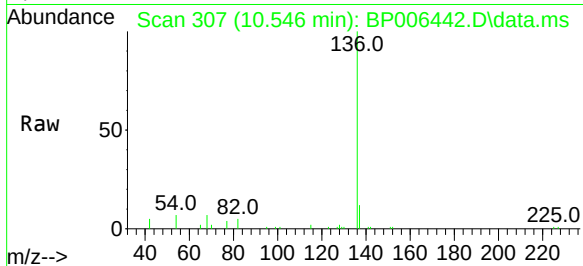

#8
Nitrobenzene-d5
Concen: 2.501 ng
RT: 8.913 min Scan# 228
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:	82	Resp:	19358
Ion	Ratio	Lower	Upper
82	100		
128	34.4	25.5	38.3
54	41.3	37.0	55.6




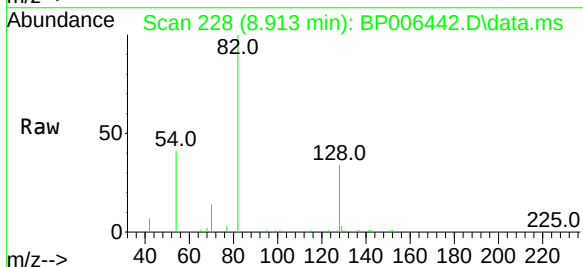




#9
Naphthalene
Concen: 1.802 ng
RT: 10.588 min Scan# 309
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:	128	Resp:	54073
Ion Ratio	Lower	Upper	
128	100		
129	10.8	9.3	13.9
127	14.0	12.0	18.0



#10
Hexachlorobutadiene
Concen: 1.535 ng
RT: 10.898 min Scan# 324
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:	225	Resp:	8910
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.2	50.0	75.0









#11
2-Methylnaphthalene-d10
Concen: 1.476 ng
RT: 12.144 min Scan# 442
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 26849
Ion Ratio Lower Upper
152 100
151 21.1 17.0 25.4



#12
2-Methylnaphthalene
Concen: 1.726 ng
RT: 12.216 min Scan# 452
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:142 Resp: 35064
Ion Ratio Lower Upper
142 100
141 88.8 71.9 107.9
115 38.6 31.9 47.9







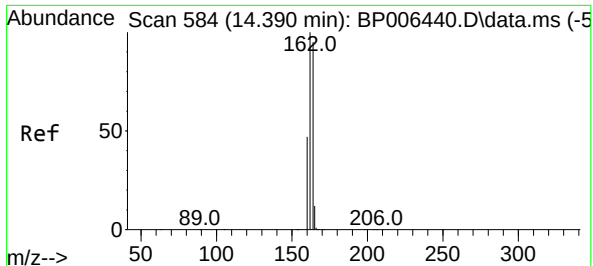

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.390 min Scan# 584
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 6064
Ion Ratio Lower Upper
164 100
162 103.5 84.3 126.5
160 49.6 40.1 60.1

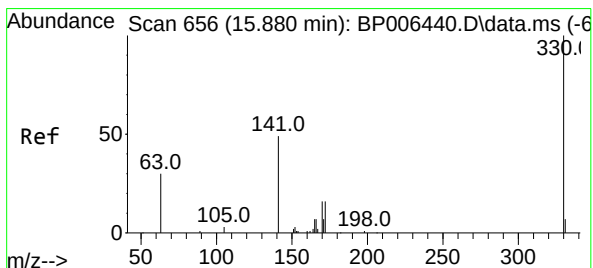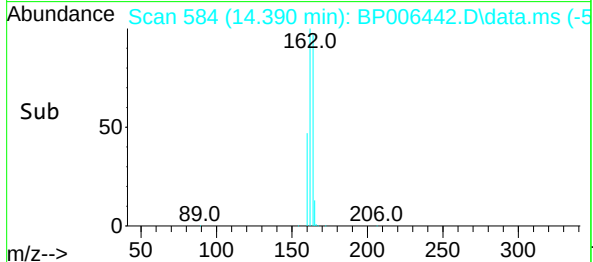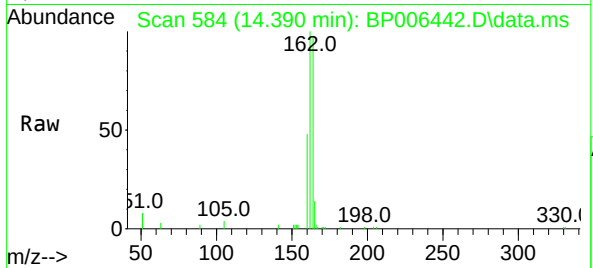

#14
2,4,6-Tribromophenol
Concen: 1.811 ng
RT: 15.880 min Scan# 656
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:330 Resp: 4456
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 45.2 36.5 54.7


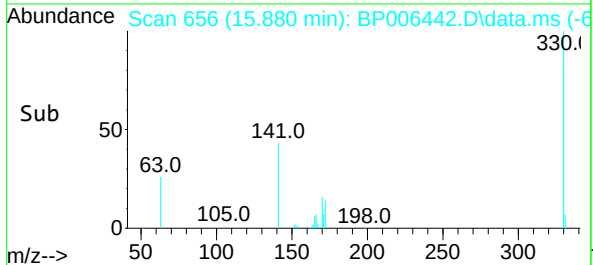

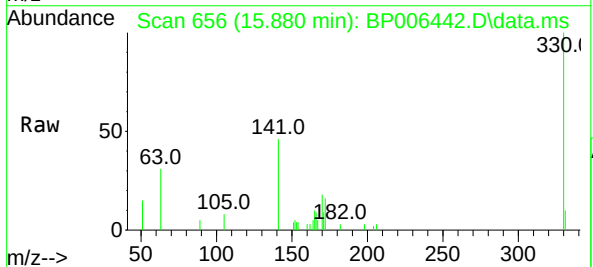




#15
2-Fluorobiphenyl
Concen: 1.686 ng
RT: 13.025 min Scan# 518
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:	172	Resp:	38949
Ion Ratio	Lower	Upper	
172	100		
171	33.2	27.4	41.0
170	21.3	18.2	27.2

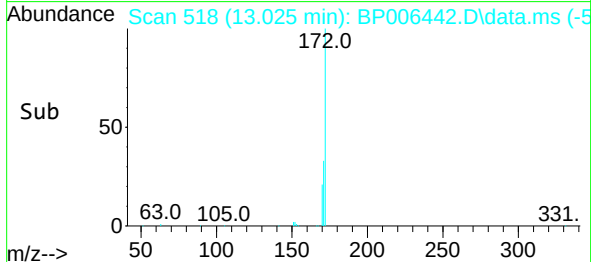

#16
Acenaphthylene
Concen: 1.685 ng
RT: 14.101 min Scan# 570
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:	152	Resp:	46437
Ion Ratio	Lower	Upper	
152	100		
151	19.5	15.7	23.5
153	12.9	10.2	15.4




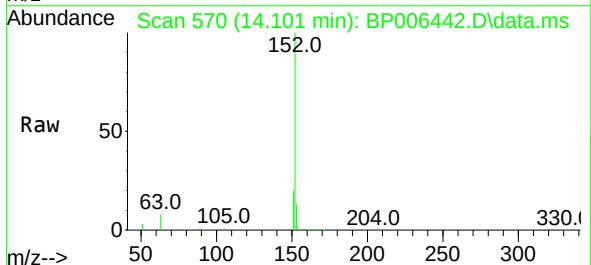




#17
Acenaphthene
Concen: 1.970 ng
RT: 14.453 min Scan# 587
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 33801
Ion Ratio Lower Upper
154 100
153 107.4 88.4 132.6
152 54.4 44.7 67.1



#18
Fluorene
Concen: 1.853 ng
RT: 15.446 min Scan# 635
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:166 Resp: 39954
Ion Ratio Lower Upper
166 100
165 98.8 80.8 121.2
167 13.6 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.136 min Scan# 719
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 11570
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 20.8 17.0 25.4



#20
4,6-Dinitro-2-methylphenol
Concen: 5.059 ng
RT: 15.529 min Scan# 639
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:198 Resp: 4358
Ion Ratio Lower Upper
198 100
182 11.9 13.8 20.8#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 1.724 ng
RT: 16.342 min Scan# 679
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 11859
Ion Ratio Lower Upper
248 100
250 98.5 77.6 116.4
141 32.6 31.0 46.6

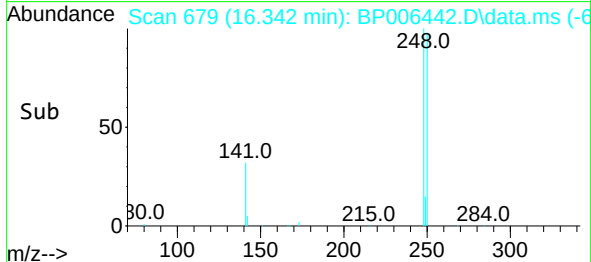

#22
Hexachlorobenzene
Concen: 1.926 ng
RT: 16.441 min Scan# 684
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:284 Resp: 12922
Ion Ratio Lower Upper
284 100
142 46.4 38.4 57.6
249 33.6 27.4 41.2




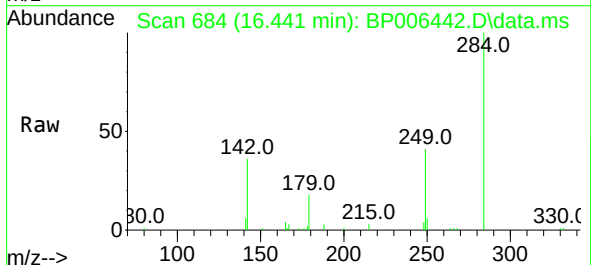




#23
Atrazine
Concen: 1.628 ng
RT: 16.620 min Scan# 693
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 10080
Ion Ratio Lower Upper
200 100
173 20.1 18.6 28.0
215 45.6 37.0 55.4



#24
Pentachlorophenol
Concen: 2.415 ng
RT: 16.798 min Scan# 702
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:266 Resp: 5935
Ion Ratio Lower Upper
266 100
264 62.5 49.8 74.8
268 65.5 51.8 77.6









#25
Phenanthrene
Concen: 1.990 ng
RT: 17.175 min Scan# 721
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 63497
Ion Ratio Lower Upper
178 100
176 19.4 15.5 23.3
179 15.1 12.3 18.5



#26
Anthracene
Concen: 1.836 ng
RT: 17.275 min Scan# 726
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:178 Resp: 56679
Ion Ratio Lower Upper
178 100
176 18.8 15.1 22.7
179 15.2 12.0 18.0









#27
Fluoranthene-d10
Concen: 1.626 ng
RT: 19.140 min Scan# 905
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 53221
Ion Ratio Lower Upper
212 100
106 18.6 14.6 21.8
104 10.9 8.9 13.3

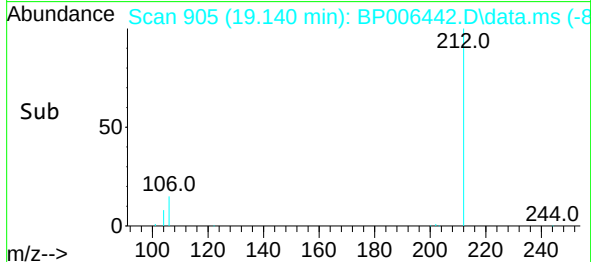

#28
Fluoranthene
Concen: 1.991 ng
RT: 19.164 min Scan# 908
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:202 Resp: 72639
Ion Ratio Lower Upper
202 100
101 14.1 11.3 16.9
203 17.0 13.4 20.2

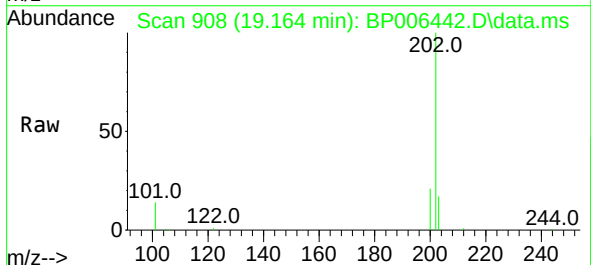



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.253 min Scan# 1086

Delta R.T. 0.000 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17

Instrument :

BNA_P

ClientSampleId :

SSTDICC1.6





Tgt Ion:240 Resp: 10633

Ion Ratio Lower Upper

240 100

120 7.8 5.8 8.8

236 27.9 22.6 33.8

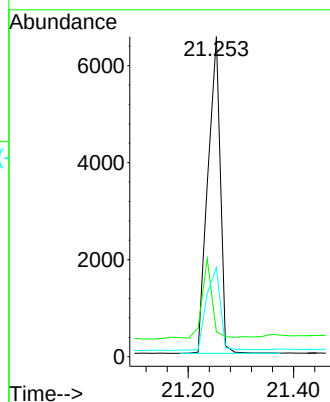

#30

Pyrene

Concen: 2.007 ng

RT: 19.522 min Scan# 953

Delta R.T. -0.000 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17




Tgt Ion:202 Resp: 72962


Ion Ratio Lower Upper

202 100

200 21.3 16.9 25.3

203 17.3 14.1 21.1



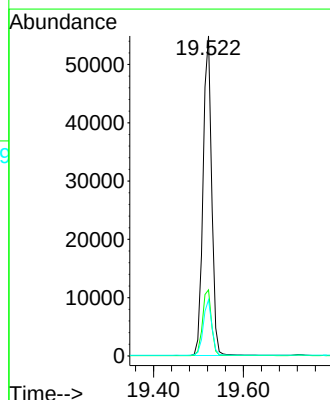



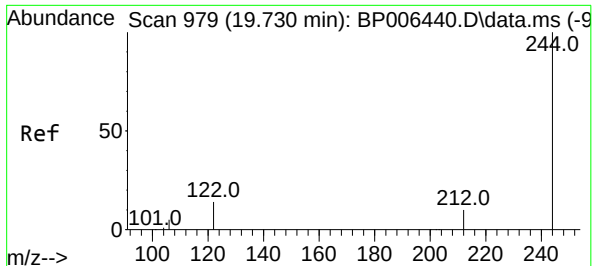

#31
 Terphenyl-d14
 Concen: 1.301 ng
 RT: 19.729 min Scan# 979
 Delta R.T. -0.000 min
 Lab File: BP006442.D
 Acq: 30 Jul 2021 17:17




Instrument :
 BNA_P
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	244	Resp:	35197
Ion Ratio	Lower	Upper	
244	100		
212	10.1	8.5	12.7
122	15.7	11.8	17.6

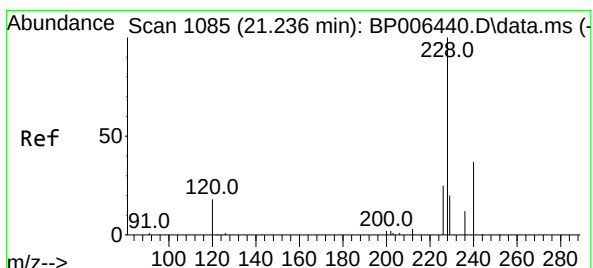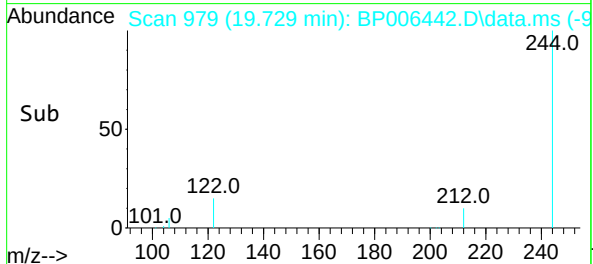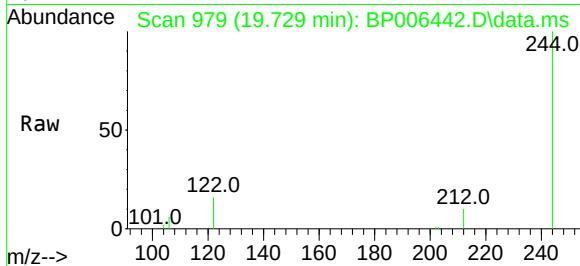

#32
 Benzo(a)anthracene
 Concen: 1.893 ng
 RT: 21.236 min Scan# 1085
 Delta R.T. 0.000 min
 Lab File: BP006442.D
 Acq: 30 Jul 2021 17:17

Tgt Ion:	228	Resp:	68343
Ion Ratio	Lower	Upper	
228	100		
226	25.2	20.6	30.8
229	20.9	16.6	25.0

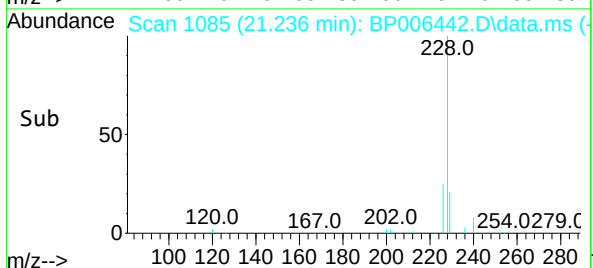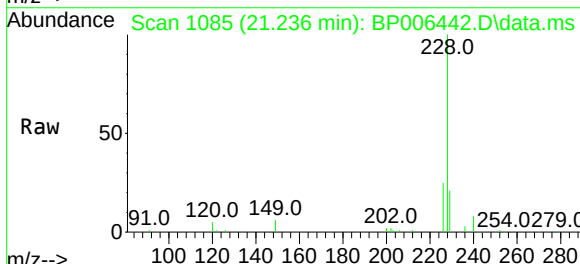

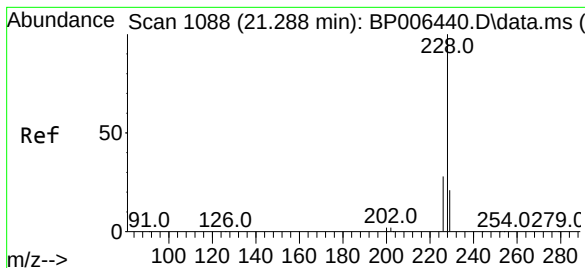

#33

Chrysene

Concen: 1.980 ng

RT: 21.288 min Scan# 1088

Delta R.T. 0.000 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17

Instrument :

BNA_P

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 67876

Ion Ratio Lower Upper

228 100

226 27.8 22.4 33.6

229 20.8 17.4 26.2

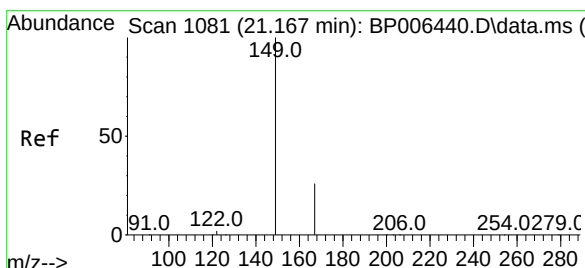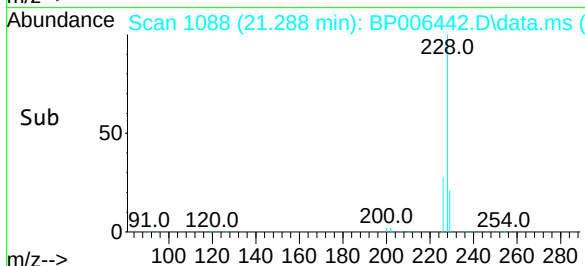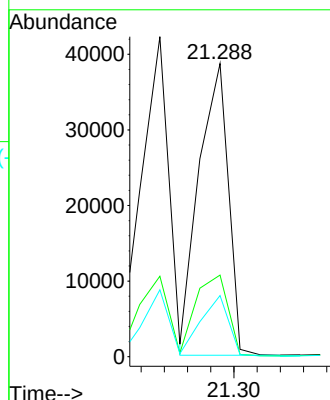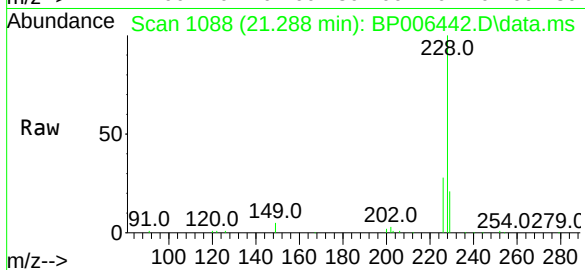

#34

Bis(2-ethylhexyl)phthalate

Concen: 2.244 ng

RT: 21.167 min Scan# 1081

Delta R.T. 0.000 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17




Tgt Ion:149 Resp: 46416


Ion Ratio Lower Upper

149 100

167 24.1 18.5 27.7

279 2.5 2.1 3.1

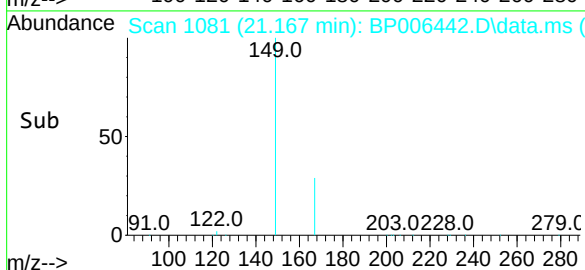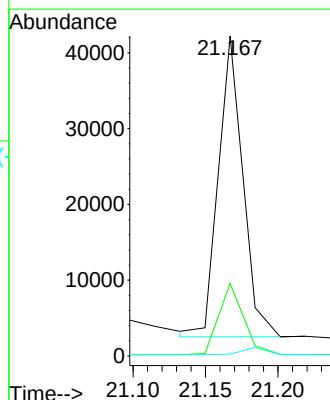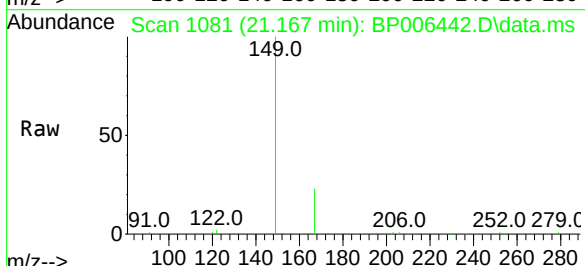



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.589 min Scan# 1370

Delta R.T. 0.005 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17





Tgt Ion:264 Resp: 9575

Ion Ratio Lower Upper

264 100

260 27.6 22.2 33.4

265 90.2 64.2 96.2

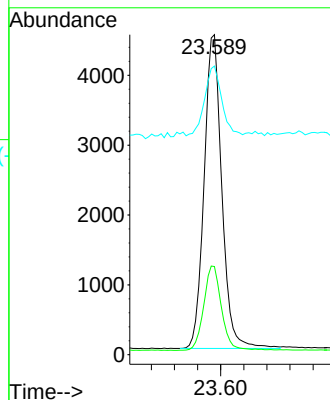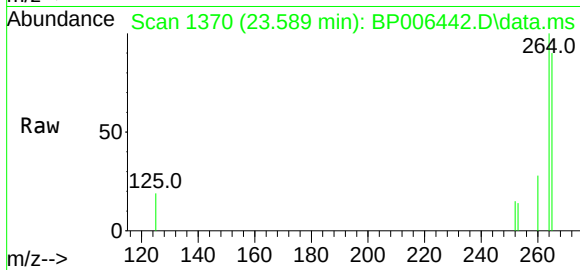

#36

Indeno(1,2,3-cd)pyrene

Concen: 2.156 ng

RT: 25.998 min Scan# 1814

Delta R.T. 0.000 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17




Tgt Ion:276 Resp: 75313


Ion Ratio Lower Upper

276 100

138 35.1 27.7 41.5

277 24.9 19.8 29.8



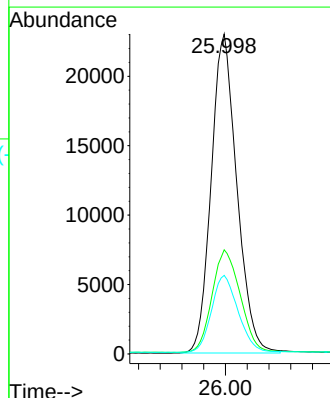
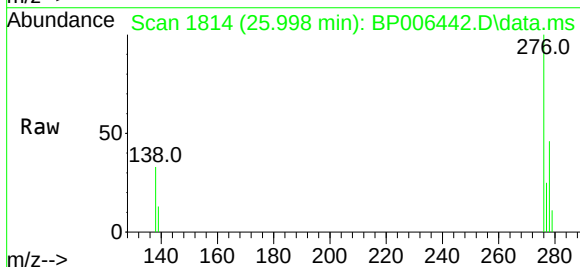




#37
Benzo(b)fluoranthene
Concen: 2.129 ng
RT: 22.873 min Scan# 1238
Delta R.T. -0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17




Instrument :
BNA_P
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 69060
Ion Ratio Lower Upper
252 100
253 22.5 20.8 31.2
125 15.8 16.3 24.5#

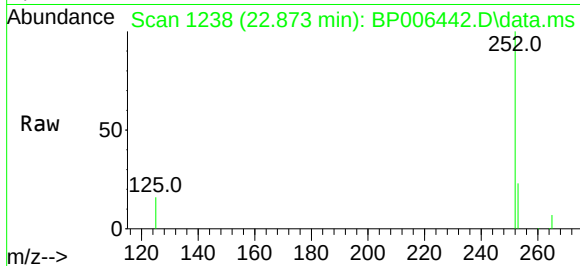

#38
Benzo(k)fluoranthene
Concen: 2.153 ng
RT: 22.922 min Scan# 1247
Delta R.T. 0.000 min
Lab File: BP006442.D
Acq: 30 Jul 2021 17:17

Tgt Ion:252 Resp: 68829
Ion Ratio Lower Upper
252 100
253 23.2 21.0 31.6
125 15.7 17.1 25.7#

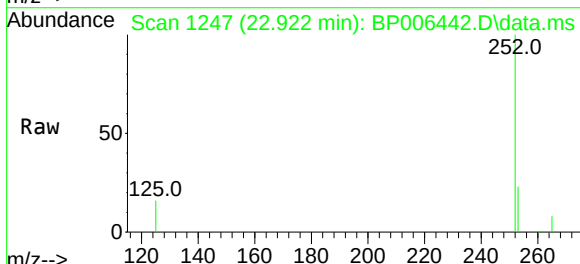



#39

Benzo(a)pyrene

Concen: 2.025 ng

RT: 23.481 min Scan# 1350

Delta R.T. 0.000 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17





Instrument :

BNA_P

ClientSampleId :

SSTDICC1.6

Tgt Ion:252	Resp:	59340
Ion Ratio	Lower	Upper
252	100	
253	23.6	22.9 34.3
125	17.7	20.2 30.2#

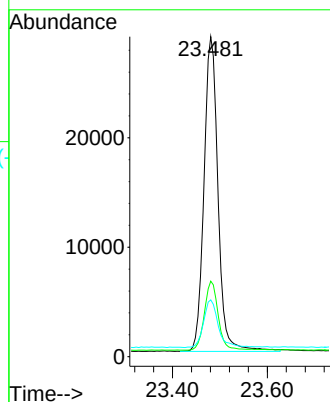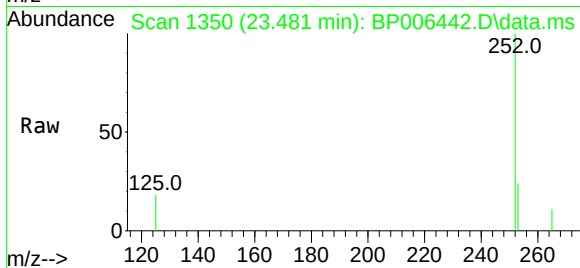

#40

Dibenzo(a,h)anthracene

Concen: 2.157 ng




RT: 26.019 min Scan# 1818


Delta R.T. 0.000 min

Lab File: BP006442.D

Acq: 30 Jul 2021 17:17

Tgt Ion:278	Resp:	63476
Ion Ratio	Lower	Upper
278	100	
139	22.8	19.3 28.9
279	24.1	21.8 32.6

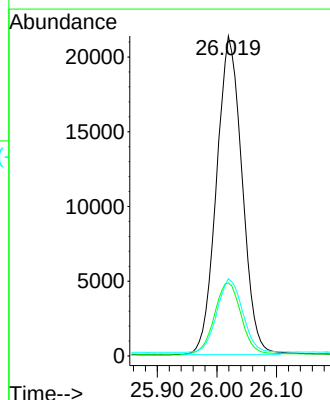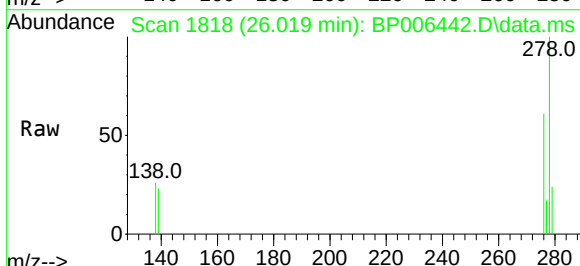

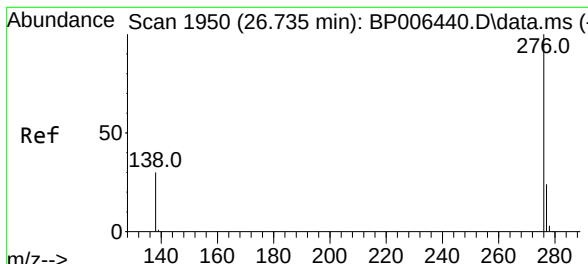

#41
 Benzo(g,h,i)perylene
 Concen: 2.193 ng
 RT: 26.735 min Scan# 1950
 Delta R.T. 0.000 min
 Lab File: BP006442.D
 Acq: 30 Jul 2021 17:17

Instrument :
 BNA_P
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	276	Resp:	65073
Ion Ratio	Lower	Upper	
276	100		
277	24.1	20.6	31.0
138	30.1	25.5	38.3

