
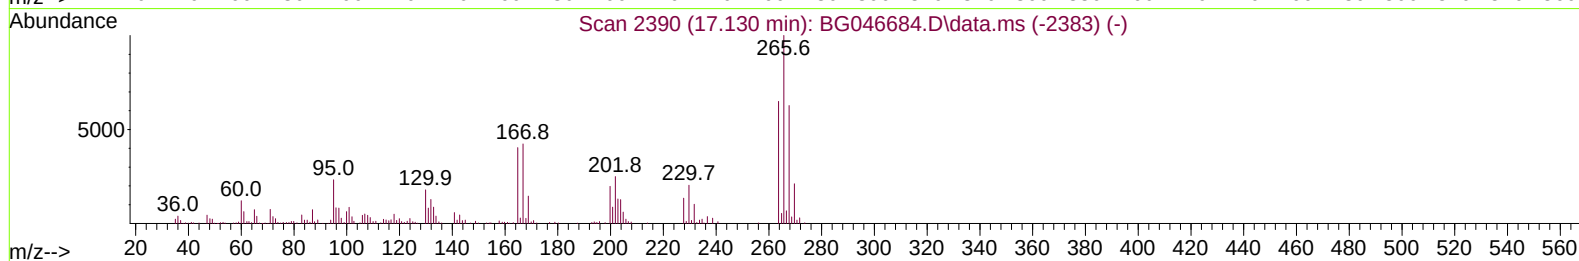
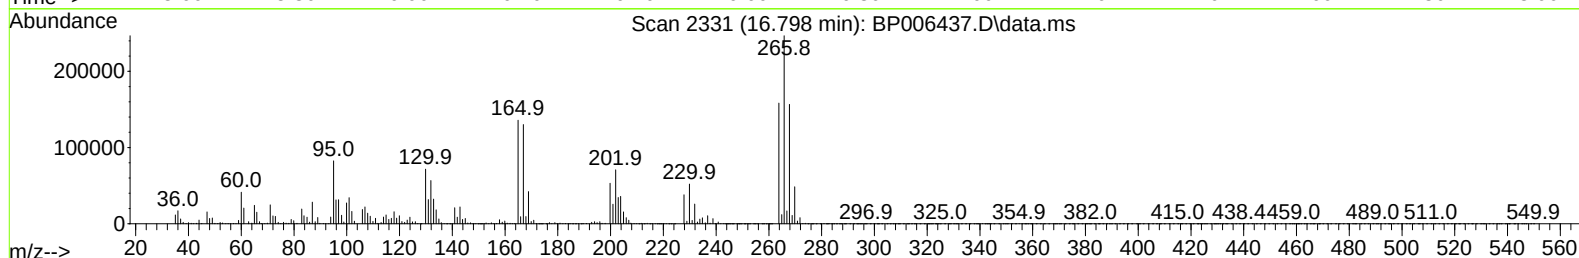


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073021\
 Data File : BP006437.D
 Acq On : 30 Jul 2021 14:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 10:19:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 10:15:39 2021
 Response via : Initial Calibration

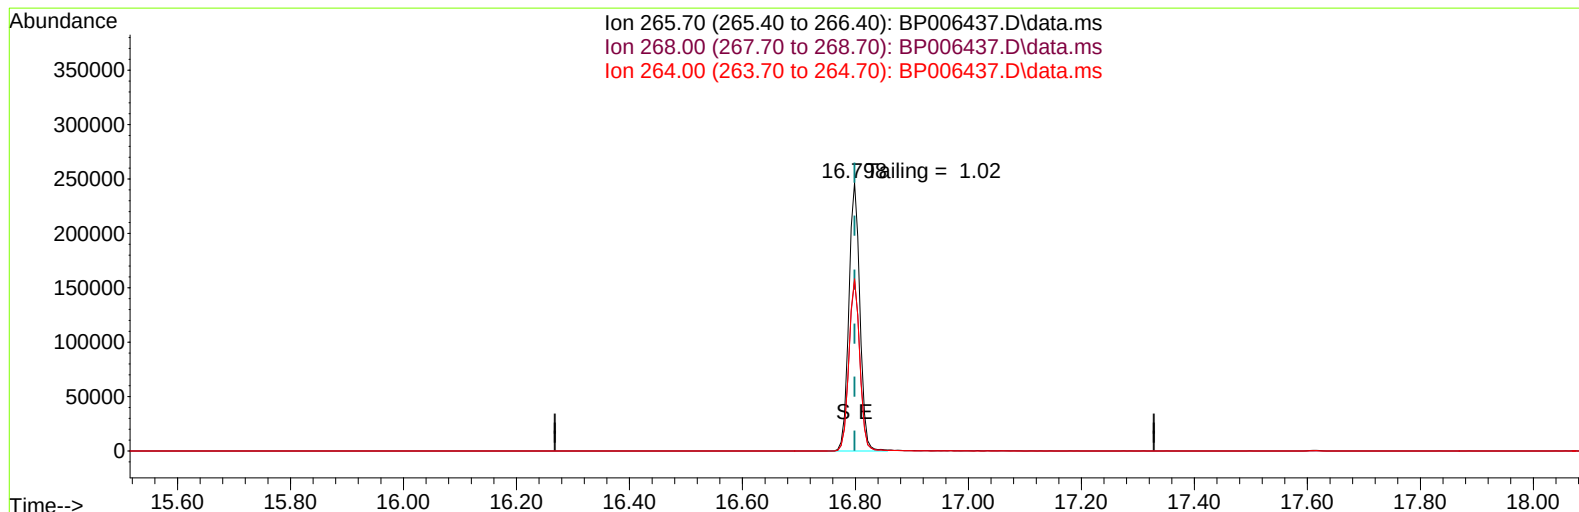

TIC: BP006437.D\data.ms

(70) Pentachlorophenol (C)




16.798min (0.000) 18255.09 ng

response 335518

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.49
264.00	61.60	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073021\
 Data File : BP006437.D
 Acq On : 30 Jul 2021 14:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 10:19:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 10:15:39 2021
 Response via : Initial Calibration

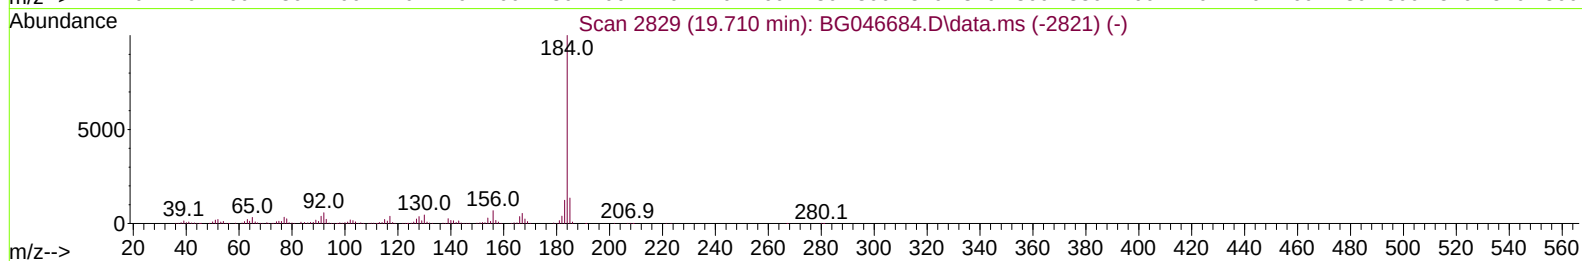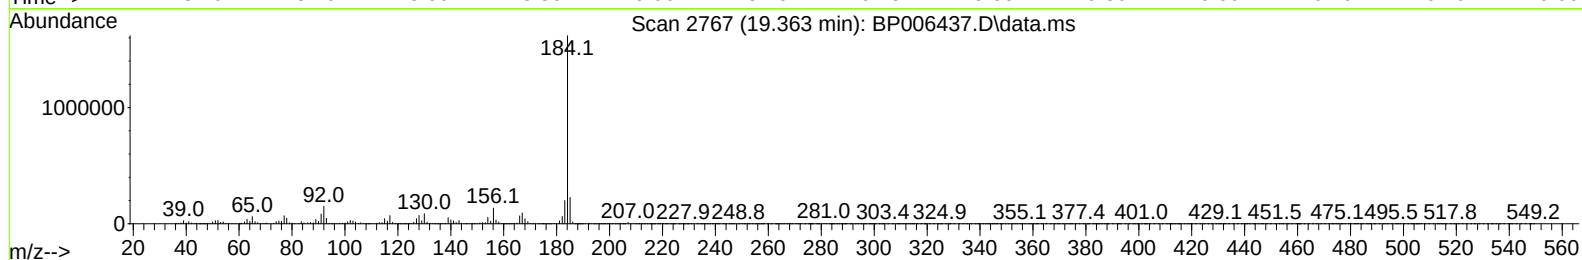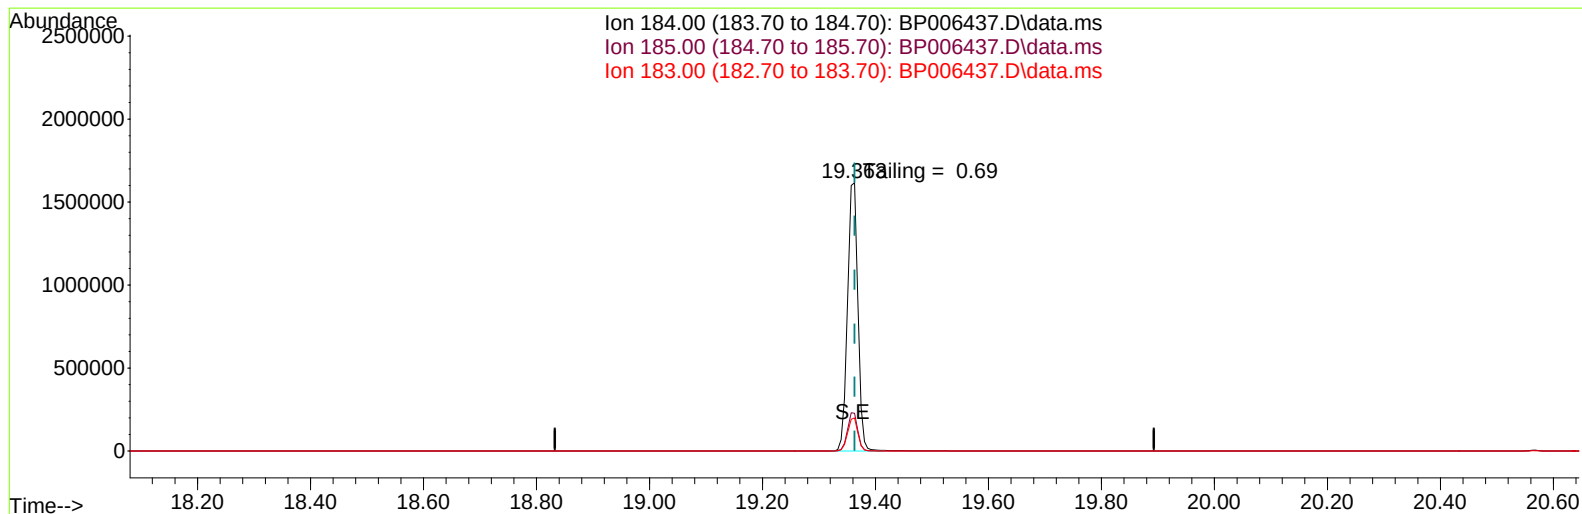

TIC: BP006437.D\data.ms

(77) Benzidine**19.363min (0.000) 2402361.25 ng****response 2073503**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.09
183.00	13.20	12.33
0.00	0.00	0.00