
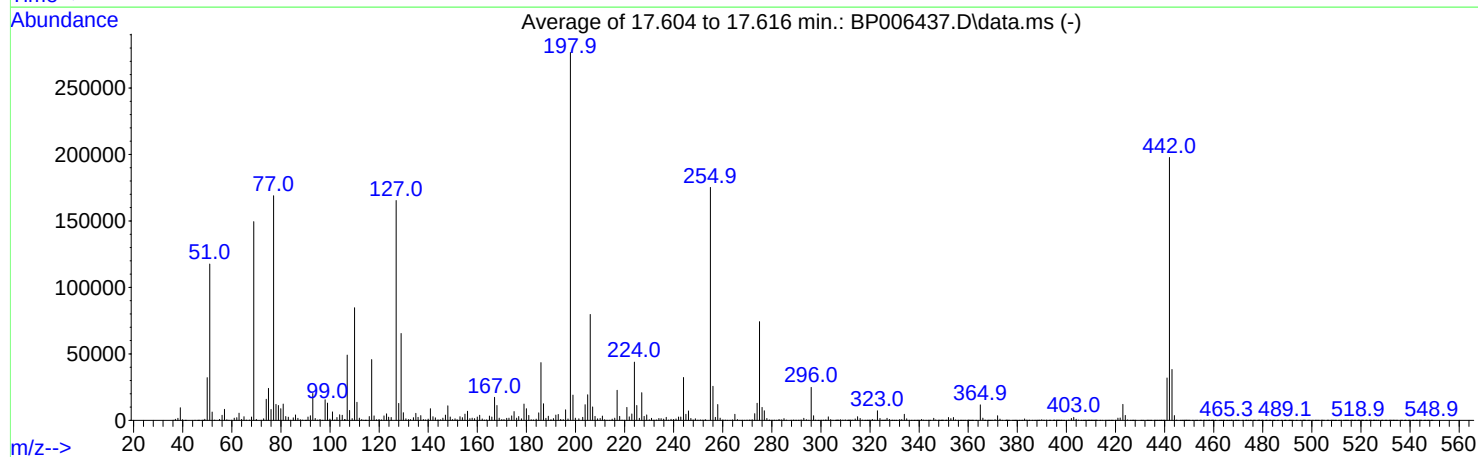


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073021\
 Data File : BP006437.D
 Acq On : 30 Jul 2021 14:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270-SIM-BP073021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 30 18:59:15 2021

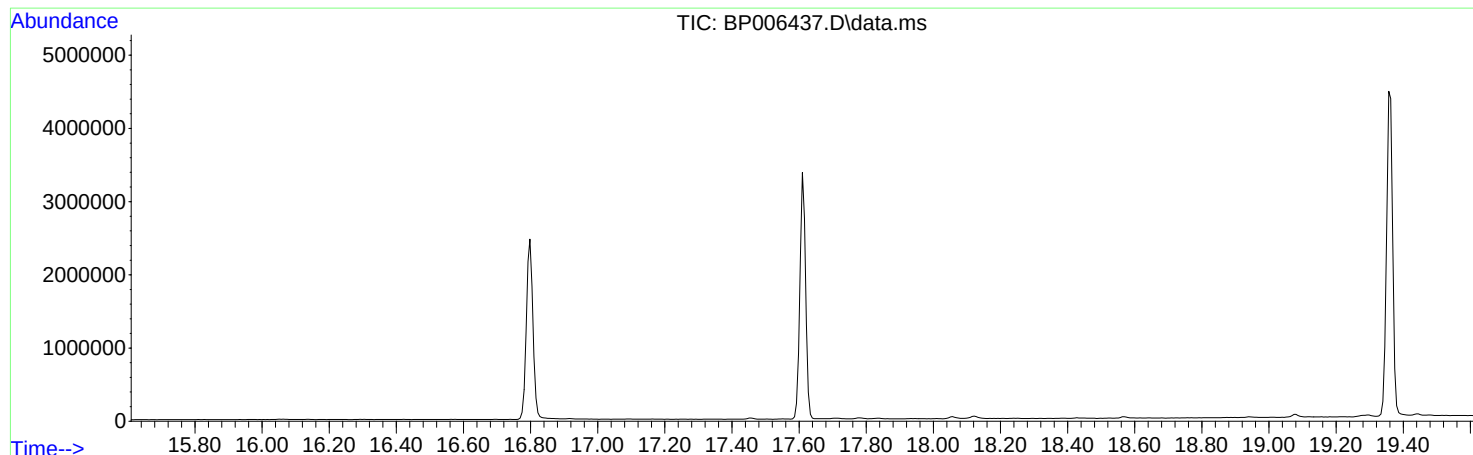

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	117602	PASS
68	69	0.00	2	1.7	2571	PASS
69	198	0.00	100	54.0	149475	PASS
70	69	0.00	2	0.5	797	PASS
127	198	10	80	59.8	165375	PASS
197	198	0.00	2	0.4	1139	PASS
198	198	100	100	100.0	276672	PASS
199	198	5	9	6.9	18987	PASS
275	198	10	60	26.8	74237	PASS
365	198	1	100	4.2	11679	PASS
441	198	0.01	100	11.5	31920	PASS
442	442	50	100	100.0	197723	PASS
443	442	15	24	19.4	38331	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/30/2021	BNA_P	<u>BP006437.D</u>
Compound Name	Response	Retention Time
DDT	994333	20.56
DDD	1622	20.13
DDE	1224	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2846	997179	0.29

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073021\
 Data File : BP006437.D
 Acq On : 30 Jul 2021 14:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 04 10:19:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 10:15:39 2021
 Response via : Initial Calibration

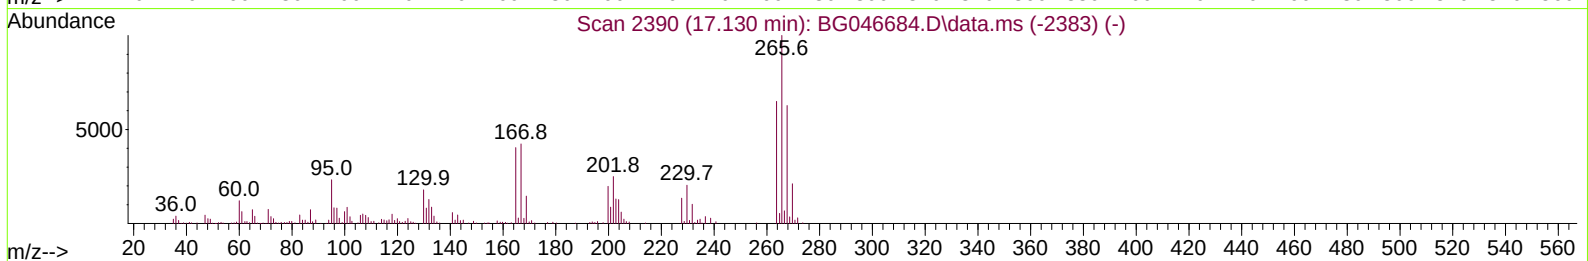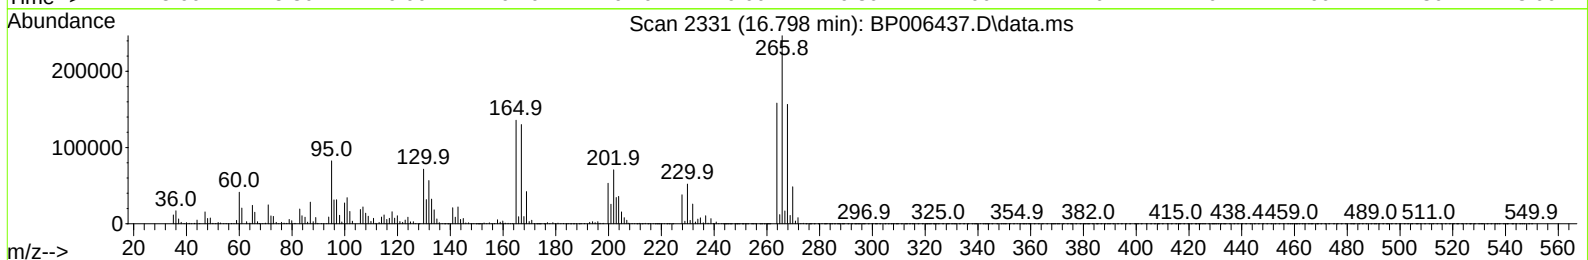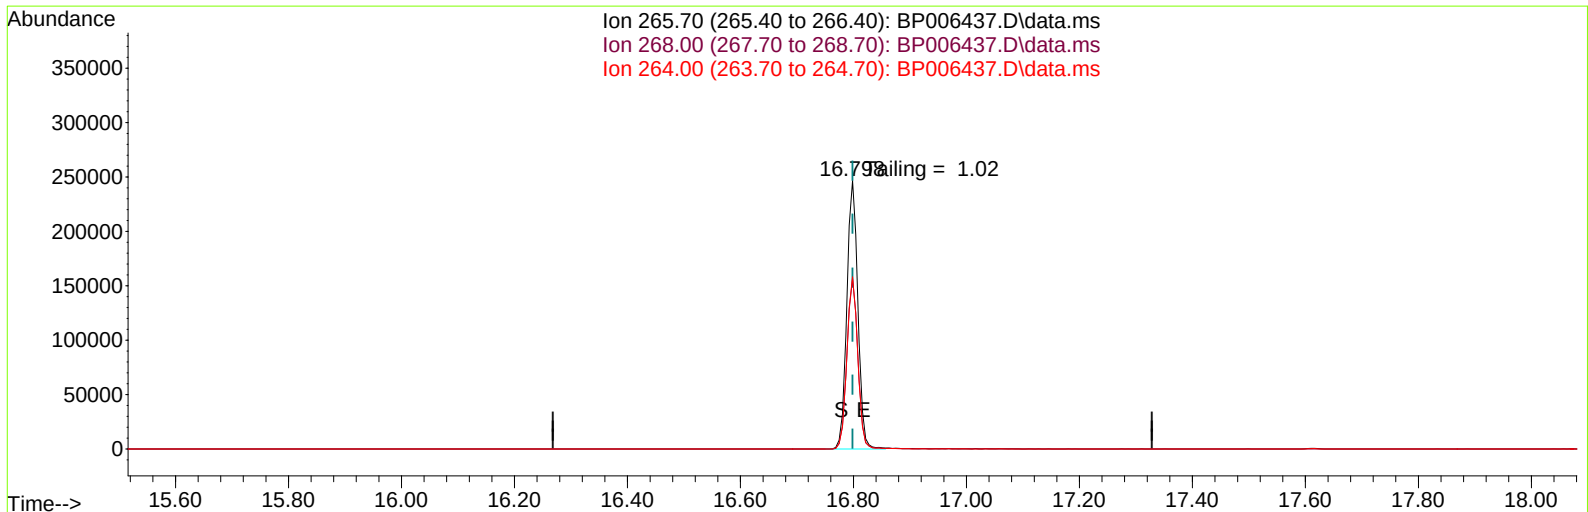

TIC: BP006437.D\data.ms

(70) Pentachlorophenol (C)

16.798min (0.000) 18255.09 ng




response 335518

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.49
264.00	61.60	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP073021\
 Data File : BP006437.D
 Acq On : 30 Jul 2021 14:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 04 10:19:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 10:15:39 2021
 Response via : Initial Calibration

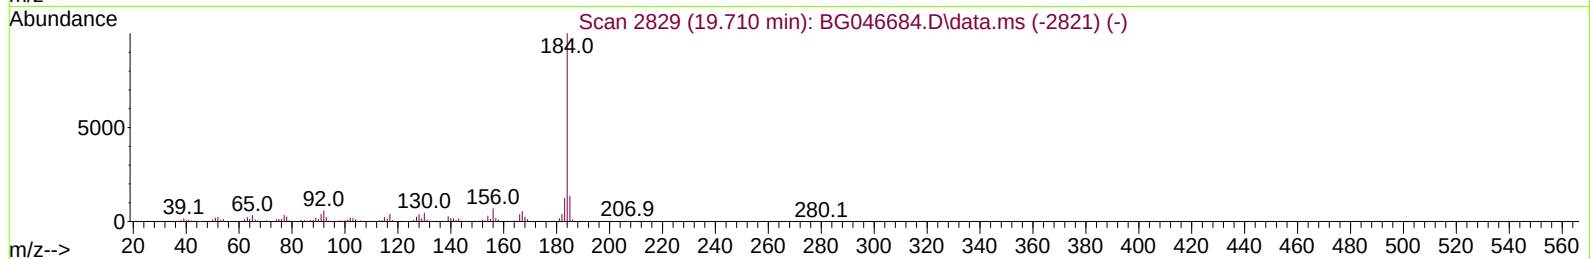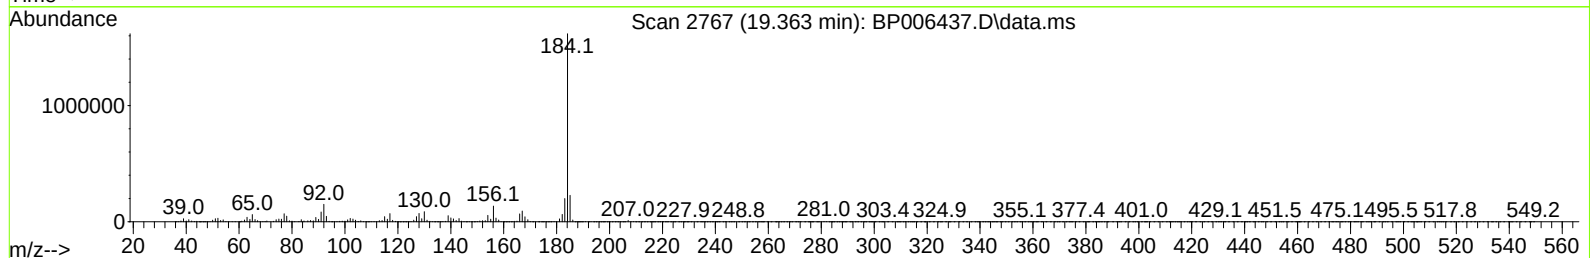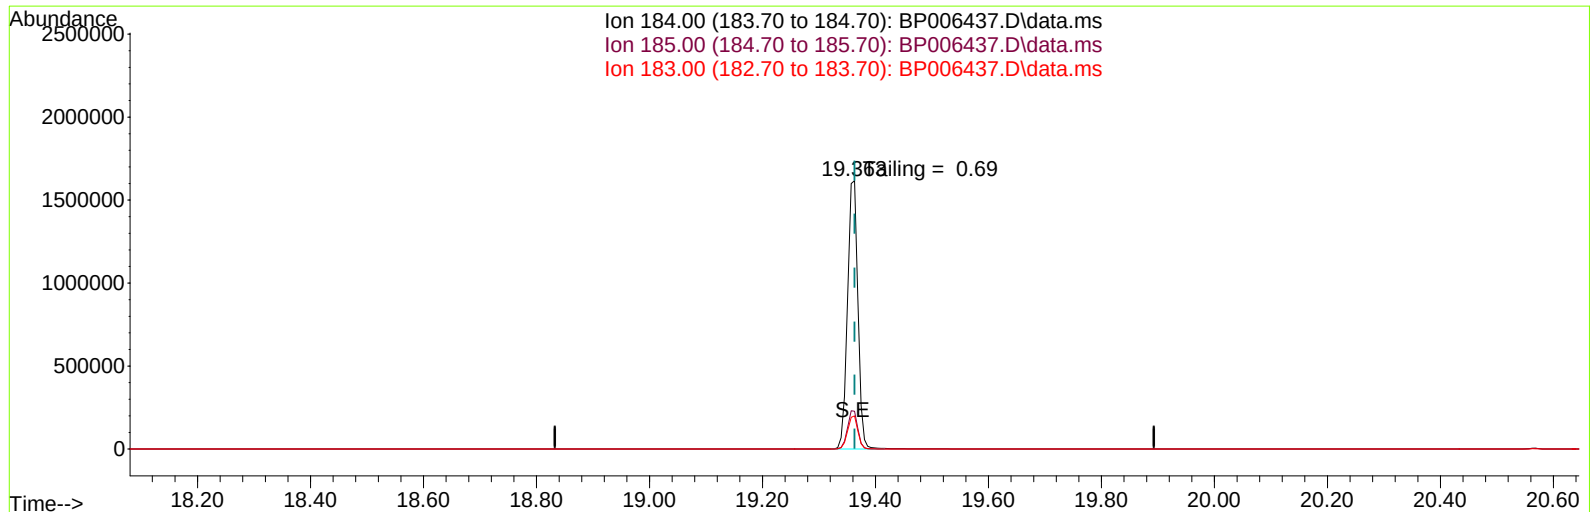

TIC: BP006437.D\data.ms

(77) Benzidine

19.363min (0.000) 2402361.25 ng

response 2073503

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.09
183.00	13.20	12.33
0.00	0.00	0.00