




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 02 10:51:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/05/2024

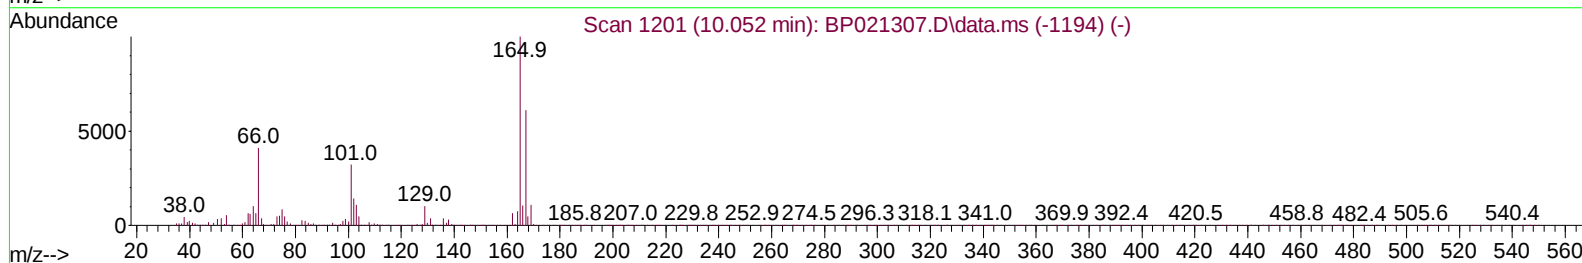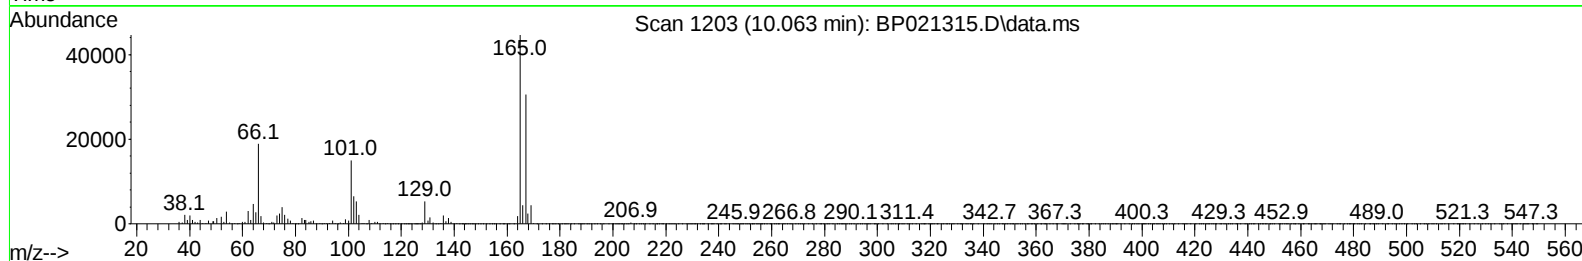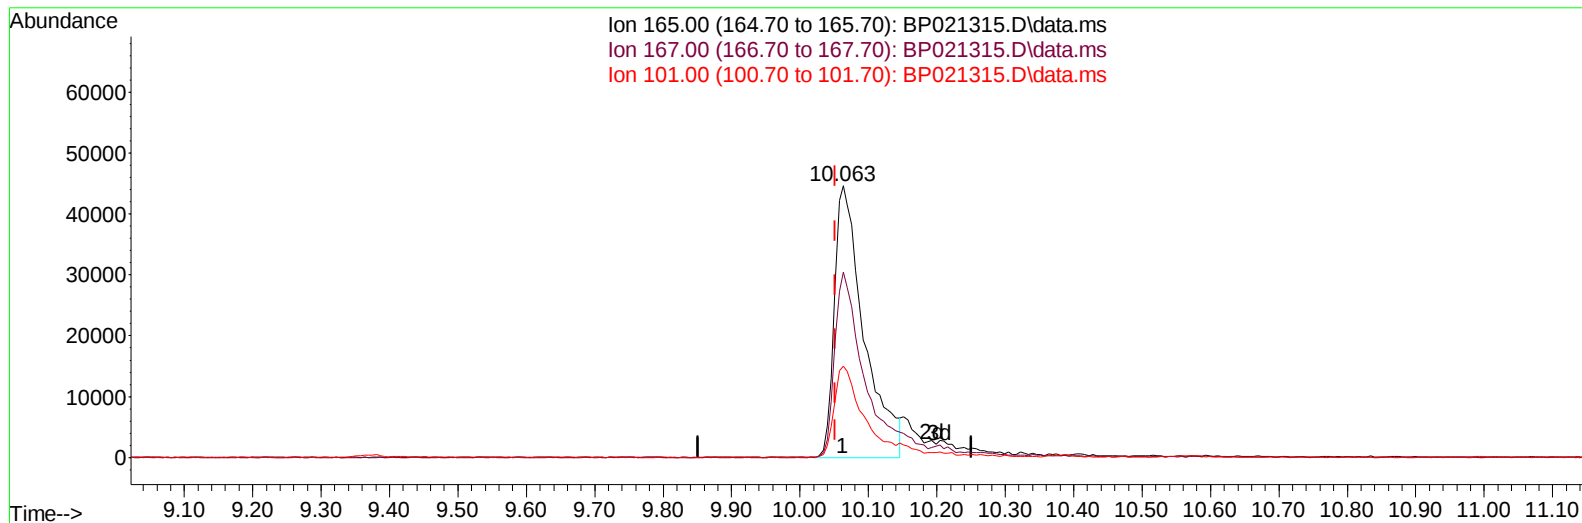

TIC: BP021315.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.063min (+ 0.012) 12.58 ng/u1

response 133655

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	68.34
101.00	35.50	33.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 02 10:51:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/05/2024

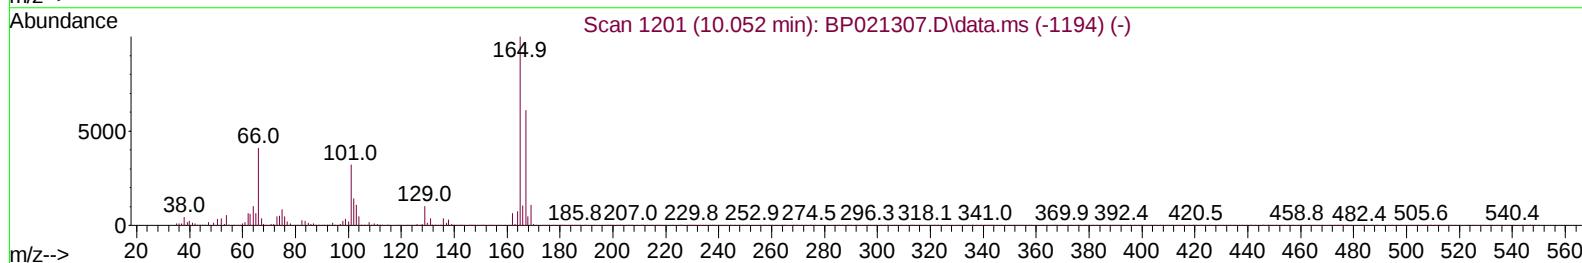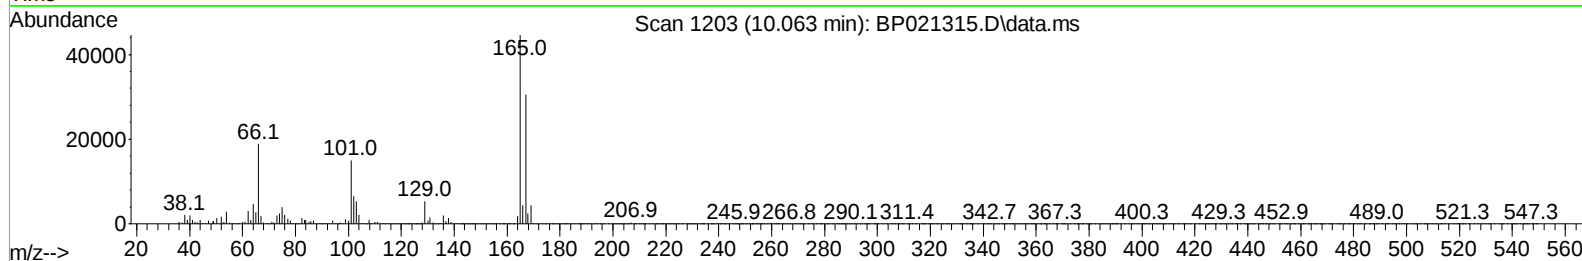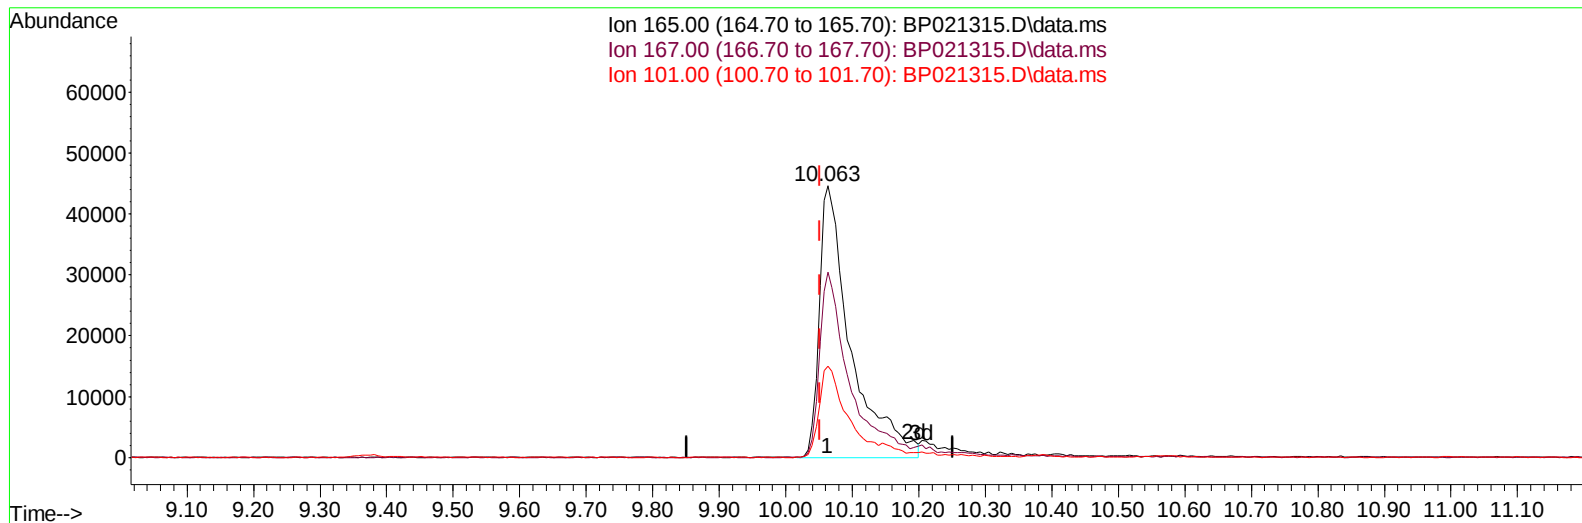

TIC: BP021315.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.063min (+ 0.012) 13.74 ng/ul m

response 145976

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	68.34
101.00	35.50	33.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 02 10:51:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/05/2024

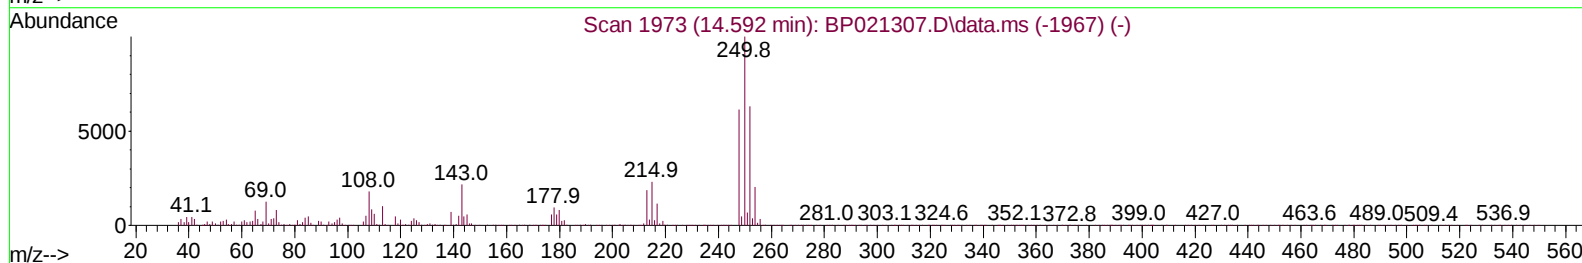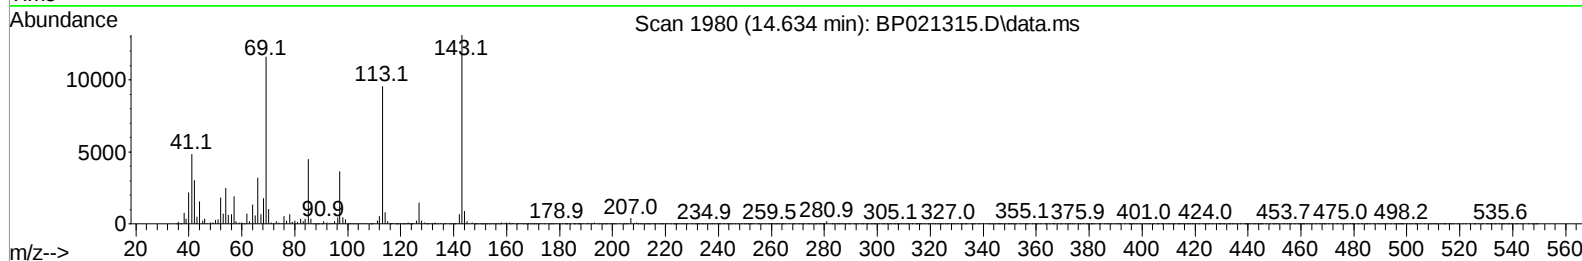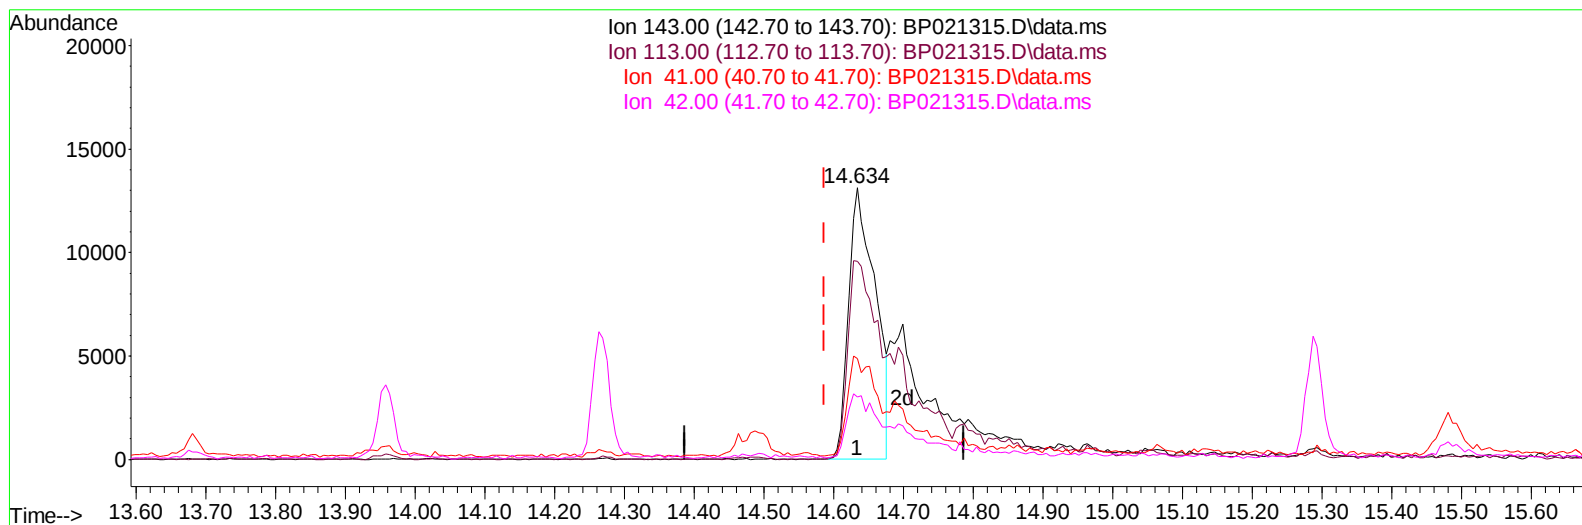

TIC: BP021315.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.634min (+ 0.047) 7.69 ng/u1

response 34848

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	72.96
41.00	37.90	37.08
42.00	27.10	22.93




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 02 10:51:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

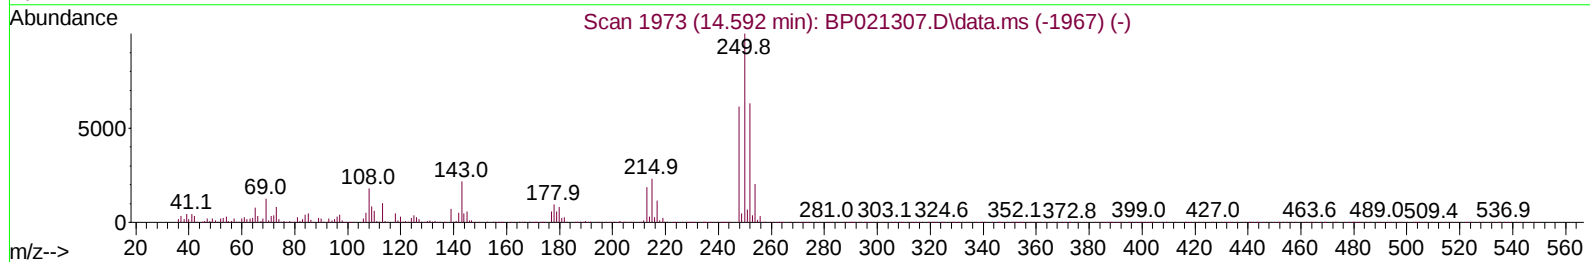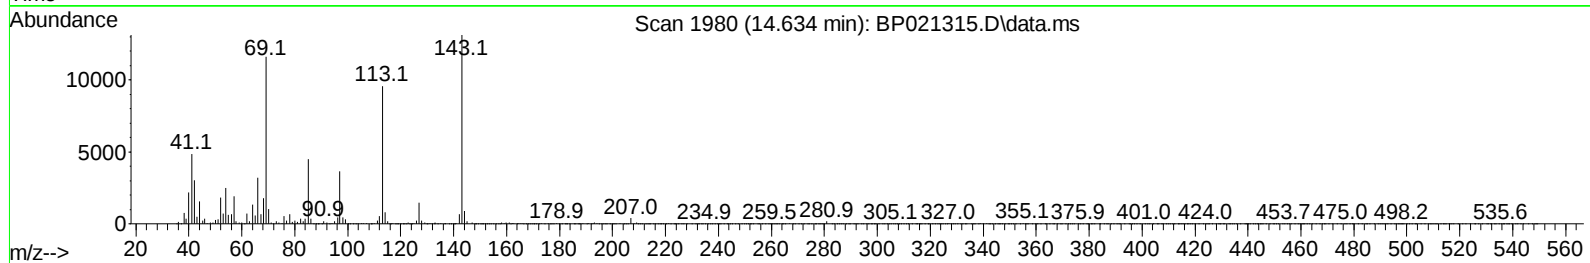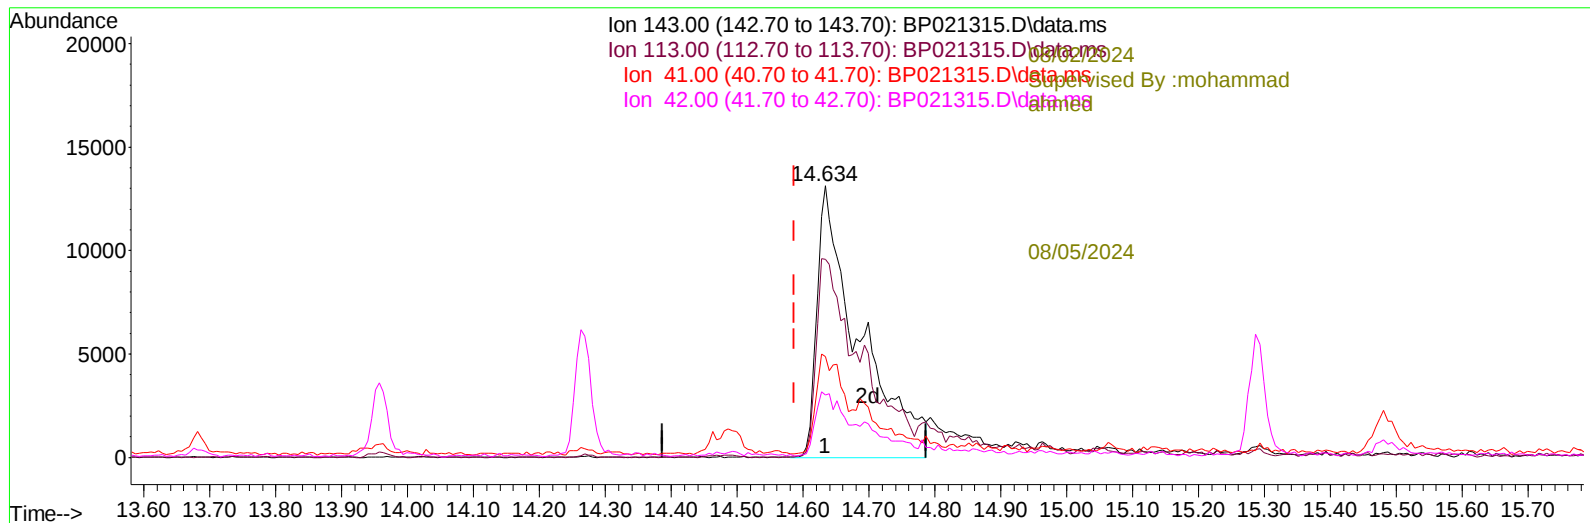

TIC: BP021315.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.634min (+ 0.047) 12.80 ng/ul m

response 57974

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	72.96
41.00	37.90	37.08
42.00	27.10	22.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
 Data File : BP021315.D
 Acq On : 02 Aug 2024 10:17
 Operator : CG/JU
 Sample : P3397-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 02 10:53:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----08/02/2024						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	170631	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	660750	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	437947	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.086	188	988182	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	1048294	20.000	ng/ul	0.00
88) Perylene-d12	24.839	264	1286464	20.000	ng/ul	0.00
-----05/2024						
Supervised By :mohammad ali med						
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	8718	2.325	ng/uL	-0.01
4) Pyridine-d5	3.599	84	49403	4.551	ng/ul	0.00
7) Phenol-d5	6.852	99	171036	12.295	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	102780	12.192	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	157517	13.743	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	150031	12.985	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	72833	14.192	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	84586	14.400	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	145976m	13.743	ng/ul	0.01
31) 4-Chloroaniline-d4	10.569	131	210904	14.988	ng/ul	0.01
46) Dimethylphthalate-d6	13.681	166	537956	16.897	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	578883	16.193	ng/ul	0.00
54) 4-Nitrophenol-d4	14.634	143	57974m	12.799	ng/ul	0.05
60) Fluorene-d10	15.287	176	467450	17.897	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	59710	9.987	ng/ul	0.02
73) Anthracene-d10	17.192	188	773574	17.625	ng/ul	0.00
81) Pyrene-d10	19.575	212	985936	15.213	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.598	264	1186140	18.695	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 02 10:53:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

