

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
 Data File : BP021313.D
 Acq On : 02 Aug 2024 08:49
 Operator : CG/JU
 Sample : P3397-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHCM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	27	31	35	rBV	16259	20539	0.56%	0.067%
2	3.634	108	110	116	rBV3	6507	11381	0.31%	0.037%
3	3.887	149	153	161	rVB	14844	24527	0.67%	0.080%
4	6.852	651	657	673	rBV	233811	553192	15.11%	1.804%
5	6.981	673	679	693	rVB	248778	432217	11.81%	1.409%
6	7.175	707	712	733	rVB	371359	607831	16.61%	1.982%
7	7.616	779	787	803	rBV	584600	1025147	28.01%	3.342%
8	8.358	906	913	936	rBV2	289355	730014	19.94%	2.380%
9	8.787	978	986	999	rBV	271332	547600	14.96%	1.785%
10	9.357	1079	1083	1091	rBV8	4517	10278	0.28%	0.034%
11	9.499	1098	1107	1125	rBV	204521	471293	12.88%	1.537%
12	10.063	1194	1203	1218	rBV	251735	692738	18.93%	2.259%
13	10.393	1251	1259	1273	rBV	822488	1391691	38.02%	4.537%
14	10.557	1280	1287	1313	rBV	242212	634158	17.33%	2.068%
15	11.187	1388	1394	1405	rBV3	16773	49865	1.36%	0.163%
16	11.487	1442	1445	1450	rBV6	1921	4029	0.11%	0.013%
17	11.993	1526	1531	1543	rVB5	6036	14508	0.40%	0.047%
18	13.681	1811	1818	1833	rBV	503810	948953	25.93%	3.094%
19	13.963	1854	1866	1881	rBV	852785	1370223	37.44%	4.467%
20	14.269	1911	1918	1932	rBV	1207642	1868946	51.06%	6.093%
21	14.493	1948	1956	1965	rVB4	31396	69376	1.90%	0.226%
22	14.628	1973	1979	1993	rBV5	62024	269926	7.37%	0.880%
23	14.775	2002	2004	2008	rVB3	7857	9186	0.25%	0.030%
24	15.075	2048	2055	2059	rBV6	3890	8048	0.22%	0.026%
25	15.281	2084	2090	2105	rBV	1026318	1732194	47.33%	5.648%
26	15.475	2118	2123	2132	rBV	117889	251981	6.88%	0.822%
27	15.869	2185	2190	2192	rBV6	3366	5602	0.15%	0.018%
28	16.604	2311	2315	2318	rBV6	3273	5103	0.14%	0.017%
29	16.875	2355	2361	2365	rVB7	4927	11517	0.31%	0.038%
30	17.087	2391	2397	2409	rBV	1544843	2276253	62.19%	7.421%
31	17.192	2409	2415	2430	rVB	1191746	1882496	51.43%	6.138%
32	17.392	2446	2449	2452	rBV5	4603	6525	0.18%	0.021%
33	17.781	2513	2515	2520	rVB3	10082	12016	0.33%	0.039%
34	18.022	2551	2556	2565	rBV3	53480	111258	3.04%	0.363%
35	19.116	2739	2742	2749	rVB4	19195	30496	0.83%	0.099%
36	19.575	2814	2820	2834	rBV	1567838	2592902	70.84%	8.454%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021313.D
Acq On : 02 Aug 2024 08:49
Operator : CG/JU
Sample : P3397-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCM6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	21.186	3089	3094	3103	rBV	218089	374581	10.23%	1.221%
38	21.533	3147	3153	3163	rBV	1790399	2943527	80.42%	9.597%
39	24.592	3665	3673	3692	rVB	1055162	3009060	82.21%	9.811%
40	24.827	3703	3713	3730	rVB2	1218795	3660195	100.00%	11.934%




Sum of corrected areas: 30671372

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021313.D
Acq On : 02 Aug 2024 08:49
Operator : CG/JU
Sample : P3397-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

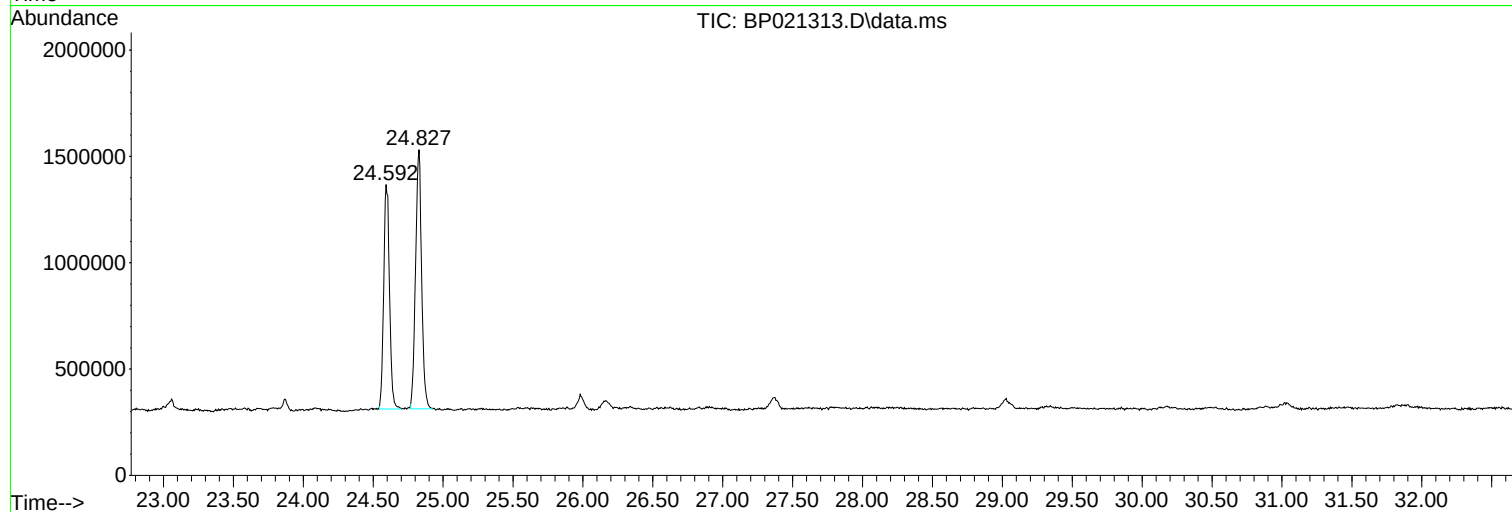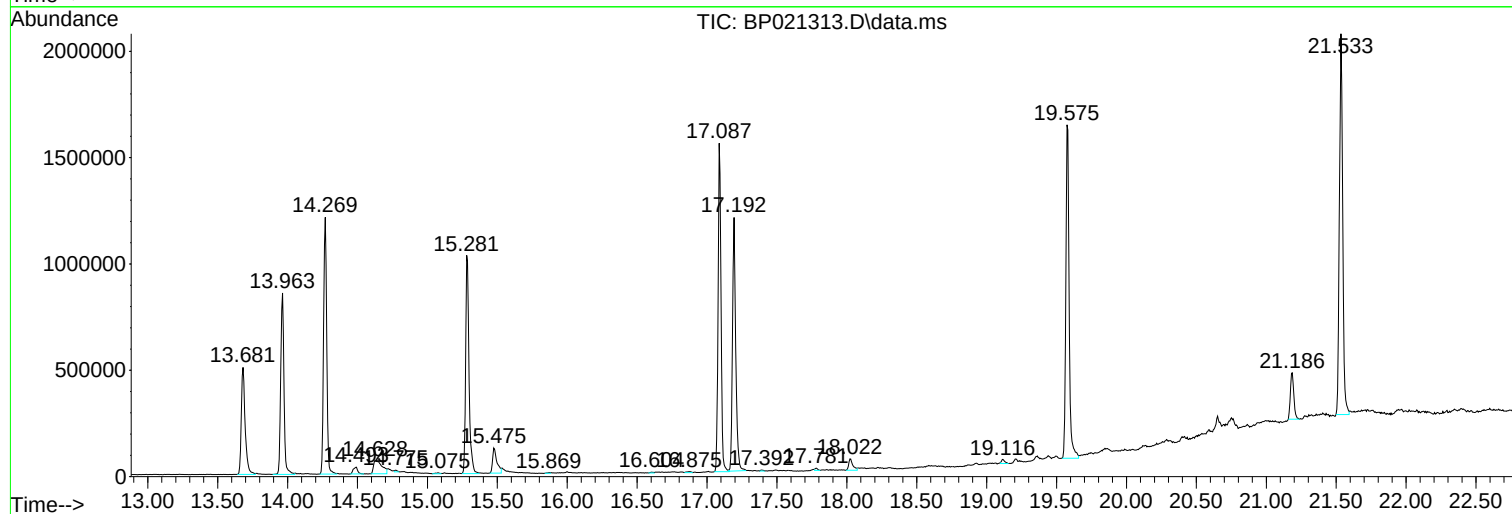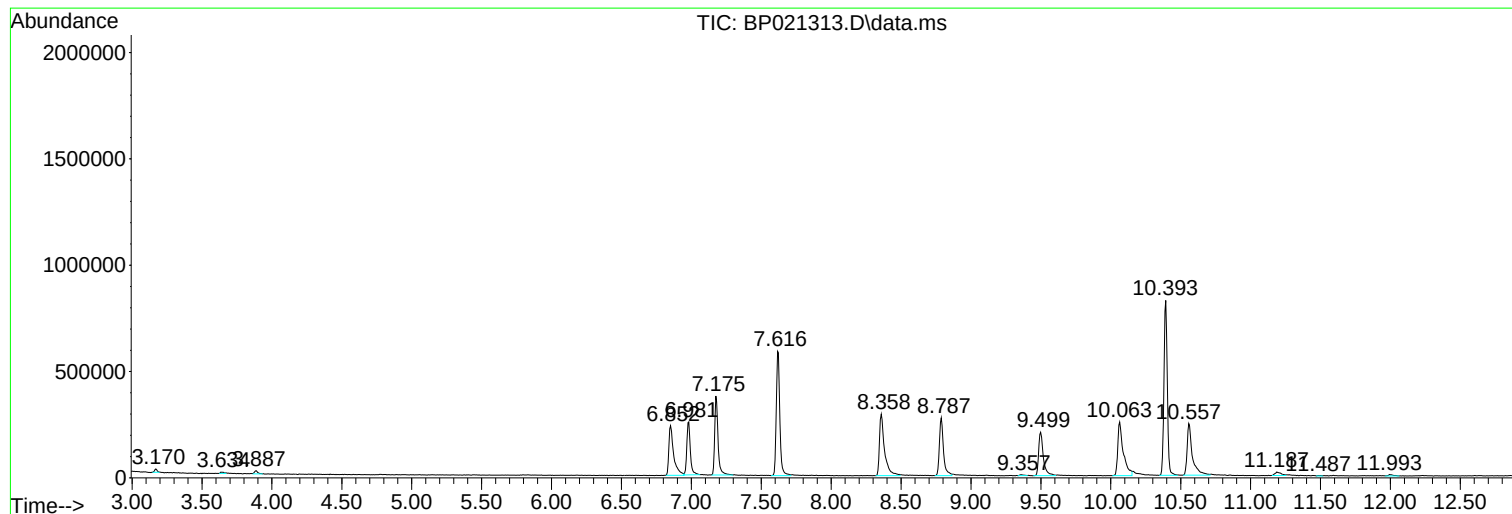

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021313.D
Acq On : 02 Aug 2024 08:49
Operator : CG/JU
Sample : P3397-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCM6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.186	2.55 ng/ul	374581	Chrysene-d12	21.533

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene			364	C26H52	018835-33-1	95
2	n-Tetracosanol-1			354	C24H50O	000506-51-4	95
3	Behenic alcohol			326	C22H46O	000661-19-8	95
4	Pentafluoropropionic acid, penta...			374	C18H31F5O2	959092-08-1	94
5	1-Heneicosyl formate			340	C22H44O2	077899-03-7	94

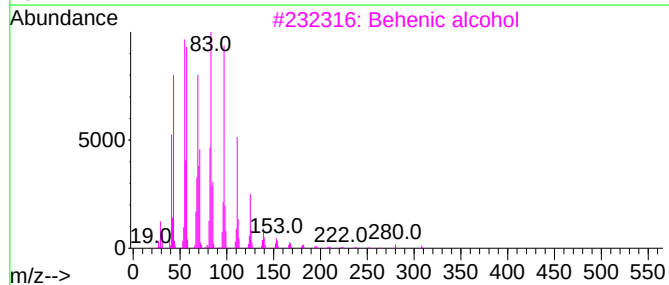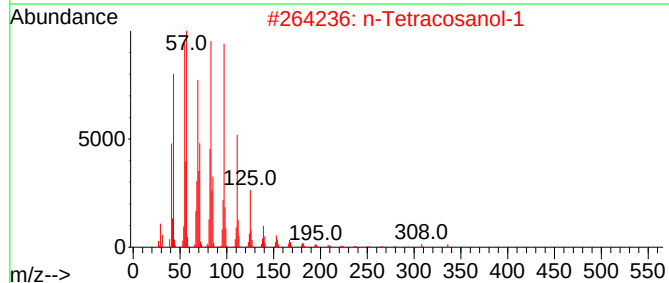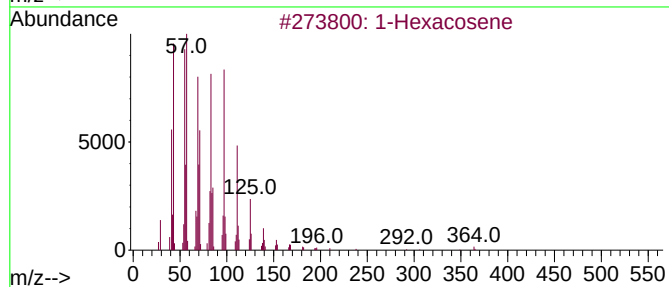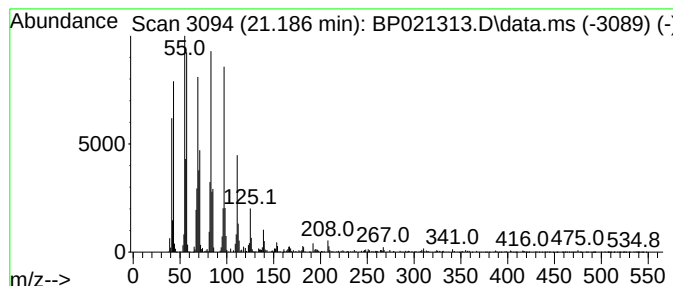

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021313.D
Acq On : 02 Aug 2024 08:49
Operator : CG/JU
Sample : P3397-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.186	2.5	ng/u1	374581	5	21.533	2943530	20.0