

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
 Data File : BP021315.D
 Acq On : 02 Aug 2024 10:17
 Operator : CG/JU
 Sample : P3397-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHCL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	27	30	35	rVB	14950	18910	0.57%	0.064%
2	3.599	102	104	120	rBV	68574	145124	4.39%	0.489%
3	3.887	149	153	157	rVB2	7726	10865	0.33%	0.037%
4	6.852	649	657	673	rBV	182638	486547	14.73%	1.639%
5	6.981	674	679	694	rVB	225141	385054	11.66%	1.297%
6	7.181	705	713	733	rBV	293699	532213	16.11%	1.793%
7	7.628	781	789	810	rBV	547596	991859	30.03%	3.341%
8	8.369	908	915	940	rBV	275086	672061	20.34%	2.264%
9	8.793	978	987	1011	rBV	254445	520226	15.75%	1.753%
10	9.122	1038	1043	1045	rBV6	2705	3909	0.12%	0.013%
11	9.504	1101	1108	1124	rBV	200961	449651	13.61%	1.515%
12	10.063	1196	1203	1224	rBV	200795	646465	19.57%	2.178%
13	10.387	1250	1258	1274	rBV	760682	1335435	40.43%	4.499%
14	10.569	1280	1289	1316	rBV	219863	679428	20.57%	2.289%
15	11.199	1391	1396	1403	rBV4	9291	25536	0.77%	0.086%
16	12.016	1527	1535	1544	rVB7	4814	12601	0.38%	0.042%
17	12.581	1627	1631	1635	rBV7	1838	3358	0.10%	0.011%
18	12.845	1672	1676	1682	rVB6	3900	5873	0.18%	0.020%
19	13.681	1812	1818	1831	rBV	774407	1105497	33.47%	3.724%
20	13.957	1856	1865	1892	rBV	785496	1327862	40.20%	4.473%
21	14.269	1911	1918	1928	rBV	1125621	1827210	55.31%	6.156%
22	14.487	1946	1955	1966	rVB3	23688	68071	2.06%	0.229%
23	14.634	1974	1980	1987	rBV2	80168	227280	6.88%	0.766%
24	14.969	2034	2037	2041	rVB6	3094	4472	0.14%	0.015%
25	15.063	2048	2053	2057	rVV2	7347	10927	0.33%	0.037%
26	15.128	2060	2064	2069	rVV8	4974	8655	0.26%	0.029%
27	15.287	2084	2091	2114	rBV	982472	1710754	51.79%	5.763%
28	15.481	2117	2124	2138	rBV2	157496	381183	11.54%	1.284%
29	16.010	2210	2214	2216	rBV5	4085	5300	0.16%	0.018%
30	16.498	2295	2297	2301	rBV4	2443	3583	0.11%	0.012%
31	16.839	2349	2355	2357	rBV7	4551	7937	0.24%	0.027%
32	16.881	2360	2362	2368	rVB5	6158	8069	0.24%	0.027%
33	16.981	2376	2379	2381	rBV4	3010	4095	0.12%	0.014%
34	17.086	2390	2397	2408	rBV	1454350	2301318	69.67%	7.753%
35	17.192	2409	2415	2429	rVV2	1190093	1906586	57.72%	6.423%
36	17.381	2443	2447	2450	rVB3	6415	8308	0.25%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	17.769	2510	2513	2517	rVB5	9568	12785	0.39%	0.043%
38	18.016	2550	2555	2565	rBV2	91168	178728	5.41%	0.602%
39	19.122	2738	2743	2747	rBV4	22464	41339	1.25%	0.139%
40	19.351	2778	2782	2788	rBV5	27840	47344	1.43%	0.159%
41	19.575	2815	2820	2831	rBV	1622674	2459968	74.47%	8.287%
42	21.180	3090	3093	3105	rVB2	183301	271883	8.23%	0.916%
43	21.533	3148	3153	3166	rBV2	1545281	2802312	84.83%	9.441%
44	24.598	3667	3674	3691	rVB	934257	2723710	82.45%	9.176%
45	24.839	3706	3715	3733	rVB	1133352	3303326	100.00%	11.128%




Sum of corrected areas: 29683617

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

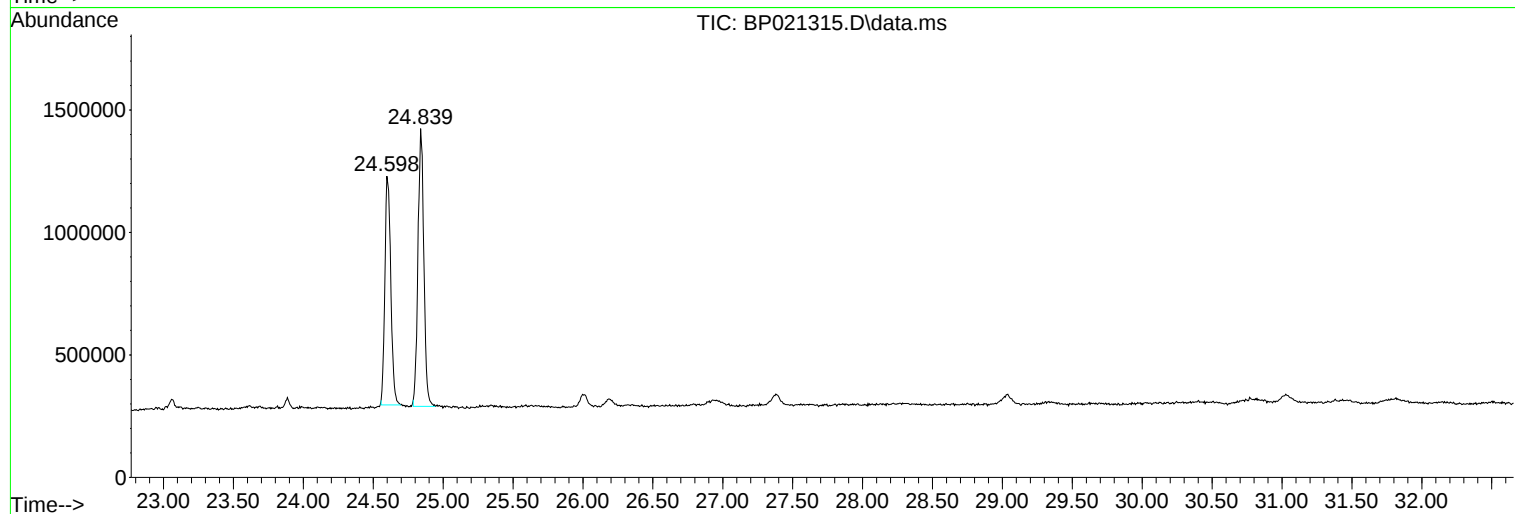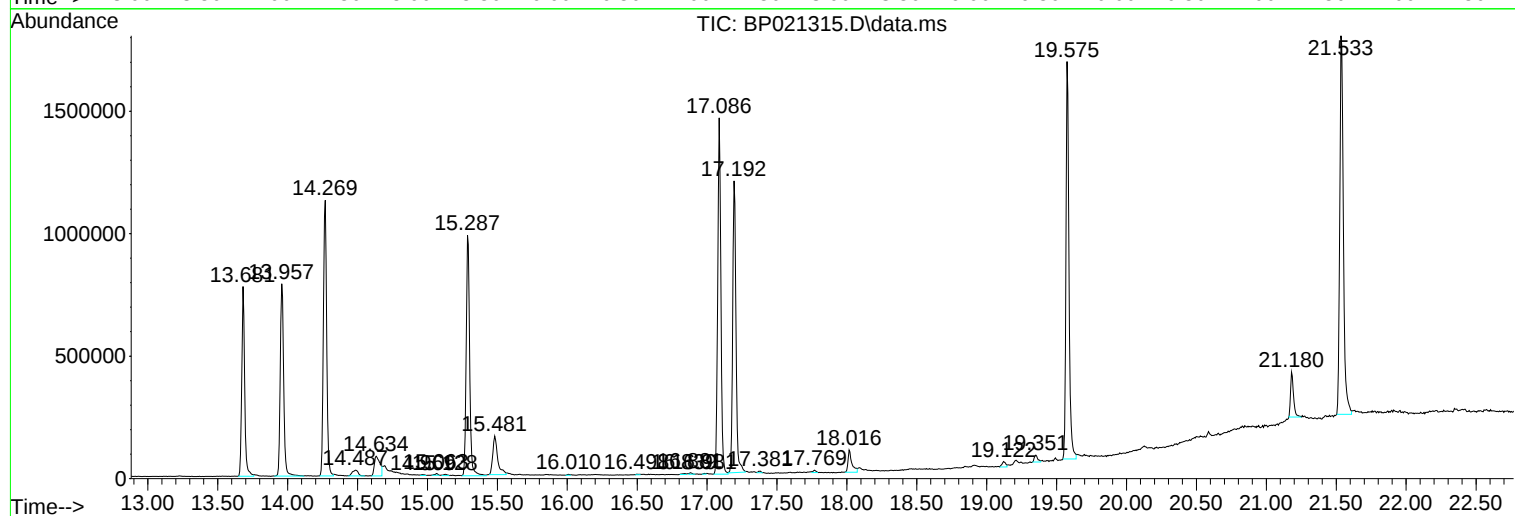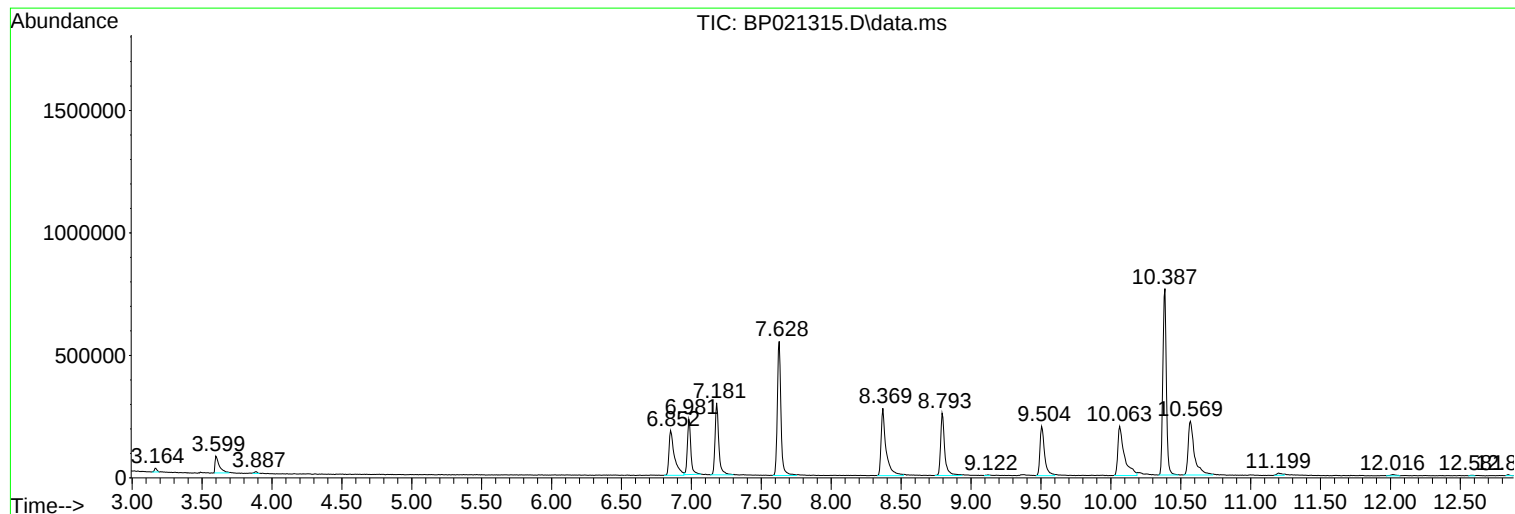

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021315.D
Acq On : 02 Aug 2024 10:17
Operator : CG/JU
Sample : P3397-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHCL0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------