

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
 Data File : BP021321.D
 Acq On : 02 Aug 2024 14:46
 Operator : CG/JU
 Sample : PB162171BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK171

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	38	rVB	37510	54572	1.67%	0.166%
2	3.581	99	101	124	rBV	403583	734659	22.47%	2.234%
3	3.875	148	151	157	rVB	12163	17307	0.53%	0.053%
4	6.840	649	655	672	rBV2	336427	880482	26.93%	2.677%
5	6.975	672	678	692	rVB	405104	683786	20.92%	2.079%
6	7.169	705	711	730	rBV	479402	920902	28.17%	2.800%
7	7.622	780	788	801	rBV	496190	954636	29.20%	2.903%
8	8.357	906	913	939	rBV	400284	1126413	34.45%	3.425%
9	8.787	979	986	1003	rBV	435455	859447	26.29%	2.613%
10	9.505	1098	1108	1131	rBV	311014	744902	22.79%	2.265%
11	10.057	1194	1202	1223	rBV	312614	997297	30.51%	3.033%
12	10.381	1250	1257	1273	rBV	724378	1294153	39.59%	3.935%
13	10.563	1281	1288	1308	rBV	306165	1017285	31.12%	3.093%
14	12.040	1532	1539	1544	rBV5	6469	15806	0.48%	0.048%
15	12.346	1588	1591	1597	rBV7	1521	3321	0.10%	0.010%
16	13.687	1812	1819	1832	rBV	882701	1459965	44.66%	4.440%
17	13.857	1846	1848	1854	rVB7	2121	3453	0.11%	0.010%
18	13.957	1858	1865	1885	rBV	1039375	1811162	55.40%	5.507%
19	14.263	1910	1917	1933	rBV	934680	1664713	50.92%	5.062%
20	14.634	1972	1980	1987	rBV2	114354	331768	10.15%	1.009%
21	15.281	2083	2090	2111	rBV	1174222	2242631	68.60%	6.819%
22	15.481	2116	2124	2142	rBV2	175402	599852	18.35%	1.824%
23	16.092	2223	2228	2234	rVB9	5450	11972	0.37%	0.036%
24	16.886	2358	2363	2364	rBV5	2986	4181	0.13%	0.013%
25	17.081	2389	2396	2406	rBV	1090814	1657590	50.70%	5.040%
26	17.192	2408	2415	2436	rVB	1155867	2100824	64.26%	6.388%
27	17.775	2511	2514	2518	rBV6	3249	4934	0.15%	0.015%
28	18.045	2554	2560	2562	rBV7	7019	13049	0.40%	0.040%
29	19.122	2739	2743	2748	rVB5	20869	32247	0.99%	0.098%
30	19.580	2815	2821	2833	rBV	1806877	2748681	84.08%	8.358%
31	21.545	3149	3155	3170	rBV	1077407	2073898	63.44%	6.306%
32	24.598	3666	3674	3695	rVB2	1157791	3269238	100.00%	9.941%
33	24.839	3707	3715	3735	rVB	838357	2550618	78.02%	7.756%




Sum of corrected areas: 32885744

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021321.D
Acq On : 02 Aug 2024 14:46
Operator : CG/JU
Sample : PB162171BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

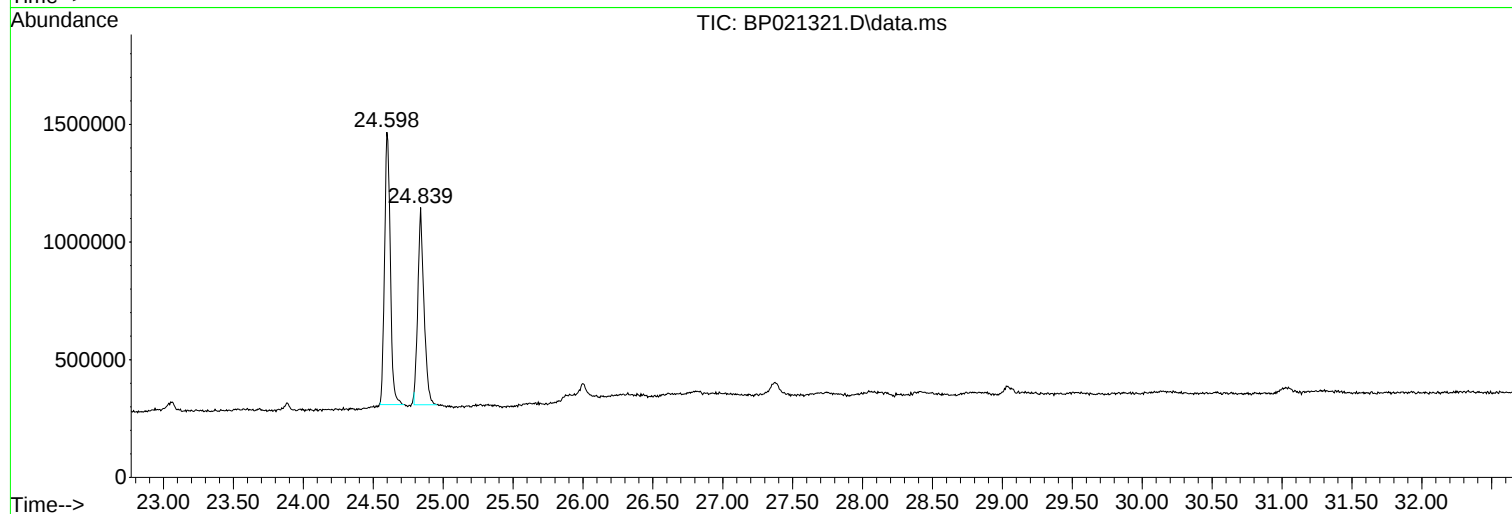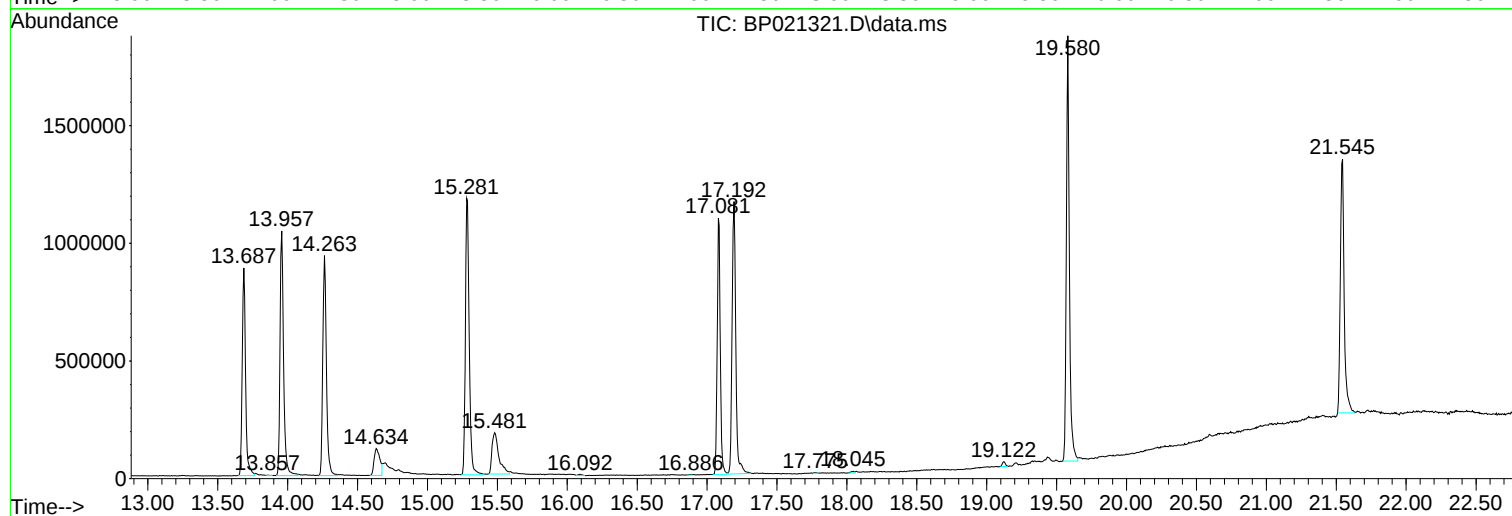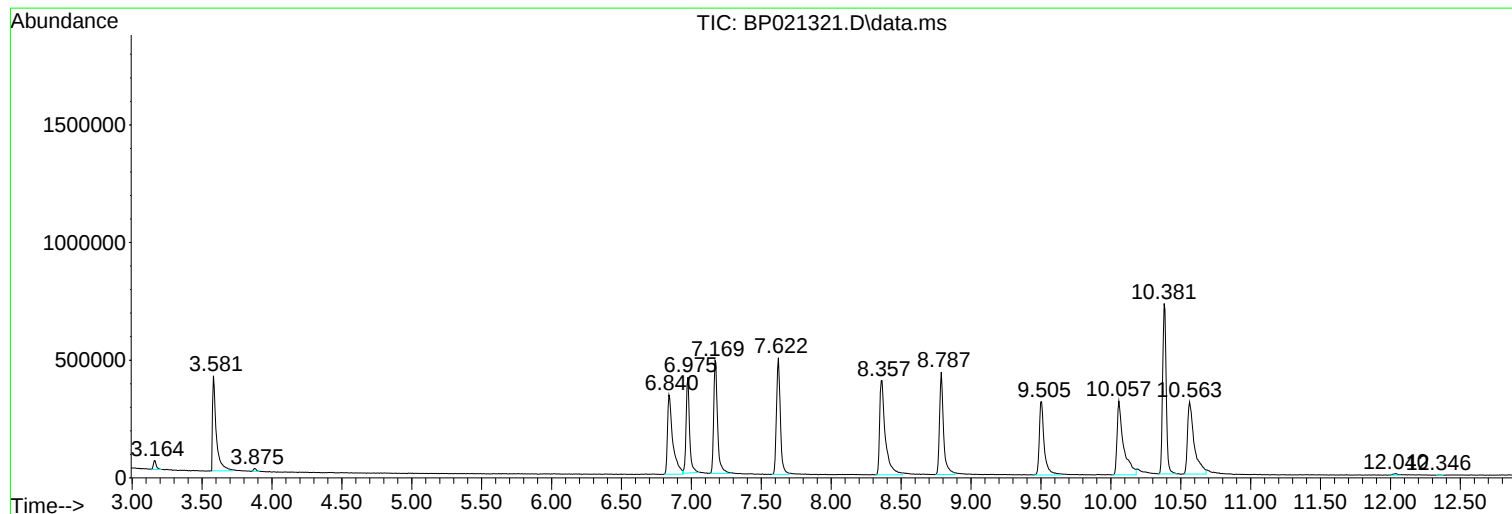

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021321.D
Acq On : 02 Aug 2024 14:46
Operator : CG/JU
Sample : PB162171BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080124\
Data File : BP021321.D
Acq On : 02 Aug 2024 14:46
Operator : CG/JU
Sample : PB162171BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK171

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc