

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080822\
 Data File : BP011313.D
 Acq On : 08 Aug 2022 16:16
 Operator : CG/JU
 Sample : SSTD02040
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020640

Quant Time: Aug 08 17:11:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 17:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	167379	20.000	ng/u1	0.00
20) Naphthalene-d8	10.381	136	718285	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.263	164	397334	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.039	188	787195	20.000	ng/u1	0.00
79) Chrysene-d12	21.169	240	739120	20.000	ng/u1	0.00
88) Perylene-d12	23.474	264	720209	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	108	0.052	ng/uL	0.12
4) Pyridine-d5	3.499	84	294792	52.794	ng/u1	0.00
7) Phenol-d5	6.775	99	314027	22.513	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	228122	22.664	ng/u1	0.00
11) 2-Chlorophenol-d4	7.122	132	257039	22.608	ng/u1	0.00
15) 4-Methylphenol-d8	8.316	113	244428	21.296	ng/u1	0.00
21) Nitrobenzene-d5	8.757	128	107434	20.795	ng/u1	0.00
24) 2-Nitrophenol-d4	9.475	143	96277	19.880	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.010	165	202258	21.901	ng/u1	0.00
31) 4-Chloroaniline-d4	10.534	131	346636	24.262	ng/u1	0.00
46) Dimethylphthalate-d6	13.687	166	607609	22.328	ng/u1	0.00
49) Acenaphthylene-d8	13.957	160	748241	21.853	ng/u1	0.00
54) 4-Nitrophenol-d4	14.492	143	99919	21.592	ng/u1	0.00
60) Fluorene-d10	15.269	176	519282	22.426	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	68281	18.680	ng/u1	0.00
73) Anthracene-d10	17.139	188	782070	22.605	ng/u1	0.00
81) Pyrene-d10	19.398	212	877668	23.486	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.327	264	797032	22.208	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.122	88	50484	26.442	ng/uL#	82
5) Pyridine	3.517	79	308769	54.609	ng/u1#	88
6) Benzaldehyde	6.746	77	73940	10.844	ng/u1	96
8) Phenol	6.799	94	342483	22.898	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.028	93	280771	22.877	ng/u1	97
12) 2-Chlorophenol	7.158	128	268614	22.746	ng/u1	98
13) 2-Methylphenol	8.046	108	244727	21.625	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.134	45	424730	20.309	ng/u1	96
16) Acetophenone	8.422	105	409578	22.020	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.410	70	208002	22.982	ng/u1	95
18) 4-Methylphenol	8.375	108	267137	22.010	ng/u1	99
19) Hexachloroethane	8.657	117	113574	20.055	ng/u1	98
22) Nitrobenzene	8.799	77	306117	21.621	ng/u1	97
23) Isophorone	9.328	82	558227	22.158	ng/u1	99
25) 2-Nitrophenol	9.504	139	116031	20.705	ng/u1	94
26) 2,4-Dimethylphenol	9.575	107	292967	23.108	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.816	93	353164	22.266	ng/u1	98
29) 2,4-Dichlorophenol	10.034	162	207485	21.498	ng/u1	98
30) Naphthalene	10.434	128	851503	22.456	ng/u1	99
32) 4-Chloroaniline	10.557	127	349654	24.163	ng/u1	99
33) Hexachlorobutadiene	10.716	225	125966	20.895	ng/u1	98
34) Caprolactam	11.351	113	63946	22.369	ng/u1	91
35) 4-Chloro-3-methylphenol	11.698	107	252473	23.132	ng/u1	99
36) 2-Methylnaphthalene	12.057	142	531034	22.413	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080822\
 Data File : BP011313.D
 Acq On : 08 Aug 2022 16:16
 Operator : CG/JU
 Sample : SSTD02040
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020640

Quant Time: Aug 08 17:11:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 17:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.281	142	541898	22.768	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.434	216	225491	20.751	ng/ul	99
40) Hexachlorocyclopentadiene	12.404	237	106492	15.511	ng/ul	99
41) 2,4,6-Trichlorophenol	12.687	196	140088	20.578	ng/ul	100
42) 2,4,5-Trichlorophenol	12.757	196	153366	20.993	ng/ul	97
43) 1,1'-Biphenyl	13.093	154	675259	21.294	ng/ul	100
44) 2-Chloronaphthalene	13.128	162	509113	21.521	ng/ul	97
45) 2-Nitroaniline	13.351	65	127818	22.462	ng/ul	95
47) Dimethylphthalate	13.734	163	616877	22.470	ng/ul	100
48) 2,6-Dinitrotoluene	13.857	165	97338	23.620	ng/ul	96
50) Acenaphthylene	13.981	152	853567	22.062	ng/ul	99
51) 3-Nitroaniline	14.187	138	70453	15.500	ng/ul	98
52) Acenaphthene	14.328	153	554713	22.166	ng/ul	98
53) 2,4-Dinitrophenol	14.398	184	44867	18.334	ng/ul	97
55) 4-Nitrophenol	14.504	109	94267	22.572	ng/ul	92
56) Dibenzofuran	14.669	168	762018	22.251	ng/ul	100
57) 2,4-Dinitrotoluene	14.651	165	152047	23.428	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	14.898	232	116401	21.101	ng/ul	96
59) Diethylphthalate	15.116	149	636088	22.451	ng/ul	99
61) Fluorene	15.322	166	613855	22.497	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.328	204	267299	22.183	ng/ul	95
63) 4-Nitroaniline	15.363	138	44362	11.665	ng/ul	91
66) 4,6-Dinitro-2-methylph...	15.416	198	73500	19.446	ng/ul#	97
67) N-Nitrosodiphenylamine	15.545	169	520315	22.614	ng/ul	99
68) 4-Bromophenyl-phenylether	16.228	248	151550	21.341	ng/ul	96
69) Hexachlorobenzene	16.328	284	174959	21.092	ng/ul	93
70) Atrazine	16.516	200	161086	23.404	ng/ul	98
71) Pentachlorophenol	16.686	266	94594	19.470	ng/ul	98
72) Phenanthrene	17.081	178	955994	22.182	ng/ul	100
74) Anthracene	17.169	178	966860	22.557	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.051	216	232937	19.336	ng/uL	99
76) Pentachlorobenzene	14.581	250	212509	20.694	ng/uL	99
77) Carbazole	17.451	167	894383	23.266	ng/ul	100
78) Di-n-butylphthalate	18.028	149	962933	20.193	ng/ul	99
80) Fluoranthene	19.069	202	1057677	23.142	ng/ul	98
82) Pyrene	19.427	202	1113207	23.341	ng/ul	98
83) Butylbenzylphthalate	20.327	149	347790	19.098	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.098	252	248613	20.566	ng/ul	99
85) Benzo(a)anthracene	21.151	228	1022312	22.130	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.092	149	541779	17.411	ng/ul	99
87) Chrysene	21.204	228	1020619	22.446	ng/ul	99
89) Di-n-octyl phthalate	21.998	149	927810	18.894	ng/ul	100
90) Benzo(b)fluoranthene	22.774	252	1024268	22.323	ng/ul	99
91) Benzo(k)fluoranthene	22.821	252	999981	23.230	ng/ul	99
93) Benzo(a)pyrene	23.374	252	996844	22.318	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.857	276	1091474	20.476	ng/ul	98
95) Dibenzo(a,h)anthracene	25.886	278	921789	20.393	ng/ul	97
96) Benzo(g,h,i)perylene	26.592	276	927865	20.313	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
 1,4-Dioxane
 Concen: 26.442 ng/uL
 RT: 3.122 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020640


Tgt Ion: 88 Resp: 50484
 Ion Ratio Lower Upper
 88 100
 43 32.7 29.6 44.4
 58 79.9 49.1 73.7#

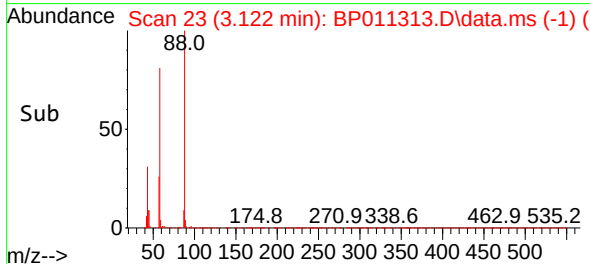

#5
 Pyridine
 Concen: 54.609 ng/uL
 RT: 3.517 min Scan# 90
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16

Tgt Ion: 79 Resp: 308769
 Ion Ratio Lower Upper
 79 100
 52 87.5 57.8 86.6#
 51 40.1 31.5 47.3


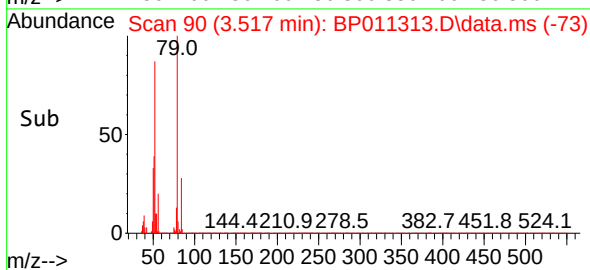

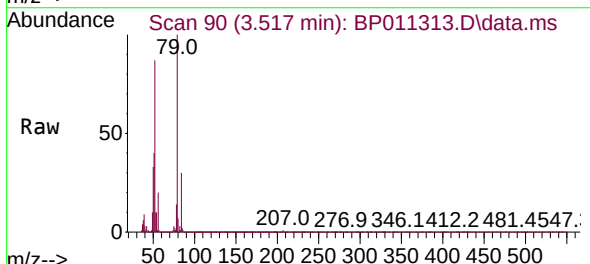




#6
Benzaldehyde
Concen: 10.844 ng/ul
RT: 6.746 min Scan# 611
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion: 77 Resp: 73940
Ion Ratio Lower Upper
77 100
105 95.9 72.0 108.0
106 87.9 69.4 104.0



#8
Phenol
Concen: 22.898 ng/ul
RT: 6.799 min Scan# 648
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion: 94 Resp: 342483
Ion Ratio Lower Upper
94 100
65 31.9 24.7 37.1
66 41.0 32.6 49.0









#10
 Bis(2-Chloroethyl)ether
 Concen: 22.877 ng/ul
 RT: 7.028 min Scan# 687
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020640

Tgt Ion: 93 Resp: 280771




Ion	Ratio	Lower	Upper
93	100		
63	84.7	71.0	106.6
95	32.0	26.0	39.0




#12
 2-Chlorophenol
 Concen: 22.746 ng/ul
 RT: 7.158 min Scan# 709
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16

Tgt Ion: 128 Resp: 268614

Ion	Ratio	Lower	Upper
128	100		
64	52.9	43.8	65.6
130	33.1	25.4	38.2









#13
2-Methylphenol
Concen: 21.625 ng/ul
RT: 8.046 min Scan# 860
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:108 Resp: 244727
Ion Ratio Lower Upper
108 100
107 89.2 71.8 107.6



#14
2,2'-oxybis(1-Chloropropane)
Concen: 20.309 ng/ul
RT: 8.134 min Scan# 875
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion: 45 Resp: 424730
Ion Ratio Lower Upper
45 100
77 13.8 9.9 14.9
79 10.6 7.2 10.8









#16
Acetophenone
Concen: 22.020 ng/ul
RT: 8.422 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:105 Resp: 409578
Ion Ratio Lower Upper
105 100
77 82.1 65.4 98.0
51 31.5 26.5 39.7



#17
N-Nitroso-di-n-propylamine
Concen: 22.982 ng/ul
RT: 8.410 min Scan# 922
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion: 70 Resp: 208002
Ion Ratio Lower Upper
70 100
42 64.1 55.5 83.3
101 9.2 7.1 10.7
130 18.9 14.8 22.2


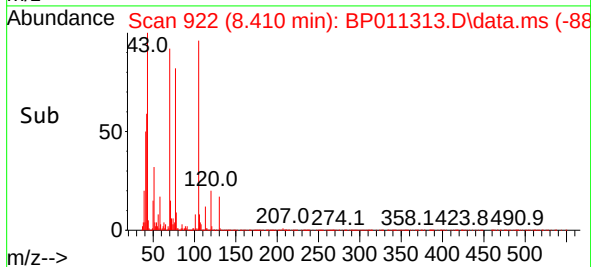

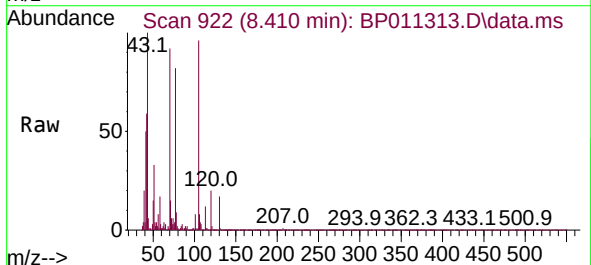




#18
4-Methylphenol
Concen: 22.010 ng/ul
RT: 8.375 min Scan# 916
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:108 Resp: 267137
Ion Ratio Lower Upper
108 100
107 109.1 88.2 132.4



#19
Hexachloroethane
Concen: 20.055 ng/ul
RT: 8.657 min Scan# 964
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:117 Resp: 113574
Ion Ratio Lower Upper
117 100
201 76.7 62.2 93.2
199 48.2 39.8 59.6



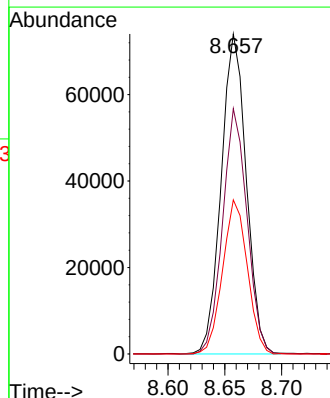





#22
Nitrobenzene
Concen: 21.621 ng/ul
RT: 8.799 min Scan# 988
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion: 77 Resp: 306117
Ion Ratio Lower Upper
77 100
123 41.1 31.4 47.0
65 14.4 10.6 15.8



#23
Isophorone
Concen: 22.158 ng/ul
RT: 9.328 min Scan# 1078
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion: 82 Resp: 558227
Ion Ratio Lower Upper
82 100
95 7.3 5.8 8.8
138 16.2 12.6 18.8









#25
2-Nitrophenol
Concen: 20.705 ng/ul
RT: 9.504 min Scan# 1108
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:139 Resp: 116031
Ion Ratio Lower Upper
139 100
65 62.7 46.7 70.1
109 33.3 24.2 36.2



#26
2,4-Dimethylphenol
Concen: 23.108 ng/ul
RT: 9.575 min Scan# 1120
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:107 Resp: 292967
Ion Ratio Lower Upper
107 100
121 49.4 40.3 60.5
122 83.4 67.7 101.5





#27

Bis(2-Chloroethoxy)methane

Concen: 22.266 ng/ul

RT: 9.816 min Scan# 1161

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Instrument :

BNA_P

ClientSampleId :

SSTD020640





Tgt Ion: 93 Resp: 353164

Ion Ratio Lower Upper

93 100

95 32.7 25.2 37.8

123 11.0 8.4 12.6



#29

2,4-Dichlorophenol

Concen: 21.498 ng/ul

RT: 10.034 min Scan# 1198

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16




Tgt Ion:162 Resp: 207485


Ion Ratio Lower Upper

162 100

164 64.0 52.6 79.0

98 44.0 34.2 51.4


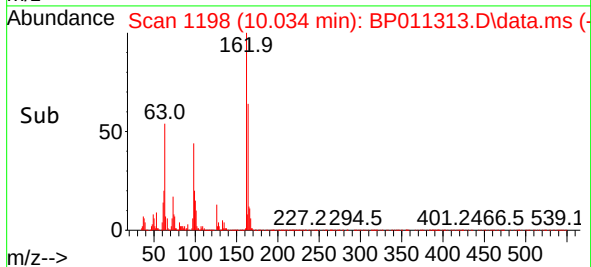

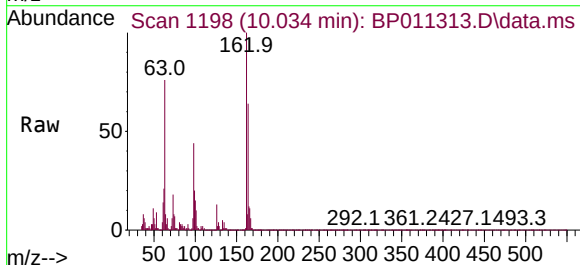




#30
Naphthalene
Concen: 22.456 ng/ul
RT: 10.434 min Scan# 1266
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:128 Resp: 851503
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.4
127 12.9 10.4 15.6

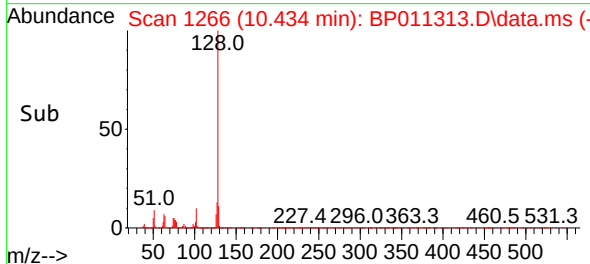

#32
4-Chloroaniline
Concen: 24.163 ng/ul
RT: 10.557 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:127 Resp: 349654
Ion Ratio Lower Upper
127 100
129 32.9 26.6 40.0

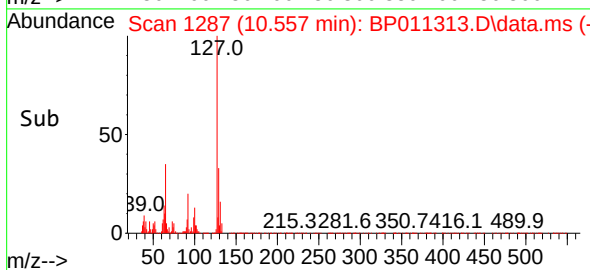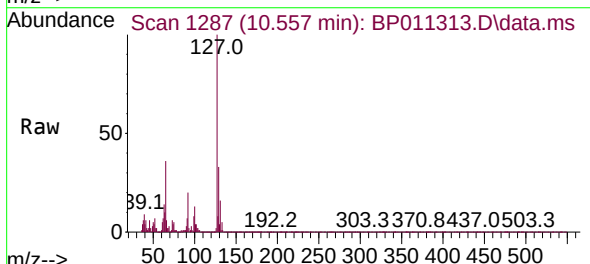



#33

Hexachlorobutadiene

Concen: 20.895 ng/ul

RT: 10.716 min Scan# 1314

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Instrument :

BNA_P

ClientSampleId :

SSTD020640





Tgt Ion:225 Resp: 125966

Ion Ratio Lower Upper

225 100

223 61.1 51.2 76.8

227 62.4 50.6 75.8

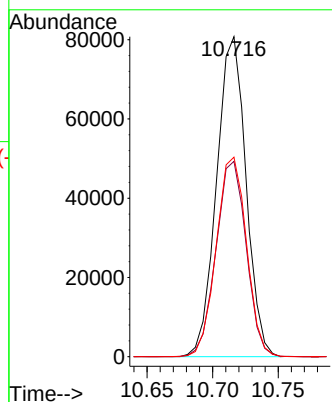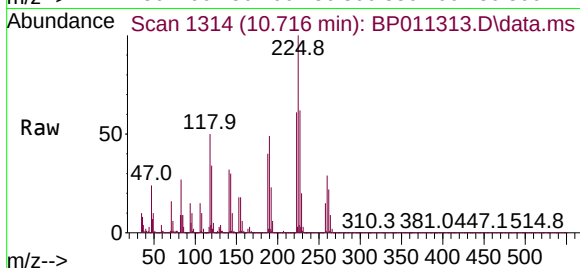

#34

Caprolactam

Concen: 22.369 ng/ul

RT: 11.351 min Scan# 1422

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16




Tgt Ion:113 Resp: 63946


Ion Ratio Lower Upper

113 100

55 195.6 164.2 246.4

56 142.5 127.0 190.6









#35
4-Chloro-3-methylphenol
Concen: 23.132 ng/ul
RT: 11.698 min Scan# 1481
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:107 Resp: 252473
Ion Ratio Lower Upper
107 100
144 24.4 19.0 28.4
142 75.2 59.8 89.8

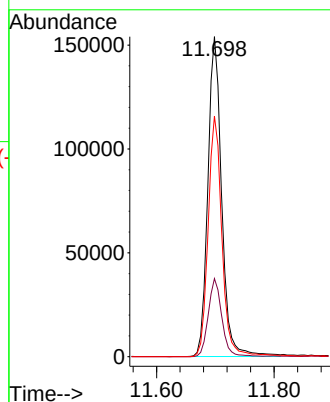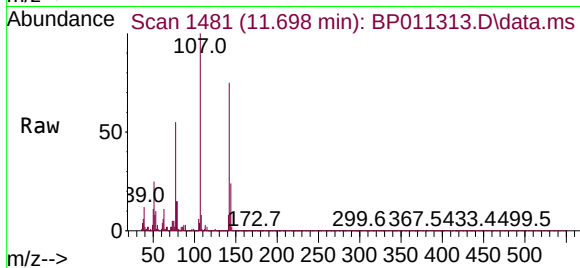

#36
2-Methylnaphthalene
Concen: 22.413 ng/ul
RT: 12.057 min Scan# 1542
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:142 Resp: 531034
Ion Ratio Lower Upper
142 100
141 88.4 71.8 107.8









#37
1-Methylnaphthalene
Concen: 22.768 ng/ul
RT: 12.281 min Scan# 1580
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:142 Resp: 541898
Ion Ratio Lower Upper
142 100
141 92.3 74.1 111.1
116 4.1 3.4 5.0



#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.751 ng/ul
RT: 12.434 min Scan# 1606
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:216 Resp: 225491
Ion Ratio Lower Upper
216 100
214 76.8 61.1 91.7
179 23.3 18.6 27.8
108 24.4 19.1 28.7

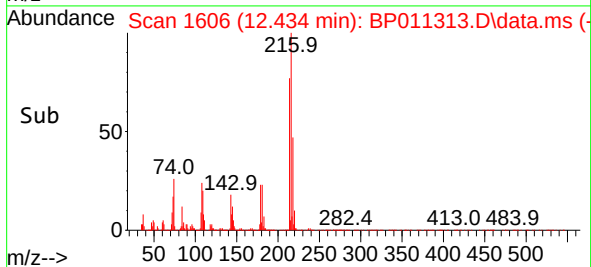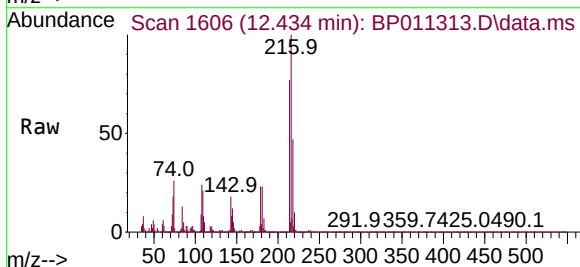



#40

Hexachlorocyclopentadiene

Concen: 15.511 ng/ul

RT: 12.404 min Scan# 1601

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Instrument :

BNA_P

ClientSampleId :

SSTD020640





Tgt Ion:237 Resp: 106492

Ion Ratio Lower Upper

237 100

235 62.7 50.4 75.6

272 12.1 9.9 14.9

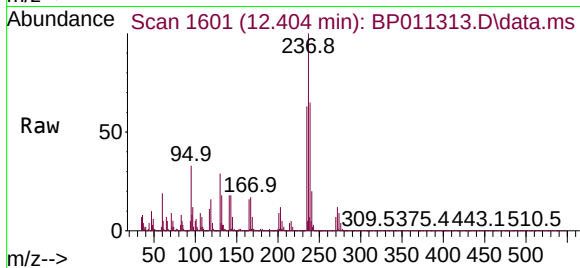

#41

2,4,6-Trichlorophenol

Concen: 20.578 ng/ul

RT: 12.687 min Scan# 1649

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16




Tgt Ion:196 Resp: 140088


Ion Ratio Lower Upper

196 100

198 94.9 75.5 113.3

200 30.6 24.4 36.6



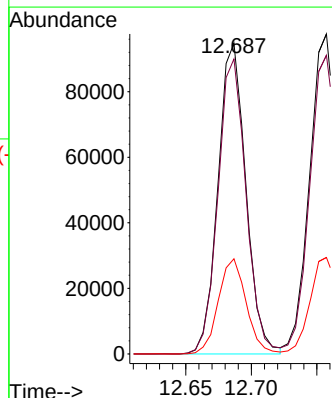





#42
2,4,5-Trichlorophenol
Concen: 20.993 ng/ul
RT: 12.757 min Scan# 1661
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:196 Resp: 153366
Ion Ratio Lower Upper
196 100
198 93.4 76.8 115.2
200 30.1 25.0 37.6

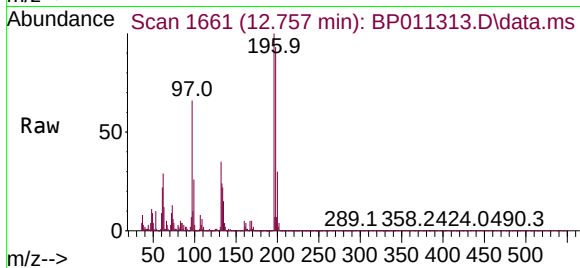

#43
1,1'-Biphenyl
Concen: 21.294 ng/ul
RT: 13.093 min Scan# 1718
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:154 Resp: 675259
Ion Ratio Lower Upper
154 100
153 39.8 31.9 47.9
76 15.2 12.2 18.2


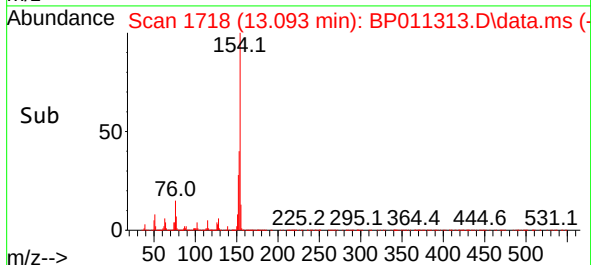

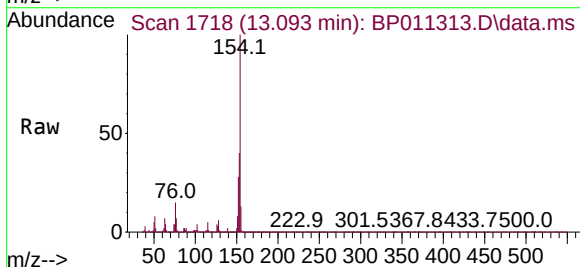




#44
2-Chloronaphthalene
Concen: 21.521 ng/ul
RT: 13.128 min Scan# 1724
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:162 Resp: 509113
Ion Ratio Lower Upper
162 100
164 33.0 25.6 38.4
127 46.0 34.6 51.8

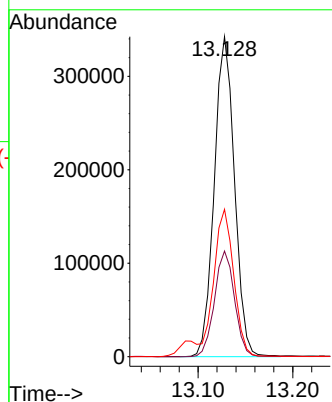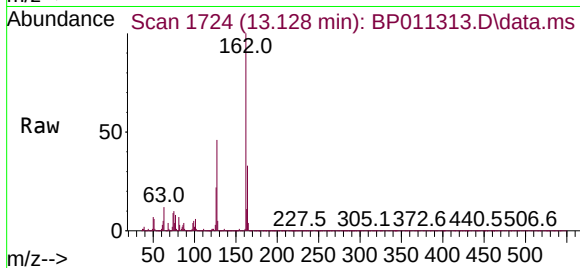

#45
2-Nitroaniline
Concen: 22.462 ng/ul
RT: 13.351 min Scan# 1762
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion: 65 Resp: 127818
Ion Ratio Lower Upper
65 100
92 64.9 51.4 77.2
138 91.3 67.4 101.0


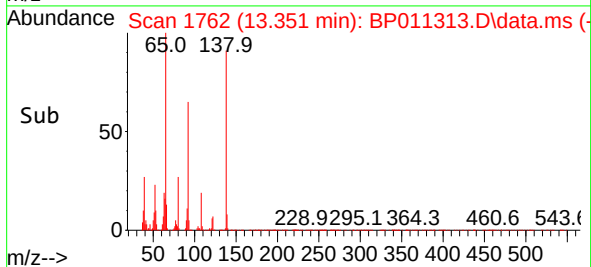
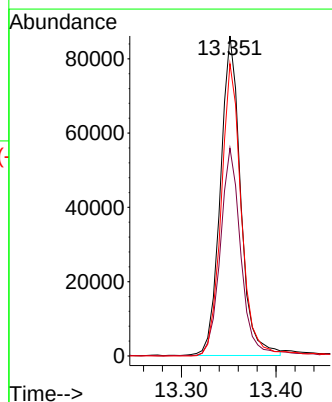
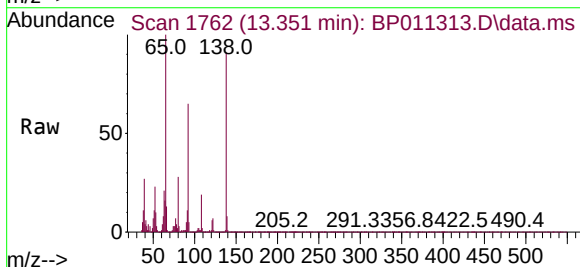




#47
Dimethylphthalate
Concen: 22.470 ng/ul
RT: 13.734 min Scan# 1827
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:163 Resp: 616877
Ion Ratio Lower Upper
163 100
194 3.6 2.9 4.3
164 10.1 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 23.620 ng/ul
RT: 13.857 min Scan# 1848
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:165 Resp: 97338
Ion Ratio Lower Upper
165 100
89 78.2 65.8 98.6
121 29.0 24.2 36.2









#50
Acenaphthylene
Concen: 22.062 ng/ul
RT: 13.981 min Scan# 1869
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:152 Resp: 853567
Ion Ratio Lower Upper
152 100
151 20.2 15.8 23.8
153 12.9 10.5 15.7



#51
3-Nitroaniline
Concen: 15.500 ng/ul
RT: 14.187 min Scan# 1904
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:138 Resp: 70453
Ion Ratio Lower Upper
138 100
108 14.5 9.9 14.9
92 135.8 106.8 160.2









#52
Acenaphthene
Concen: 22.166 ng/ul
RT: 14.328 min Scan# 1928
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:153 Resp: 554713
Ion Ratio Lower Upper
153 100
152 49.3 39.5 59.3
154 88.5 68.6 103.0



#53
2,4-Dinitrophenol
Concen: 18.334 ng/ul
RT: 14.398 min Scan# 1940
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:184 Resp: 44867
Ion Ratio Lower Upper
184 100
63 93.9 75.0 112.6
154 71.8 53.1 79.7









#55
4-Nitrophenol
Concen: 22.572 ng/ul
RT: 14.504 min Scan# 1958
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:109 Resp: 94267
Ion Ratio Lower Upper
109 100
139 117.9 100.6 150.8
65 142.0 122.6 184.0



#56
Dibenzofuran
Concen: 22.251 ng/ul
RT: 14.669 min Scan# 1986
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:168 Resp: 762018
Ion Ratio Lower Upper
168 100
139 42.8 34.2 51.2









#57
2,4-Dinitrotoluene
Concen: 23.428 ng/ul
RT: 14.651 min Scan# 1983
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:165 Resp: 152047
Ion Ratio Lower Upper
165 100
63 63.8 50.6 75.8
182 2.7 2.2 3.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.101 ng/ul
RT: 14.898 min Scan# 2025
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:232 Resp: 116401
Ion Ratio Lower Upper
232 100
131 67.2 50.4 75.6
130 3.6 2.6 3.8
166 39.2 31.9 47.9



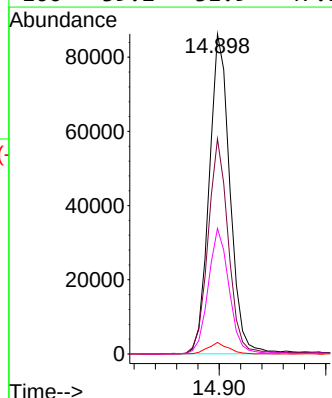





#59
Diethylphthalate
Concen: 22.451 ng/ul
RT: 15.116 min Scan# 2062
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:149 Resp: 636088
Ion Ratio Lower Upper
149 100
177 19.6 16.1 24.1
150 12.3 9.4 14.0



#61
Fluorene
Concen: 22.497 ng/ul
RT: 15.322 min Scan# 2097
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:166 Resp: 613855
Ion Ratio Lower Upper
166 100
165 98.1 77.7 116.5
167 13.5 11.0 16.4









#62
4-Chlorophenyl-phenylether
Concen: 22.183 ng/ul
RT: 15.328 min Scan# 2098
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:204 Resp: 267299
Ion Ratio Lower Upper
204 100
206 32.6 27.3 40.9
141 76.9 57.7 86.5

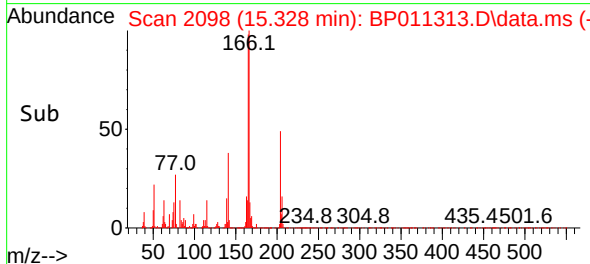

#63
4-Nitroaniline
Concen: 11.665 ng/ul
RT: 15.363 min Scan# 2104
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:138 Resp: 44362
Ion Ratio Lower Upper
138 100
92 59.1 55.9 83.9
108 89.2 67.1 100.7


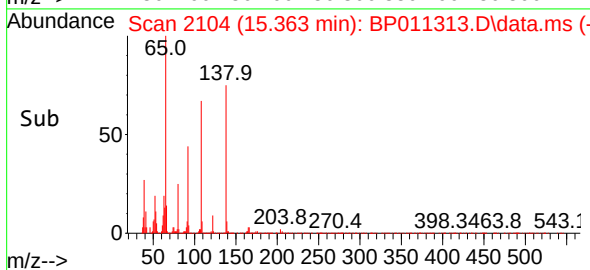

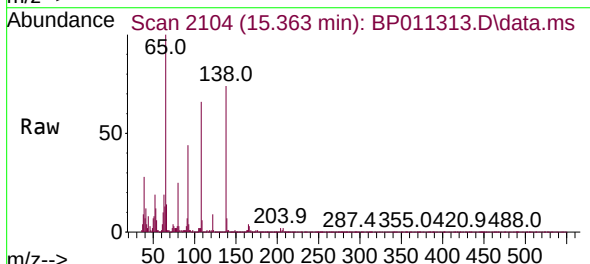


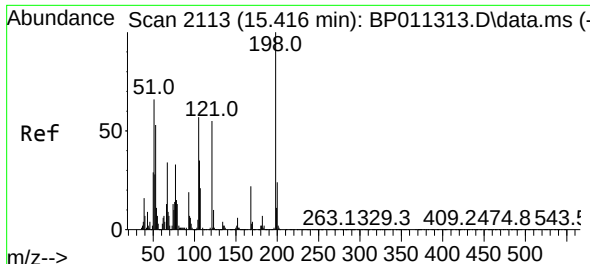

#66
 4,6-Dinitro-2-methylphenol
 Concen: 19.446 ng/ul
 RT: 15.416 min Scan# 2113
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020640


Tgt Ion:198 Resp: 73500
 Ion Ratio Lower Upper
 198 100
 182 6.8 7.4 11.0#
 77 34.6 28.6 42.8



#67
 N-Nitrosodiphenylamine
 Concen: 22.614 ng/ul
 RT: 15.545 min Scan# 2135
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16

Tgt Ion:169 Resp: 520315
 Ion Ratio Lower Upper
 169 100
 168 67.6 53.6 80.4
 167 37.0 30.0 45.0


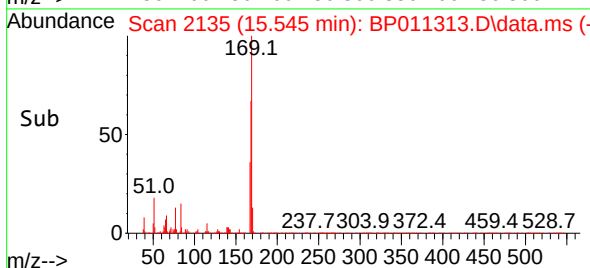
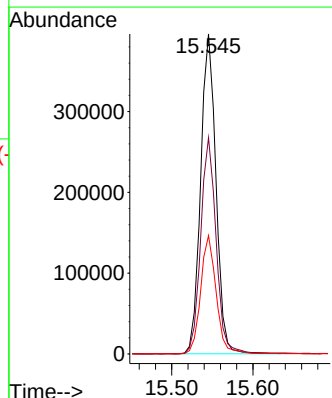
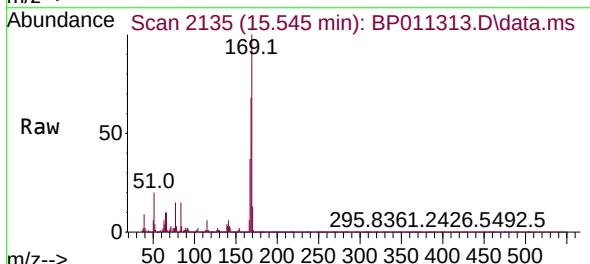




#68
4-Bromophenyl-phenylether
Concen: 21.341 ng/ul
RT: 16.228 min Scan# 2251
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:248 Resp: 151550
Ion Ratio Lower Upper
248 100
250 96.2 77.3 115.9
141 102.4 76.4 114.6



#69
Hexachlorobenzene
Concen: 21.092 ng/ul
RT: 16.328 min Scan# 2268
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:284 Resp: 174959
Ion Ratio Lower Upper
284 100
142 54.0 39.5 59.3
249 35.3 25.1 37.7

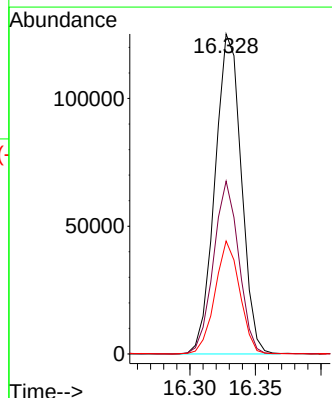

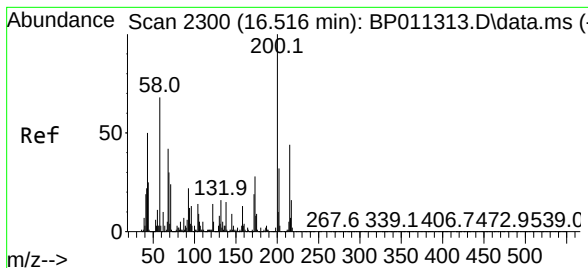

#70

Atrazine

Concen: 23.404 ng/ul

RT: 16.516 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Instrument :

BNA_P

ClientSampleId :

SSTD020640





Tgt Ion:200 Resp: 161086

Ion Ratio Lower Upper

200 100

173 28.5 22.6 34.0

215 43.5 36.5 54.7

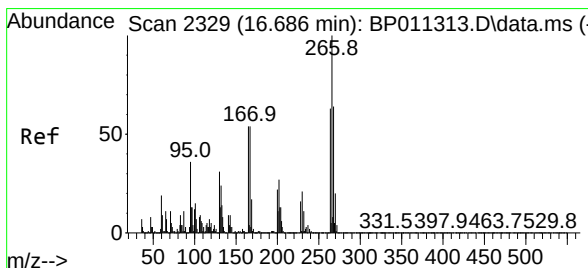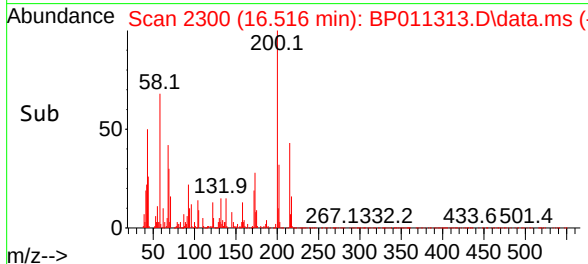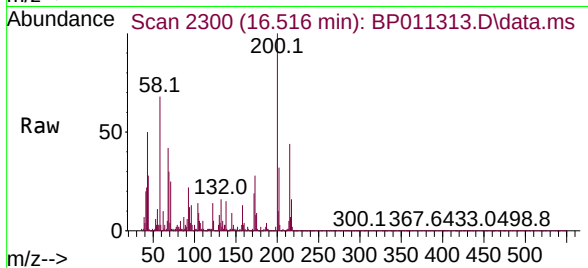

#71

Pentachlorophenol

Concen: 19.470 ng/ul

RT: 16.686 min Scan# 2329

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16




Tgt Ion:266 Resp: 94594


Ion Ratio Lower Upper

266 100

264 63.3 52.2 78.2

268 64.0 50.6 75.8


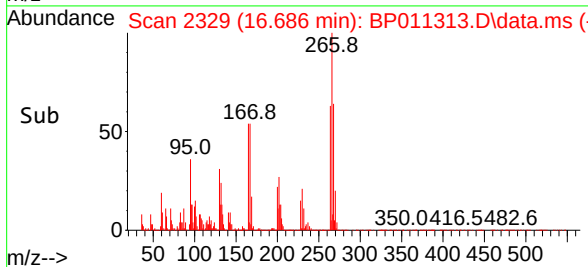

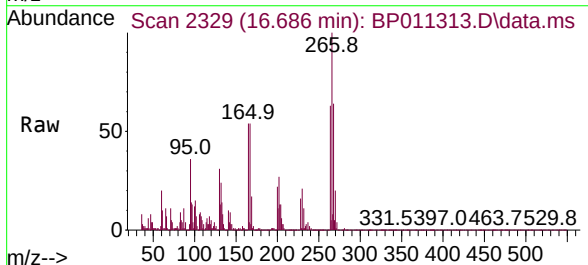




#72
Phenanthrene
Concen: 22.182 ng/ul
RT: 17.081 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:178 Resp: 955994
Ion Ratio Lower Upper
178 100
179 15.1 12.1 18.1
176 19.5 15.4 23.2



#74
Anthracene
Concen: 22.557 ng/ul
RT: 17.169 min Scan# 2411
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:178 Resp: 966860
Ion Ratio Lower Upper
178 100
179 15.3 12.3 18.5
176 18.6 14.7 22.1









#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.336 ng/uL
RT: 13.051 min Scan# 1711
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:216 Resp: 232937
Ion Ratio Lower Upper
216 100
214 78.7 62.0 93.0
218 48.1 38.2 57.4

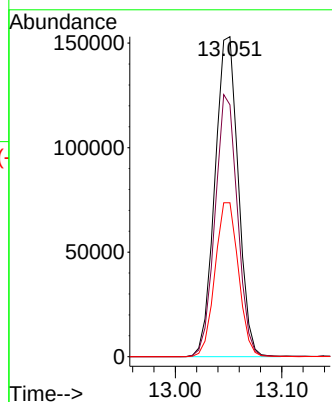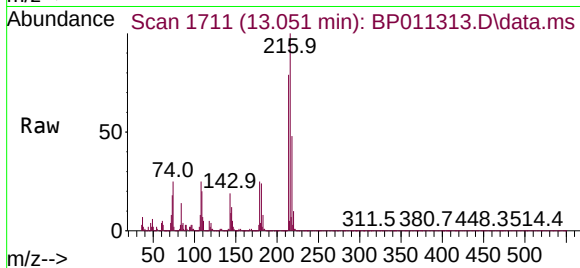

#76
Pentachlorobenzene
Concen: 20.694 ng/uL
RT: 14.581 min Scan# 1971
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:250 Resp: 212509
Ion Ratio Lower Upper
250 100
248 63.6 49.2 73.8
252 63.4 50.8 76.2



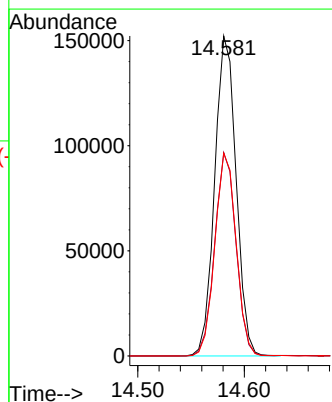





#77
 Carbazole
 Concen: 23.266 ng/ul
 RT: 17.451 min Scan# 2459
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020640


Tgt Ion:167 Resp: 894383
 Ion Ratio Lower Upper
 167 100
 166 21.5 17.1 25.7
 139 14.5 11.5 17.3



#78
 Di-n-butylphthalate
 Concen: 20.193 ng/ul
 RT: 18.028 min Scan# 2557
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16

Tgt Ion:149 Resp: 962933
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.4 11.0
 104 6.2 5.1 7.7









#80
Fluoranthene
Concen: 23.142 ng/ul
RT: 19.069 min Scan# 2734
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:202 Resp: 1057677
Ion Ratio Lower Upper
202 100
101 15.8 11.9 17.9
100 12.0 9.3 13.9

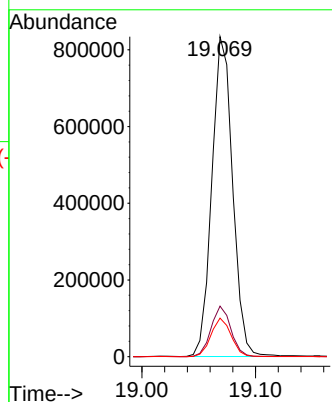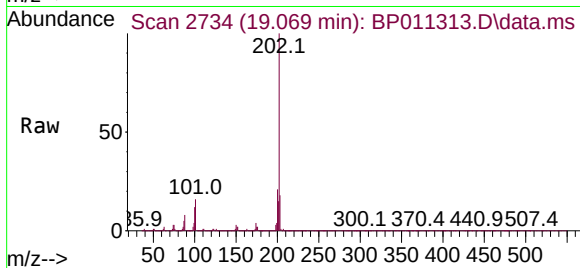

#82
Pyrene
Concen: 23.341 ng/ul
RT: 19.427 min Scan# 2795
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:202 Resp: 1113207
Ion Ratio Lower Upper
202 100
101 16.6 14.3 21.5
100 14.2 11.8 17.6


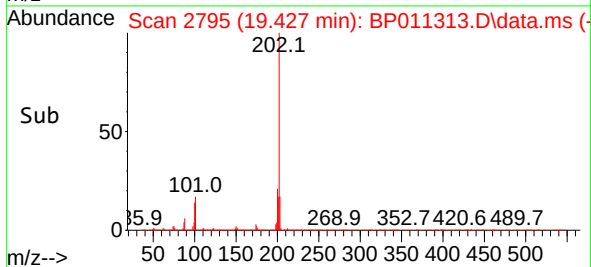
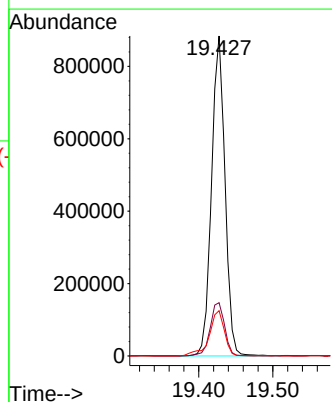
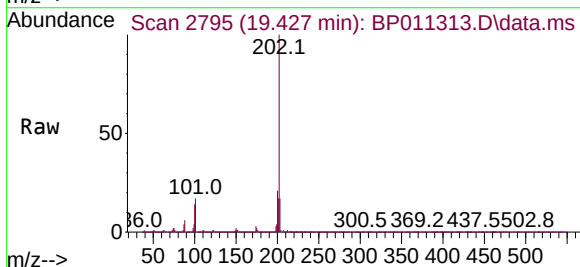




#83
Butylbenzylphthalate
Concen: 19.098 ng/ul
RT: 20.327 min Scan# 2948
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:149 Resp: 347790
Ion Ratio Lower Upper
149 100
91 82.0 64.2 96.4
206 17.1 14.0 21.0



#84
3,3'-Dichlorobenzidine
Concen: 20.566 ng/ul
RT: 21.098 min Scan# 3079
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:252 Resp: 248613
Ion Ratio Lower Upper
252 100
254 64.0 51.8 77.6
126 14.5 11.4 17.0





#85

Benzo(a)anthracene

Concen: 22.130 ng/ul

RT: 21.151 min Scan# 3088

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Instrument :

BNA_P

ClientSampleId :

SSTD020640





Tgt Ion:228 Resp: 1022312

Ion Ratio Lower Upper

228 100

229 19.8 15.8 23.6

226 27.5 21.8 32.6

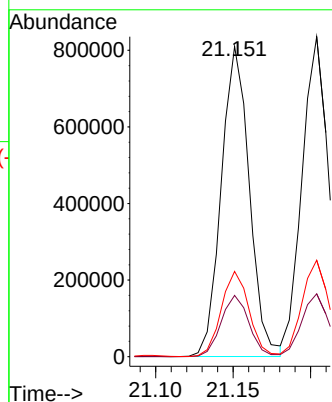

#86

Bis(2-ethylhexyl)phthalate

Concen: 17.411 ng/ul

RT: 21.092 min Scan# 3078

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16




Tgt Ion:149 Resp: 541779


Ion Ratio Lower Upper

149 100

167 25.7 20.4 30.6

279 3.0 2.9 4.3



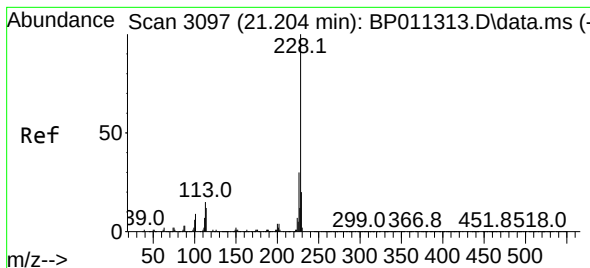

#87

Chrysene

Concen: 22.446 ng/ul

RT: 21.204 min Scan# 3097

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Instrument :

BNA_P

ClientSampleId :

SSTD020640





Tgt Ion:228 Resp: 1020619

Ion Ratio Lower Upper

228 100

226 30.1 23.8 35.6

229 19.7 15.7 23.5

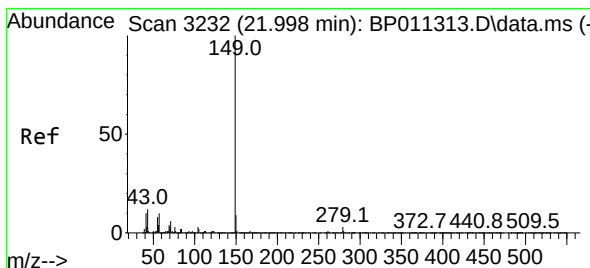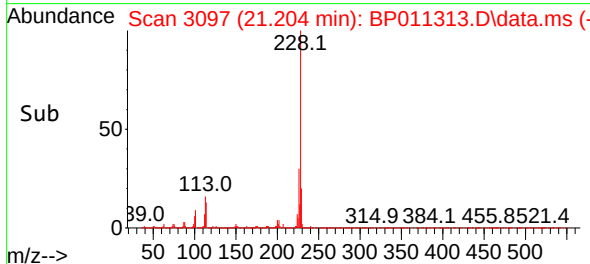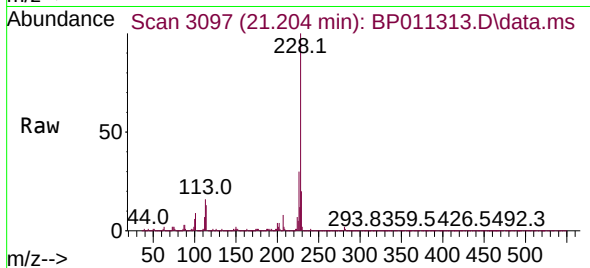

#89

Di-n-octyl phthalate

Concen: 18.894 ng/ul




RT: 21.998 min Scan# 3232


Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Tgt Ion:149 Resp: 927810


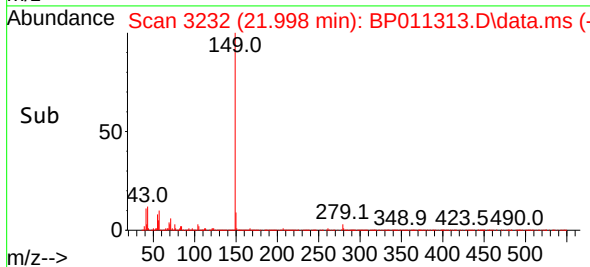

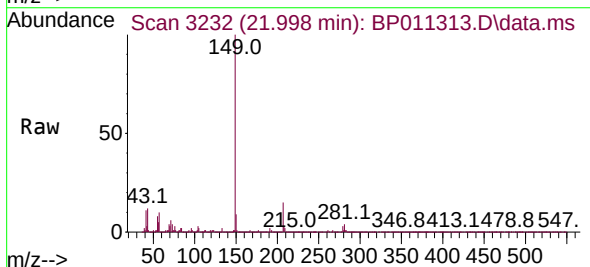




#90
Benzo(b)fluoranthene
Concen: 22.323 ng/ul
RT: 22.774 min Scan# 3364
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16




Instrument :
BNA_P
ClientSampleId :
SSTD020640


Tgt Ion:252 Resp: 1024268
Ion Ratio Lower Upper
252 100
253 22.1 17.4 26.0
125 14.4 10.8 16.2

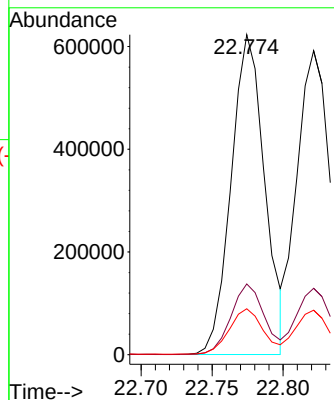

#91
Benzo(k)fluoranthene
Concen: 23.230 ng/ul
RT: 22.821 min Scan# 3372
Delta R.T. 0.000 min
Lab File: BP011313.D
Acq: 08 Aug 2022 16:16

Tgt Ion:252 Resp: 999981
Ion Ratio Lower Upper
252 100
253 21.8 17.6 26.4
125 14.6 11.0 16.6

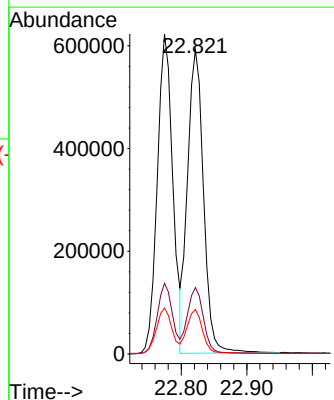



#93

Benzo(a)pyrene

Concen: 22.318 ng/ul

RT: 23.374 min Scan# 3466

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16

Instrument :

BNA_P

ClientSampleId :

SSTD020640





Tgt Ion:252 Resp: 996844

Ion Ratio Lower Upper

252 100

253 22.0 17.4 26.2

125 16.5 12.5 18.7

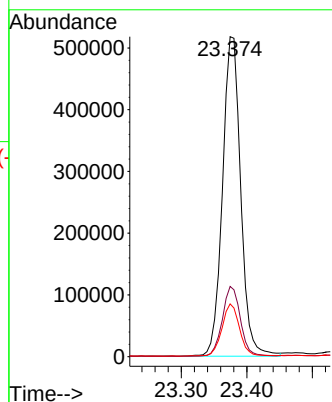

#94

Indeno(1,2,3-cd)pyrene

Concen: 20.476 ng/ul

RT: 25.857 min Scan# 3888

Delta R.T. 0.000 min

Lab File: BP011313.D

Acq: 08 Aug 2022 16:16




Tgt Ion:276 Resp: 1091474


Ion Ratio Lower Upper

276 100

138 30.0 25.5 38.3

277 25.0 19.8 29.8









#95
 Dibenzo(a,h)anthracene
 Concen: 20.393 ng/ul
 RT: 25.886 min Scan# 3893
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020640

Tgt Ion:278 Resp: 921789
 Ion Ratio Lower Upper
 278 100
 139 21.3 18.5 27.7
 279 23.6 19.6 29.4



#96
 Benzo(g,h,i)perylene
 Concen: 20.313 ng/ul
 RT: 26.592 min Scan# 4013
 Delta R.T. 0.000 min
 Lab File: BP011313.D
 Acq: 08 Aug 2022 16:16

Tgt Ion:276 Resp: 927865
 Ion Ratio Lower Upper
 276 100
 138 29.0 22.8 34.2
 277 24.2 18.5 27.7

