

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081621\
Data File : BP006680.D
Acq On : 16 Aug 2021 11:13
Operator : CG/JU
Sample : M2250-02
Misc : SFAM-MDL-WATER-02
ALS Vial : 4 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06

Manual Integrations
APPROVED

mohammad

8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:40:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 16 11:01:16 2021
Response via : Initial Calibration

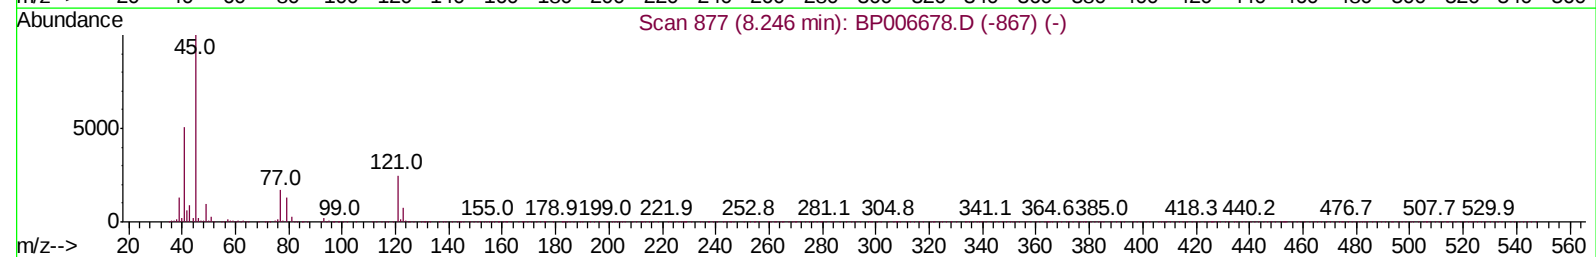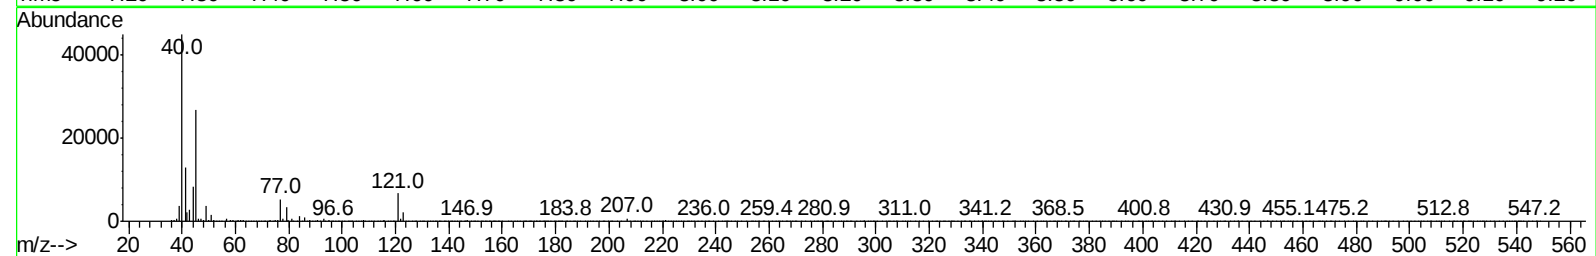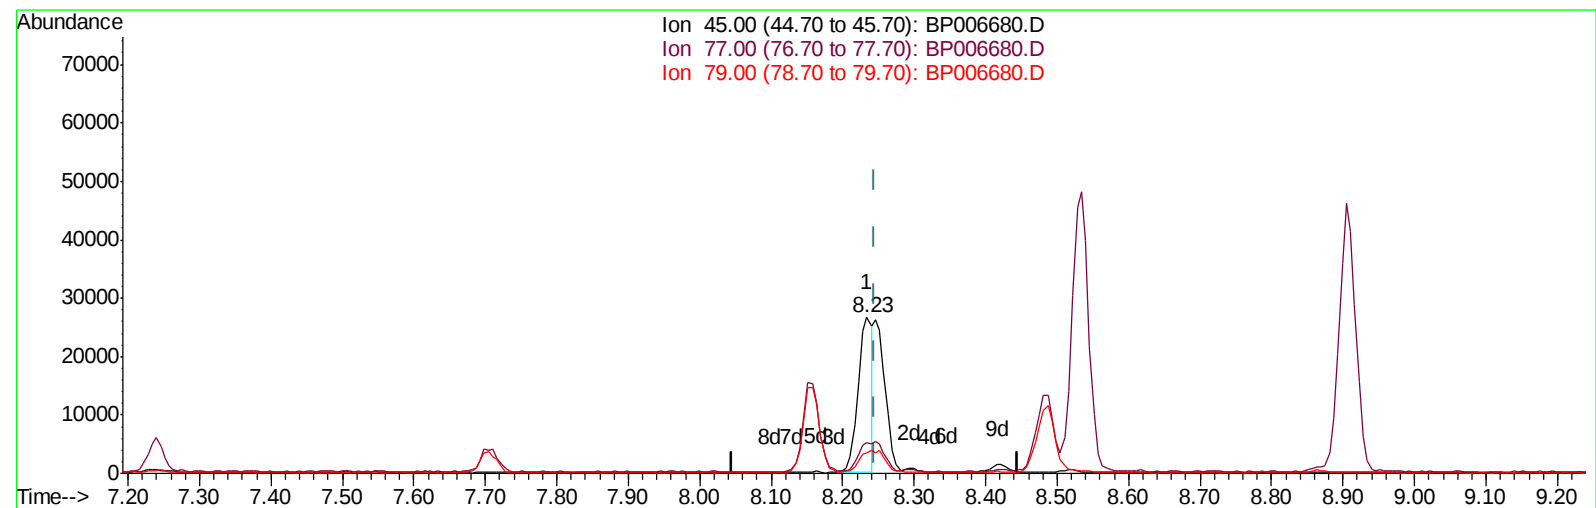

TIC: BP006680.D

(14) 2,2'-oxybis(1-Chloropropane)

8.234min (-0.012) 2.34ng/ul

response 36156

Ion	Exp%	Act%
45.00	100	100
77.00	17.30	19.95
79.00	13.60	13.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081621\
Data File : BP006680.D
Acq On : 16 Aug 2021 11:13
Operator : CG/JU
Sample : M2250-02
Misc : SFAM-MDL-WATER-02
ALS Vial : 4 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06

Manual Integrations
APPROVED

mohammad

8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:40:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 16 11:01:16 2021
Response via : Initial Calibration

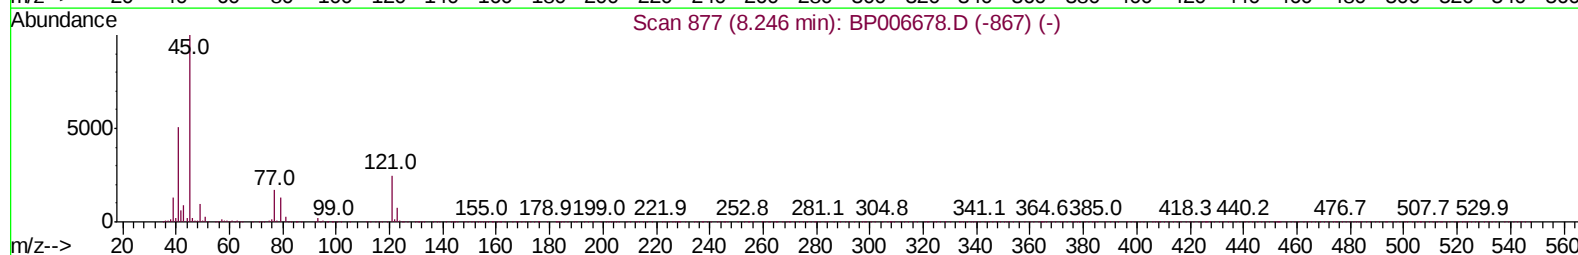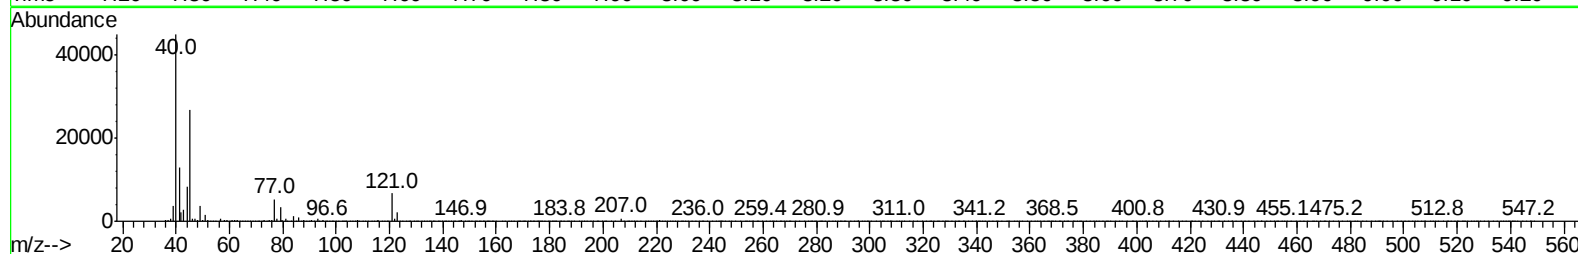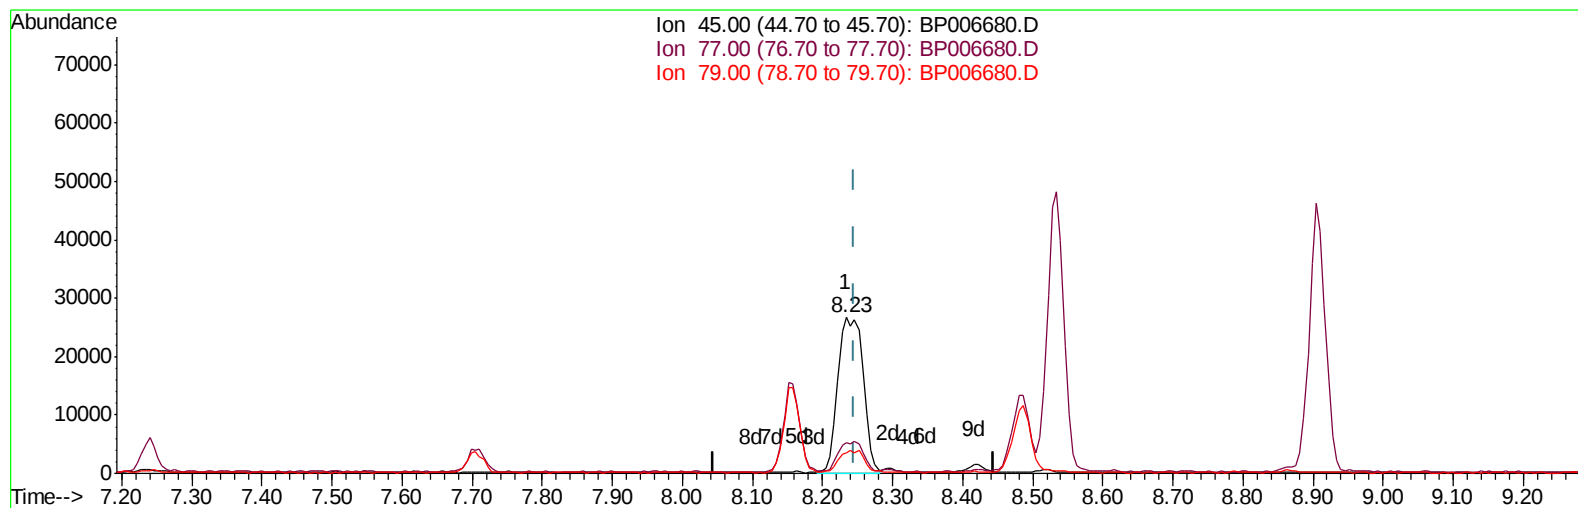

TIC: BP006680.D

(14) 2,2'-oxybis(1-Chloropropane)

8.234min (-0.012) 4.31ng/ul m

response 66552

Ion	Exp%	Act%
45.00	100	100
77.00	17.30	19.95
79.00	13.60	13.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081621\
 Data File : BP006680.D
 Acq On : 16 Aug 2021 11:13
 Operator : CG/JU
 Sample : M2250-02
 Misc : SFAM-MDL-WATER-02
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

mohammad
 8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:41:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 16 11:01:16 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	166975	20.00	ng/ul	0.00
20) Naphthalene-d8	10.49	136	703202	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.35	164	420314	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.11	188	835716	20.00	ng/ul	0.00
79) Chrysene-d12	21.22	240	824434	20.00	ng/ul	0.00
88) Perylene-d12	23.53	264	863298	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	24628	4.99	ng/uL	0.00
4) Pyridine-d5	3.63	84	244289	17.21	ng/ul	0.00
7) Phenol-d5	6.89	99	369133	21.99	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.05	67	247629	24.00	ng/ul	0.00
11) 2-Chlorophenol-d4	7.24	132	292183	23.37	ng/ul	0.00
15) 4-Methylphenol-d8	8.42	113	282589	21.07	ng/ul	0.00
21) Nitrobenzene-d5	8.86	128	144372	24.19	ng/ul	0.00
24) 2-Nitrophenol-d4	9.58	143	145720	23.33	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.12	165	242462	22.98	ng/ul	0.00
31) 4-Chloroaniline-d4	10.64	131	380204	22.17	ng/ul	0.00
46) Dimethylphthalate-d6	13.77	166	792547	24.59	ng/ul	0.00
49) Acenaphthylene-d8	14.04	160	972786	24.60	ng/ul	0.00
54) 4-Nitrophenol-d4	14.57	143	143388	21.30	ng/ul	0.00
60) Fluorene-d10	15.35	176	655129	24.99	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.48	200	107601	19.48	ng/ul	0.00
73) Anthracene-d10	17.21	188	984602	24.90	ng/ul	0.00
81) Pyrene-d10	19.46	212	1051337	24.28	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.39	264	1184750	25.45	ng/ul	0.01

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.25	88	6847	1.365 ng/uL#	90
5) Pyridine	3.65	79	65822	4.480 ng/ul#	80
6) Benzaldehyde	6.86	77	49790	6.033 ng/ul	99
8) Phenol	6.91	94	72382	4.222 ng/ul	100
10) Bis(2-Chloroethyl)ether	7.15	93	57274	4.335 ng/ul	97
12) 2-Chlorophenol	7.27	128	54518	4.325 ng/ul	99
13) 2-Methylphenol	8.16	108	51092	4.051 ng/ul	98
14) 2,2'-oxybis(1-Chloropropan	8.23	45	66552m	4.311 ng/ul	
16) Acetophenone	8.53	105	92840	4.398 ng/ul	96
17) N-Nitroso-di-n-propylamine	8.52	70	48110	4.237 ng/ul	97
18) 4-Methylphenol	8.49	108	55214	4.026 ng/ul	98
19) Hexachloroethane	8.78	117	25921	4.725 ng/ul	93
22) Nitrobenzene	8.90	77	74080	4.740 ng/ul	99
23) Isophorone	9.43	82	129417	4.441 ng/ul	99
25) 2-Nitrophenol	9.61	139	28757	4.365 ng/ul	95
26) 2,4-Dimethylphenol	9.68	107	64277	4.542 ng/ul	100
27) Bis(2-Chloroethoxy)methane	9.92	93	76582	4.533 ng/ul	99
29) 2,4-Dichlorophenol	10.15	162	45630	4.457 ng/ul	95
30) Naphthalene	10.54	128	179187	4.695 ng/ul	99
32) 4-Chloroaniline	10.66	127	74015	4.398 ng/ul	95
33) Hexachlorobutadiene	10.82	225	29439	4.877 ng/ul	95
34) Caprolactam	11.47	113	15163	3.699 ng/ul	95

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081621\
 Data File : BP006680.D
 Acq On : 16 Aug 2021 11:13
 Operator : CG/JU
 Sample : M2250-02
 Misc : SFAM-MDL-WATER-02
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleID :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

mohammad
 8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:41:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 16 11:01:16 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 4-Chloro-3-methylphenol	11.79	107	56169	4.289	ng/ul	96
36) 2-Methylnaphthalene	12.16	142	120745	4.604	ng/ul	100
37) 1-Methylnaphthalene	12.38	142	117340	4.496	ng/ul	100
39) 1,2,4,5-Tetrachlorobenzene	12.53	216	52734	4.656	ng/ul	97
40) Hexachlorocyclopentadiene	12.50	237	27504	3.701	ng/ul	98
41) 2,4,6-Trichlorophenol	12.77	196	32579	4.188	ng/ul	98
42) 2,4,5-Trichlorophenol	12.85	196	33367	4.029	ng/ul	96
43) 1,1'-Biphenyl	13.18	154	150966	4.620	ng/ul	100
44) 2-Chloronaphthalene	13.22	162	112263	4.529	ng/ul	98
45) 2-Nitroaniline	13.43	65	33210	3.715	ng/ul	92
47) Dimethylphthalate	13.82	163	148543	4.659	ng/ul	100
48) 2,6-Dinitrotoluene	13.94	165	22100	3.591	ng/ul	90
50) Acenaphthylene	14.07	152	183594	4.750	ng/ul	99
51) 3-Nitroaniline	14.26	138	26235	3.723	ng/ul#	93
52) Acenaphthene	14.42	153	126396	4.586	ng/ul	99
53) 2,4-Dinitrophenol	14.47	184	14077	3.537	ng/ul	98
55) 4-Nitrophenol	14.58	109	26771	4.434	ng/ul	96
56) Dibenzofuran	14.75	168	171180	4.645	ng/ul	99
57) 2,4-Dinitrotoluene	14.73	165	36115	3.989	ng/ul#	96
58) 2,3,4,6-Tetrachlorophenol	14.98	232	30540	4.442	ng/ul	98
59) Diethylphthalate	15.19	149	153251	4.522	ng/ul	99
61) Fluorene	15.40	166	142776	4.647	ng/ul	100
62) 4-Chlorophenyl-phenylether	15.40	204	66103	4.752	ng/ul	98
63) 4-Nitroaniline	15.43	138	27063	4.101	ng/ul	92
66) 4,6-Dinitro-2-methylphenol	15.49	198	21958	3.976	ng/ul#	94
67) N-Nitrosodiphenylamine	15.62	169	119381	4.651	ng/ul	99
68) 4-Bromophenyl-phenylether	16.30	248	37831	4.590	ng/ul	95
69) Hexachlorobenzene	16.40	284	43270	4.645	ng/ul	97
70) Atrazine	16.59	200	35116	3.856	ng/ul	97
71) Pentachlorophenol	16.76	266	22290	3.653	ng/ul	93
72) Phenanthrene	17.15	178	222238	4.707	ng/ul	99
74) Anthracene	17.25	178	223791	4.668	ng/ul	99
75) 1,2,3,4-Tetrachlorobenzene	13.14	216	51306	4.515	ng/uL	97
76) Pentachlorobenzene	14.67	250	50767	4.534	ng/uL	97
77) Carbazole	17.52	167	202437	4.521	ng/ul	100
78) Di-n-butylphthalate	18.09	149	230280	3.977	ng/ul	99
80) Fluoranthene	19.13	202	239869	4.408	ng/ul	99
82) Pyrene	19.49	202	260530	4.635	ng/ul	98
83) Butylbenzylphthalate	20.37	149	99740	3.590	ng/ul	93
84) 3,3'-Dichlorobenzidine	21.14	252	66573	3.539	ng/ul	97
85) Benzo(a)anthracene	21.20	228	245953	4.580	ng/ul	99
86) Bis(2-ethylhexyl)phthalate	21.15	149	161065	3.762	ng/ul	100
87) Chrysene	21.25	228	237209	4.582	ng/ul	99
89) Di-n-octyl phthalate	22.04	149	273309	3.662	ng/ul	100
90) Benzo(b)fluoranthene	22.83	252	248600	4.433	ng/ul	99
91) Benzo(k)fluoranthene	22.87	252	248475	4.576	ng/ul	98
93) Benzo(a)pyrene	23.43	252	226147	4.451	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.92	276	296666	4.466	ng/ul	98
95) Dibenzo(a,h)anthracene	25.94	278	252052	4.517	ng/ul	98
96) Benzo(g,h,i)perylene	26.66	276	247903	4.495	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081621\
Data File : BP006680.D
Acq On : 16 Aug 2021 11:13
Operator : CG/JU
Sample : M2250-02
Misc : SFAM-MDL-WATER-02
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06

Manual Integrations
APPROVED

mohammad

8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:41:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 16 11:01:16 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

