

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081621\
 Data File : BP006680.D
 Acq On : 16 Aug 2021 11:13
 Operator : CG/JU
 Sample : M2250-02
 Misc : SFAM-MDL-WATER-02
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

mohammad
 8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:40:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 16 11:01:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	166975	20.000	ng/u1	0.00
20) Naphthalene-d8	10.493	136	703202	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.351	164	420314	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.110	188	835716	20.000	ng/u1	0.00
79) Chrysene-d12	21.216	240	824434	20.000	ng/u1	0.00
88) Perylene-d12	23.533	264	863298	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	24628	4.989	ng/uL	0.00
4) Pyridine-d5	3.628	84	244289	17.214	ng/u1	0.00
7) Phenol-d5	6.887	99	369133	21.991	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.052	67	247629	24.004	ng/u1	0.00
11) 2-Chlorophenol-d4	7.240	132	292183	23.372	ng/u1	0.00
15) 4-Methylphenol-d8	8.422	113	282589	21.073	ng/u1	0.00
21) Nitrobenzene-d5	8.863	128	144372	24.186	ng/u1	0.00
24) 2-Nitrophenol-d4	9.581	143	145720	23.330	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	242462	22.976	ng/u1	0.00
31) 4-Chloroaniline-d4	10.640	131	380204	22.167	ng/u1	0.00
46) Dimethylphthalate-d6	13.775	166	792547	24.588	ng/u1	0.00
49) Acenaphthylene-d8	14.040	160	972786	24.604	ng/u1	0.00
54) 4-Nitrophenol-d4	14.569	143	143388	21.296	ng/u1	0.00
60) Fluorene-d10	15.351	176	655129	24.990	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	107601	19.479	ng/u1	0.00
73) Anthracene-d10	17.210	188	984602	24.900	ng/u1	0.00
81) Pyrene-d10	19.457	212	1051337	24.283	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.386	264	1184750	25.449	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	6847	1.365	ng/uL#	90
5) Pyridine	3.646	79	65822	4.480	ng/u1#	80
6) Benzaldehyde	6.858	77	49790	6.033	ng/u1	99
8) Phenol	6.910	94	72382	4.222	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.146	93	57274	4.335	ng/u1	97
12) 2-Chlorophenol	7.269	128	54518	4.325	ng/u1	99
13) 2-Methylphenol	8.157	108	51092	4.051	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.234	45	66552m	4.311	ng/u1	
16) Acetophenone	8.534	105	92840	4.398	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.522	70	48110	4.237	ng/u1	97
18) 4-Methylphenol	8.487	108	55214	4.026	ng/u1	98
19) Hexachloroethane	8.775	117	25921	4.725	ng/u1	93
22) Nitrobenzene	8.904	77	74080	4.740	ng/u1	99
23) Isophorone	9.434	82	129417	4.441	ng/u1	99
25) 2-Nitrophenol	9.610	139	28757	4.365	ng/u1	95
26) 2,4-Dimethylphenol	9.681	107	64277	4.542	ng/u1	100
27) Bis(2-Chloroethoxy)met...	9.922	93	76582	4.533	ng/u1	99
29) 2,4-Dichlorophenol	10.146	162	45630	4.457	ng/u1	95
30) Naphthalene	10.540	128	179187	4.695	ng/u1	99
32) 4-Chloroaniline	10.663	127	74015	4.398	ng/u1	95
33) Hexachlorobutadiene	10.822	225	29439	4.877	ng/u1	95
34) Caprolactam	11.475	113	15163	3.699	ng/u1	95
35) 4-Chloro-3-methylphenol	11.793	107	56169	4.289	ng/u1	96
36) 2-Methylnaphthalene	12.163	142	120745	4.604	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081621\
 Data File : BP006680.D
 Acq On : 16 Aug 2021 11:13
 Operator : CG/JU
 Sample : M2250-02
 Misc : SFAM-MDL-WATER-02
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

mohammad
 8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:40:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 16 11:01:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.381	142	117340	4.496	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.528	216	52734	4.656	ng/ul	97
40) Hexachlorocyclopentadiene	12.504	237	27504	3.701	ng/ul	98
41) 2,4,6-Trichlorophenol	12.775	196	32579	4.188	ng/ul	98
42) 2,4,5-Trichlorophenol	12.845	196	33367	4.029	ng/ul	96
43) 1,1'-Biphenyl	13.181	154	150966	4.620	ng/ul	100
44) 2-Chloronaphthalene	13.222	162	112263	4.529	ng/ul	98
45) 2-Nitroaniline	13.434	65	33210	3.715	ng/ul	92
47) Dimethylphthalate	13.822	163	148543	4.659	ng/ul	100
48) 2,6-Dinitrotoluene	13.940	165	22100	3.591	ng/ul	90
50) Acenaphthylene	14.069	152	183594	4.750	ng/ul	99
51) 3-Nitroaniline	14.263	138	26235	3.723	ng/ul#	93
52) Acenaphthene	14.416	153	126396	4.586	ng/ul	99
53) 2,4-Dinitrophenol	14.475	184	14077	3.537	ng/ul	98
55) 4-Nitrophenol	14.581	109	26771	4.434	ng/ul	96
56) Dibenzofuran	14.751	168	171180	4.645	ng/ul	99
57) 2,4-Dinitrotoluene	14.728	165	36115	3.989	ng/ul#	96
58) 2,3,4,6-Tetrachlorophenol	14.981	232	30540	4.442	ng/ul	98
59) Diethylphthalate	15.192	149	153251	4.522	ng/ul	99
61) Fluorene	15.404	166	142776	4.647	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.404	204	66103	4.752	ng/ul	98
63) 4-Nitroaniline	15.434	138	27063	4.101	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.492	198	21958	3.976	ng/ul#	94
67) N-Nitrosodiphenylamine	15.622	169	119381	4.651	ng/ul	99
68) 4-Bromophenyl-phenylether	16.304	248	37831	4.590	ng/ul	95
69) Hexachlorobenzene	16.404	284	43270	4.645	ng/ul	97
70) Atrazine	16.586	200	35116	3.856	ng/ul	97
71) Pentachlorophenol	16.757	266	22290	3.653	ng/ul	93
72) Phenanthrene	17.151	178	222238	4.707	ng/ul	99
74) Anthracene	17.245	178	223791	4.668	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.140	216	51306	4.515	ng/ul	97
76) Pentachlorobenzene	14.669	250	50767	4.534	ng/ul	97
77) Carbazole	17.522	167	202437	4.521	ng/ul	100
78) Di-n-butylphthalate	18.092	149	230280	3.977	ng/ul	99
80) Fluoranthene	19.127	202	239869	4.408	ng/ul	99
82) Pyrene	19.486	202	260530	4.635	ng/ul	98
83) Butylbenzylphthalate	20.374	149	99740	3.590	ng/ul	93
84) 3,3'-Dichlorobenzidine	21.139	252	66573	3.539	ng/ul	97
85) Benzo(a)anthracene	21.198	228	245953	4.580	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.145	149	161065	3.762	ng/ul	100
87) Chrysene	21.251	228	237209	4.582	ng/ul	99
89) Di-n-octyl phthalate	22.045	149	273309	3.662	ng/ul	100
90) Benzo(b)fluoranthene	22.827	252	248600	4.433	ng/ul	99
91) Benzo(k)fluoranthene	22.874	252	248475	4.576	ng/ul	98
93) Benzo(a)pyrene	23.433	252	226147	4.451	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.921	276	296666	4.466	ng/ul	98
95) Dibenzo(a,h)anthracene	25.945	278	252052	4.517	ng/ul	98
96) Benzo(g,h,i)perylene	26.656	276	247903	4.495	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081621\
 Data File : BP006680.D
 Acq On : 16 Aug 2021 11:13
 Operator : CG/JU
 Sample : M2250-02
 Misc : SFAM-MDL-WATER-02
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Manual Integrations
 APPROVED

mohammad
 8/17/2021 1:21:25 PM

Quant Time: Aug 16 11:40:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP081021.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 16 11:01:16 2021
 Response via : Initial Calibration

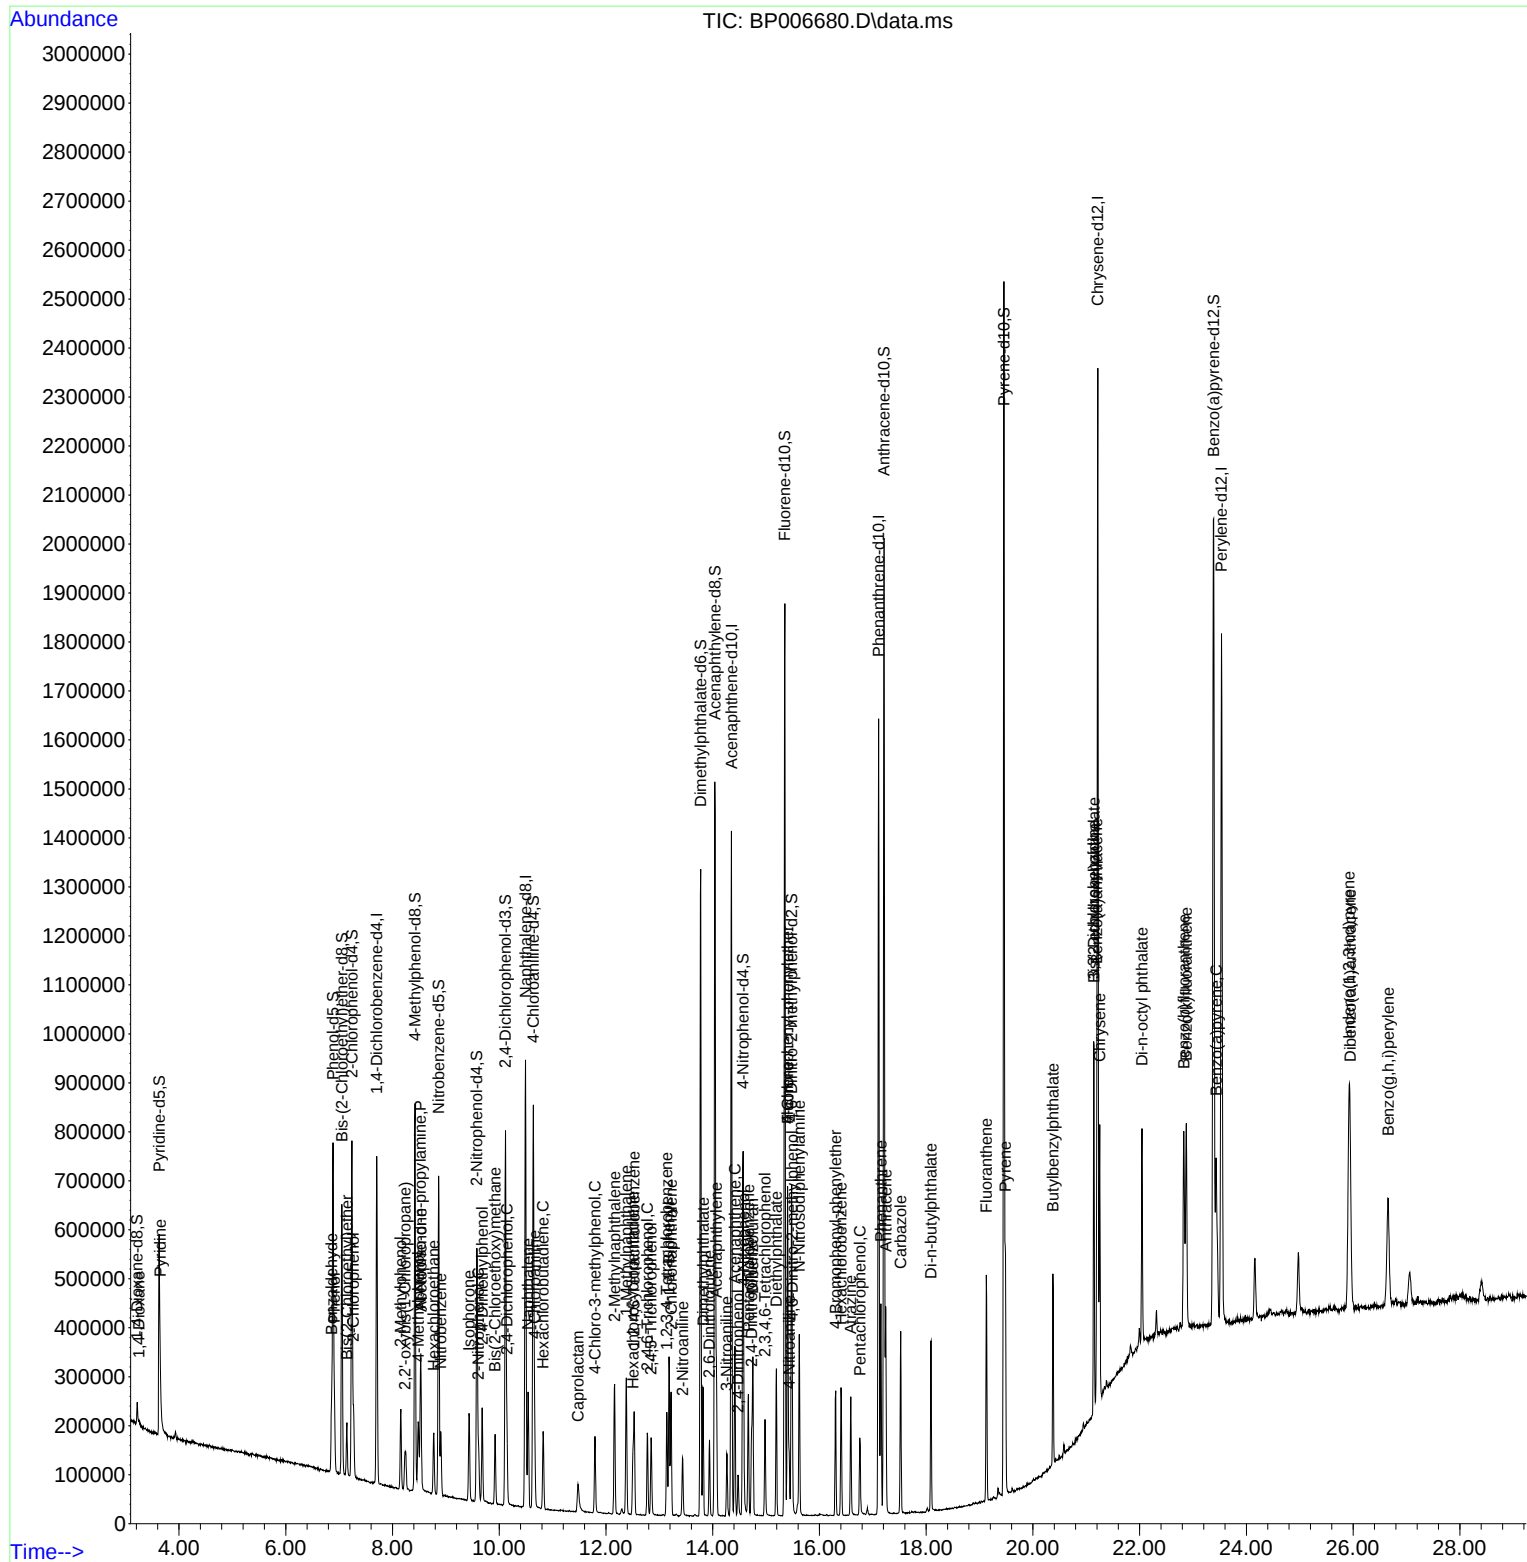







#2
1,4-Dioxane
Concen: 1.365 ng/uL
RT: 3.252 min Scan# 28
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion: 88 Resp: 6847
Ion Ratio Lower Upper
88 100
43 32.3 20.1 30.1#
58 54.4 48.4 72.6

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM

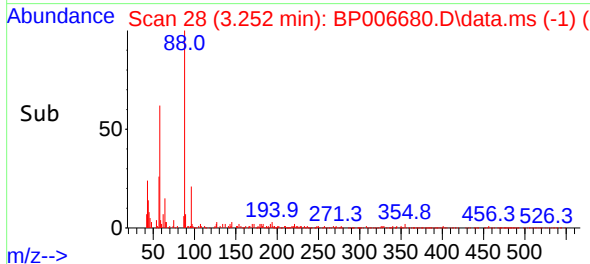

#5
Pyridine
Concen: 4.480 ng/uL
RT: 3.646 min Scan# 95
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion: 79 Resp: 65822
Ion Ratio Lower Upper
79 100
52 82.2 49.2 73.8#
51 31.3 22.7 34.1

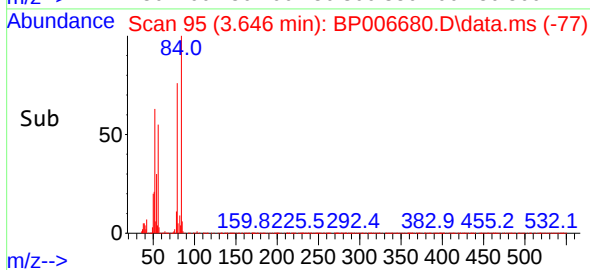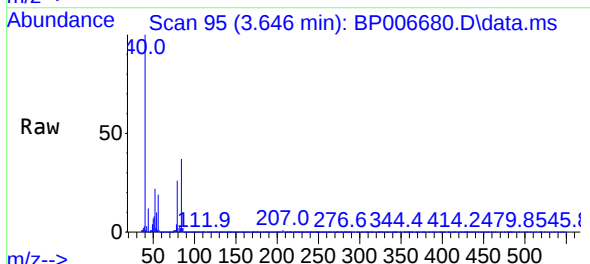



#6
Benzaldehyde
Concen: 6.033 ng/ul
RT: 6.858 min Scan# 641
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion: 77 Resp: 49790
Ion Ratio Lower Upper
77 100
105 92.8 74.4 111.6
106 86.3 70.3 105.5

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM

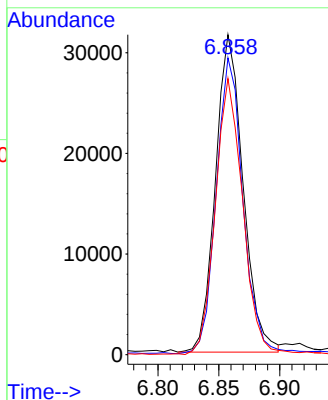


#8
Phenol
Concen: 4.222 ng/ul
RT: 6.910 min Scan# 650
Delta R.T. -0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13



Tgt Ion: 94 Resp: 72382
Ion Ratio Lower Upper
94 100
65 30.3 24.4 36.6
66 40.0 31.8 47.6

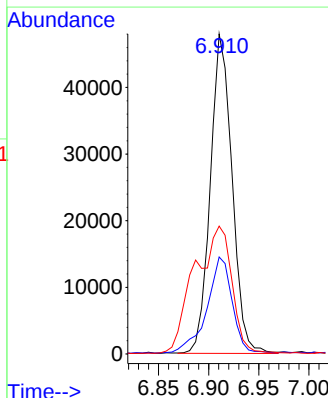

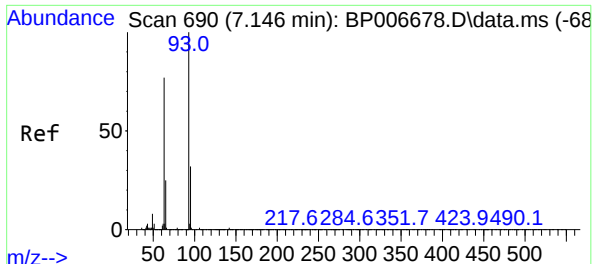

#10





Bis(2-Chloroethyl)ether
Concen: 4.335 ng/ul
RT: 7.146 min Scan# 690
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06

Tgt Ion:	93	Resp:	57274
Ion	Ratio	Lower	Upper
93	100		
63	77.5	59.7	89.5
95	31.2	25.3	37.9

Manual Integrations
APPROVED




mohammad
8/17/2021 1:21:25 PM

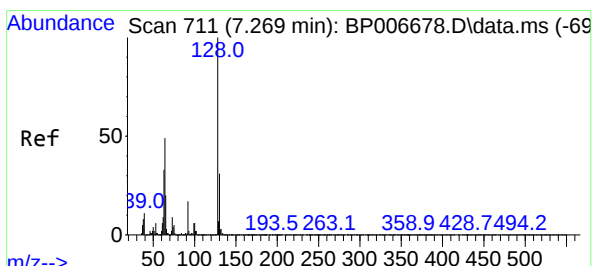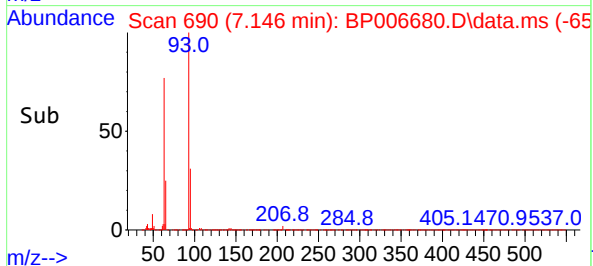


#12

2-Chlorophenol
Concen: 4.325 ng/ul
RT: 7.269 min Scan# 711
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:	128	Resp:	54518
Ion	Ratio	Lower	Upper
128	100		
64	49.6	40.6	60.8
130	32.9	26.4	39.6

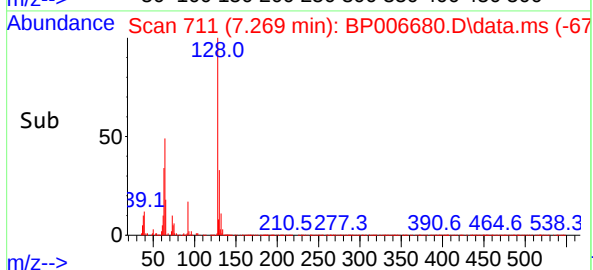



#13
2-Methylphenol
Concen: 4.051 ng/ul
RT: 8.157 min Scan# 862
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:108 Resp: 51092
Ion Ratio Lower Upper
108 100
107 91.7 72.2 108.2

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#14
2,2'-oxybis(1-Chloropropane)
Concen: 4.311 ng/ul m
RT: 8.234 min Scan# 875
Delta R.T. -0.012 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion: 45 Resp: 66552
Ion Ratio Lower Upper
45 100
77 20.0 13.8 20.8
79 13.0 10.9 16.3

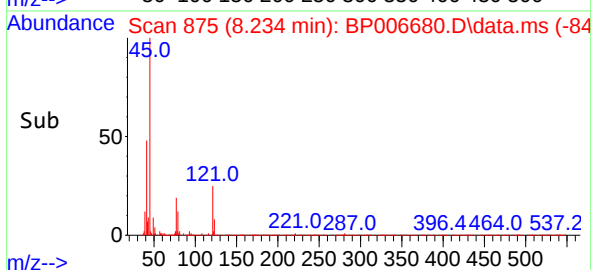



#16
Acetophenone
Concen: 4.398 ng/ul
RT: 8.534 min Scan# 926
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06



Tgt Ion:	105	Resp:	92840
Ion Ratio	Lower	Upper	
105	100		
77	79.7	67.0	100.4
51	23.2	19.0	28.6




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#17
N-Nitroso-di-n-propylamine
Concen: 4.237 ng/ul
RT: 8.522 min Scan# 924
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:	70	Resp:	48110
Ion Ratio	Lower	Upper	
70	100		
42	53.5	40.4	60.6
101	8.5	7.2	10.8
130	19.0	14.9	22.3

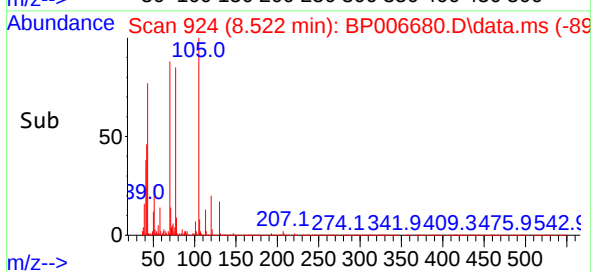



#18
4-Methylphenol
Concen: 4.026 ng/ul
RT: 8.487 min Scan# 918
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:108 Resp: 55214
Ion Ratio Lower Upper
108 100
107 108.4 88.6 133.0

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM

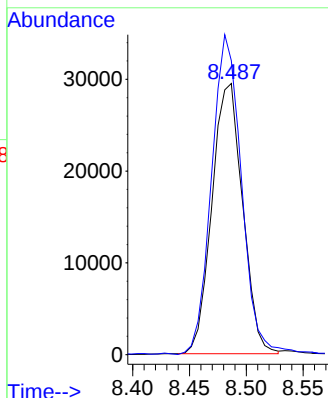


#19
Hexachloroethane
Concen: 4.725 ng/ul
RT: 8.775 min Scan# 967
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:117 Resp: 25921
Ion Ratio Lower Upper
117 100
201 78.5 68.2 102.2
199 50.1 43.5 65.3

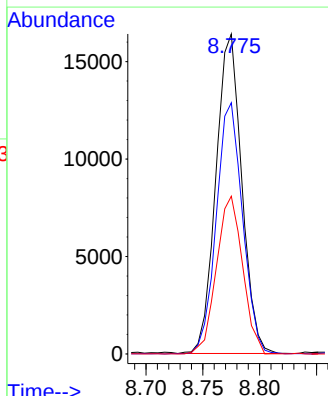



#22
Nitrobenzene
Concen: 4.740 ng/ul
RT: 8.904 min Scan# 989
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion: 77 Resp: 74080
Ion Ratio Lower Upper
77 100
123 38.4 31.1 46.7
65 12.1 10.6 16.0

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM

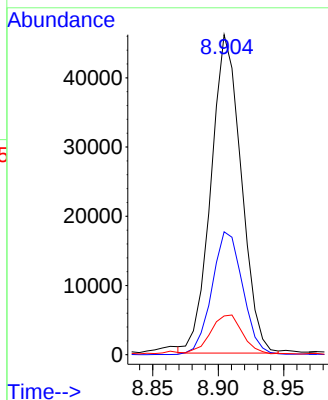


#23
Isophorone
Concen: 4.441 ng/ul
RT: 9.434 min Scan# 1079
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13



Tgt Ion: 82 Resp: 129417
Ion Ratio Lower Upper
82 100
95 6.6 5.8 8.8
138 15.5 12.5 18.7

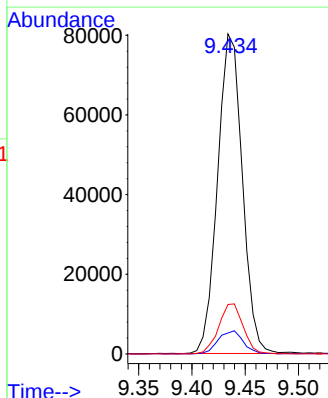







#25
2-Nitrophenol
Concen: 4.365 ng/ul
RT: 9.610 min Scan# 1109
Delta R.T. -0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion	Ratio	Lower	Upper
139	100		
65	65.7	48.4	72.6
109	34.5	28.2	42.2

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#26
2,4-Dimethylphenol
Concen: 4.542 ng/ul
RT: 9.681 min Scan# 1121
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion	Ratio	Lower	Upper
107	100		
121	47.7	38.1	57.1
122	80.6	64.2	96.4





#27
 Bis(2-Chloroethoxy)methane
 Concen: 4.533 ng/ul
 RT: 9.922 min Scan# 1162
 Delta R.T. -0.000 min
 Lab File: BP006680.D
 Acq: 16 Aug 2021 11:13




Instrument :
 BNA_P
 ClientSampleId :
 MDL-WATER-QT3-2021-06




Tgt Ion:	93	Resp:	76582
Ion	Ratio	Lower	Upper
93	100		
95	32.5	25.6	38.4
123	10.0	8.2	12.4

Manual Integrations
 APPROVED



mohammad
 8/17/2021 1:21:25 PM




#29
 2,4-Dichlorophenol
 Concen: 4.457 ng/ul
 RT: 10.146 min Scan# 1200
 Delta R.T. -0.000 min
 Lab File: BP006680.D
 Acq: 16 Aug 2021 11:13




Tgt Ion:	162	Resp:	45630
Ion	Ratio	Lower	Upper
162	100		
164	69.5	52.0	78.0
98	46.1	34.3	51.5

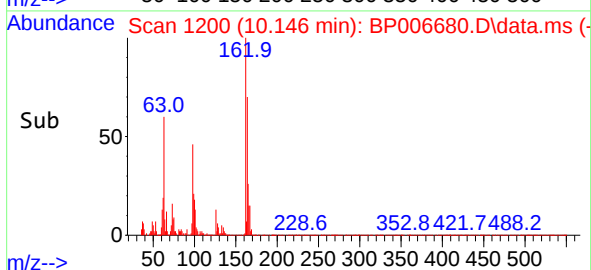





#30
Naphthalene
Concen: 4.695 ng/ul
RT: 10.540 min Scan# 1267
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:128 Resp: 179187
Ion Ratio Lower Upper
128 100
129 11.4 8.8 13.2
127 12.9 10.6 15.8




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#32
4-Chloroaniline
Concen: 4.398 ng/ul
RT: 10.663 min Scan# 1288
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:127 Resp: 74015
Ion Ratio Lower Upper
127 100
129 34.7 25.7 38.5



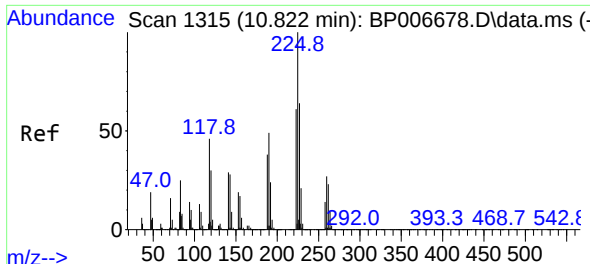

#33
Hexachlorobutadiene
Concen: 4.877 ng/ul
RT: 10.822 min Scan# 1315
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion	Ratio	Lower	Upper
225	100		
223	64.2	48.2	72.2
227	65.8	49.6	74.4

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#34
Caprolactam
Concen: 3.699 ng/ul
RT: 11.475 min Scan# 1426
Delta R.T. 0.023 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

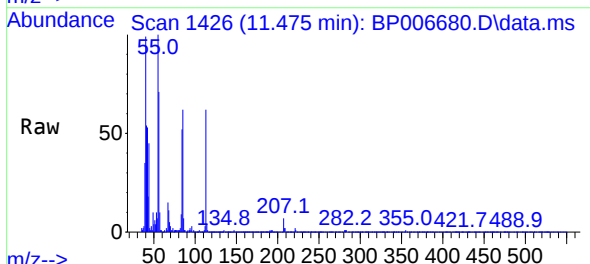


Tgt Ion	Ratio	Lower	Upper
113	100		
55	160.2	125.8	188.6
56	113.2	98.2	147.2

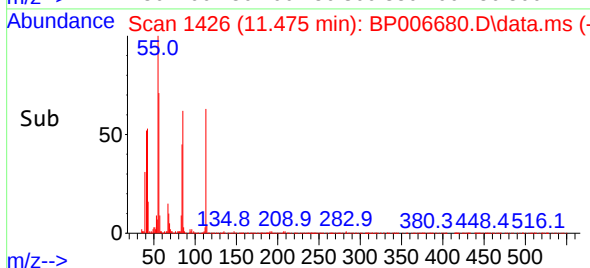



#35
4-Chloro-3-methylphenol
Concen: 4.289 ng/ul
RT: 11.793 min Scan# 1480
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:107 Resp: 56169
Ion Ratio Lower Upper
107 100
144 24.4 18.8 28.2
142 69.6 58.4 87.6

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM

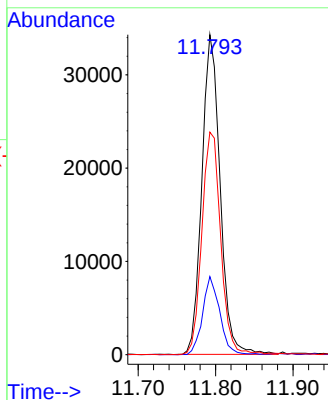


#36
2-Methylnaphthalene
Concen: 4.604 ng/ul
RT: 12.163 min Scan# 1543
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:142 Resp: 120745
Ion Ratio Lower Upper
142 100
141 90.0 72.3 108.5

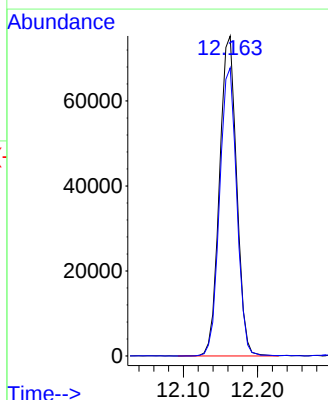



#37
1-Methylnaphthalene
Concen: 4.496 ng/ul
RT: 12.381 min Scan# 1580
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:142 Resp: 117340
Ion Ratio Lower Upper
142 100
141 93.2 74.9 112.3
116 4.3 3.3 4.9

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#39
1,2,4,5-Tetrachlorobenzene
Concen: 4.656 ng/ul
RT: 12.528 min Scan# 1605
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:216 Resp: 52734
Ion Ratio Lower Upper
216 100
214 77.5 64.3 96.5
179 23.2 19.3 28.9
108 23.8 19.8 29.6

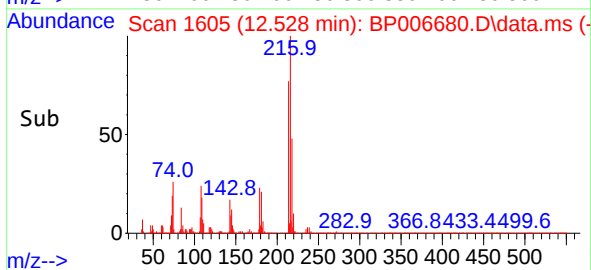



#40
Hexachlorocyclopentadiene
Concen: 3.701 ng/ul
RT: 12.504 min Scan# 1601
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:237 Resp: 27504
Ion Ratio Lower Upper
237 100
235 65.0 50.4 75.6
272 12.3 9.7 14.5

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#41
2,4,6-Trichlorophenol
Concen: 4.188 ng/ul
RT: 12.775 min Scan# 1647
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:196 Resp: 32579
Ion Ratio Lower Upper
196 100
198 92.4 76.2 114.4
200 30.3 24.6 36.8





#42
2,4,5-Trichlorophenol
Concen: 4.029 ng/ul
RT: 12.845 min Scan# 1659
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:196 Resp: 33367
Ion Ratio Lower Upper
196 100
198 96.2 79.3 118.9
200 28.6 25.8 38.8

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#43
1,1'-Biphenyl
Concen: 4.620 ng/ul
RT: 13.181 min Scan# 1716
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:154 Resp: 150966
Ion Ratio Lower Upper
154 100
153 40.4 32.4 48.6
76 16.1 12.9 19.3

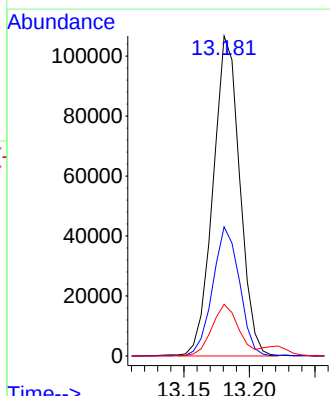



#44
2-Chloronaphthalene
Concen: 4.529 ng/ul
RT: 13.222 min Scan# 1723
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:162 Resp: 112263
Ion Ratio Lower Upper
162 100
164 33.5 25.6 38.4
127 44.4 36.2 54.2

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#45
2-Nitroaniline
Concen: 3.715 ng/ul
RT: 13.434 min Scan# 1759
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion: 65 Resp: 33210
Ion Ratio Lower Upper
65 100
92 69.1 53.7 80.5
138 77.5 71.4 107.2





#47
Dimethylphthalate
Concen: 4.659 ng/ul
RT: 13.822 min Scan# 1825
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:163 Resp: 148543
Ion Ratio Lower Upper
163 100
194 3.9 3.0 4.4
164 9.9 7.8 11.8

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#48
2,6-Dinitrotoluene
Concen: 3.591 ng/ul
RT: 13.940 min Scan# 1845
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13



Tgt Ion:165 Resp: 22100
Ion Ratio Lower Upper
165 100
89 87.4 62.2 93.2
121 31.4 22.1 33.1









#50
Acenaphthylene
Concen: 4.750 ng/ul
RT: 14.069 min Scan# 1867
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:	152	Resp:	183594
Ion Ratio	Lower	Upper	
152	100		
151	20.2	15.9	23.9
153	13.2	10.4	15.6

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#51
3-Nitroaniline
Concen: 3.723 ng/ul
RT: 14.263 min Scan# 1900
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:	138	Resp:	26235
Ion Ratio	Lower	Upper	
138	100		
108	15.5	9.7	14.5#
92	141.5	106.7	160.1



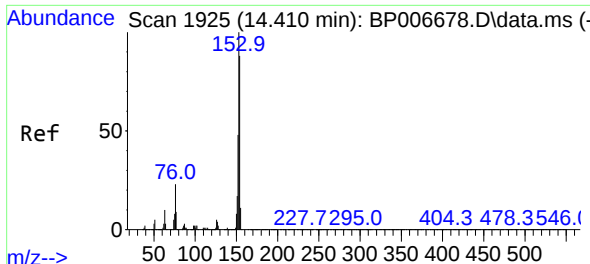

#52
Acenaphthene
Concen: 4.586 ng/ul
RT: 14.416 min Scan# 1926
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:153 Resp: 126396
Ion Ratio Lower Upper
153 100
152 49.1 38.6 57.8
154 85.5 69.0 103.6

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM

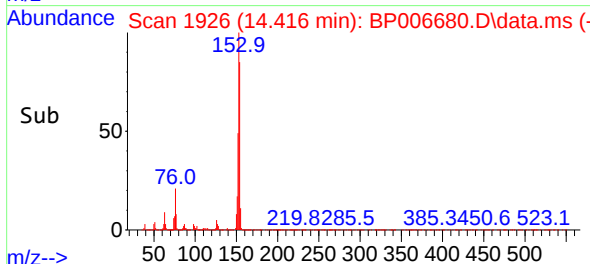


#53
2,4-Dinitrophenol
Concen: 3.537 ng/ul
RT: 14.475 min Scan# 1936
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

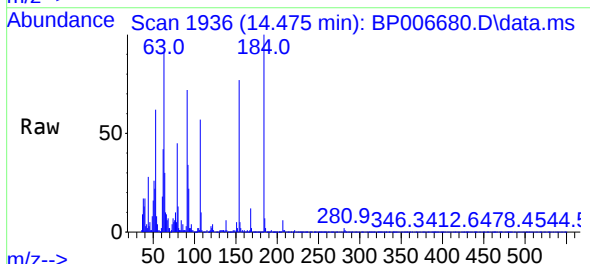


Tgt Ion:184 Resp: 14077
Ion Ratio Lower Upper
184 100
63 91.2 73.4 110.2
154 77.4 59.4 89.0





#55
4-Nitrophenol
Concen: 4.434 ng/ul
RT: 14.581 min Scan# 1954
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:109 Resp: 26771
Ion Ratio Lower Upper
109 100
139 109.5 90.3 135.5
65 134.0 102.2 153.2

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#56
Dibenzofuran
Concen: 4.645 ng/ul
RT: 14.751 min Scan# 1983
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13



Tgt Ion:168 Resp: 171180
Ion Ratio Lower Upper
168 100
139 44.7 35.3 52.9









#57
2,4-Dinitrotoluene
Concen: 3.989 ng/ul
RT: 14.728 min Scan# 1979
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:165 Resp: 36115
Ion Ratio Lower Upper
165 100
63 59.9 45.2 67.8
182 1.9 1.9 2.9#

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#58
2,3,4,6-Tetrachlorophenol
Concen: 4.442 ng/ul
RT: 14.981 min Scan# 2022
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:232 Resp: 30540
Ion Ratio Lower Upper
232 100
131 64.6 51.8 77.6
130 4.6 3.1 4.7
166 35.0 31.0 46.4

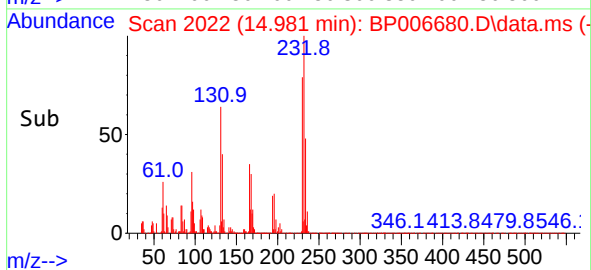



#59
Diethylphthalate
Concen: 4.522 ng/ul
RT: 15.192 min Scan# 2058
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06



Tgt Ion:149 Resp: 153251
Ion Ratio Lower Upper
149 100
177 19.4 15.5 23.3
150 11.3 9.9 14.9




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#61
Fluorene
Concen: 4.647 ng/ul
RT: 15.404 min Scan# 2094
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:166 Resp: 142776
Ion Ratio Lower Upper
166 100
165 99.9 79.6 119.4
167 13.3 10.7 16.1

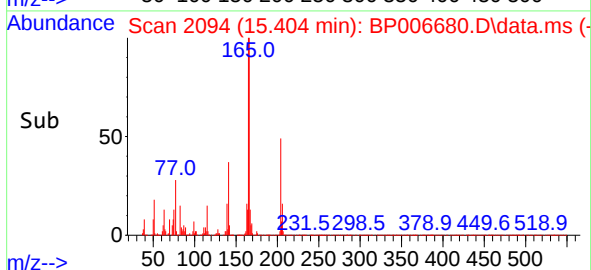



#62
4-Chlorophenyl-phenylether
Concen: 4.752 ng/ul
RT: 15.404 min Scan# 2094
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:204 Resp: 66103
Ion Ratio Lower Upper
204 100
206 32.2 26.3 39.5
141 75.7 62.0 93.0

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#63
4-Nitroaniline
Concen: 4.101 ng/ul
RT: 15.434 min Scan# 2099
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13



Tgt Ion:138 Resp: 27063
Ion Ratio Lower Upper
138 100
92 66.8 47.1 70.7
108 98.8 73.8 110.8









#66
4,6-Dinitro-2-methylphenol
Concen: 3.976 ng/ul
RT: 15.492 min Scan# 2109
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:198 Resp: 21958
Ion Ratio Lower Upper
198 100
182 7.9 4.5 6.7#
77 43.5 31.7 47.5

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#67
N-Nitrosodiphenylamine
Concen: 4.651 ng/ul
RT: 15.622 min Scan# 2131
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:169 Resp: 119381
Ion Ratio Lower Upper
169 100
168 66.7 53.9 80.9
167 37.2 30.0 45.0

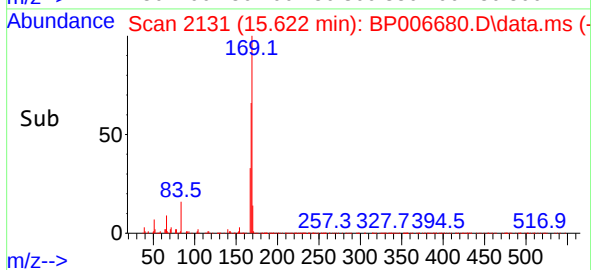

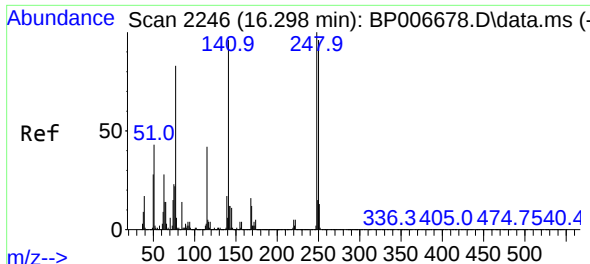

#68
4-Bromophenyl-phenylether
Concen: 4.590 ng/ul
RT: 16.304 min Scan# 2247
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06



Tgt Ion:248 Resp: 37831
Ion Ratio Lower Upper
248 100
250 97.1 78.4 117.6
141 92.2 80.6 121.0




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#69
Hexachlorobenzene
Concen: 4.645 ng/ul
RT: 16.404 min Scan# 2264
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:284 Resp: 43270
Ion Ratio Lower Upper
284 100
142 50.9 37.8 56.6
249 33.6 27.1 40.7

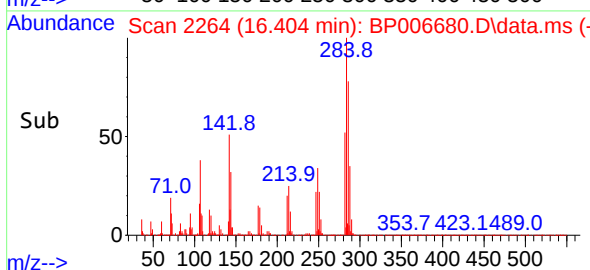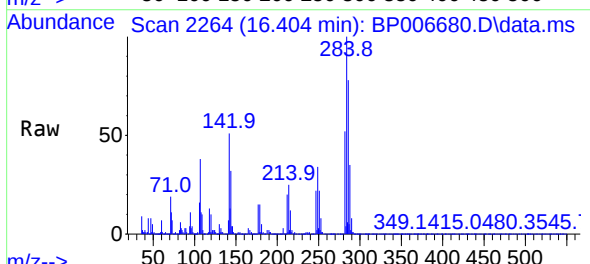







#70
Atrazine
Concen: 3.856 ng/ul
RT: 16.586 min Scan# 2295
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion	Ratio	Lower	Upper
200	100		
173	26.6	22.2	33.4
215	46.3	35.4	53.0

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#71
Pentachlorophenol
Concen: 3.653 ng/ul
RT: 16.757 min Scan# 2324
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion	Ratio	Lower	Upper
266	100		
264	69.7	51.0	76.4
268	66.4	49.4	74.2

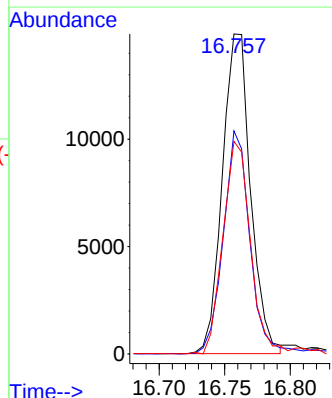



#72
Phenanthrene
Concen: 4.707 ng/u1
RT: 17.151 min Scan# 2391
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06



Tgt Ion:178 Resp: 222238
Ion Ratio Lower Upper
178 100
179 14.8 12.0 18.0
176 18.8 15.6 23.4




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#74
Anthracene
Concen: 4.668 ng/u1
RT: 17.245 min Scan# 2407
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:178 Resp: 223791
Ion Ratio Lower Upper
178 100
179 14.6 12.1 18.1
176 18.7 14.9 22.3

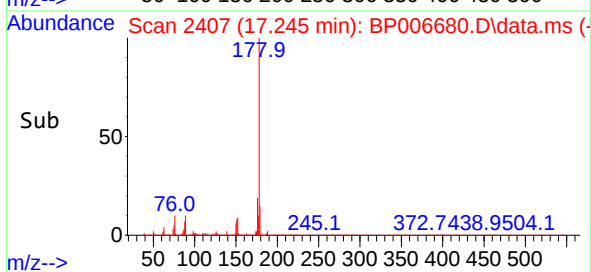







#75
1,2,3,4-Tetrachlorobenzene
Concen: 4.515 ng/uL
RT: 13.140 min Scan# 1709
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06

Tgt Ion:	216	Resp:	51306
Ion Ratio	Lower	Upper	
216	100		
214	74.9	62.9	94.3
218	47.4	37.8	56.8




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#76
Pentachlorobenzene
Concen: 4.534 ng/uL
RT: 14.669 min Scan# 1969
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:	250	Resp:	50767
Ion Ratio	Lower	Upper	
250	100		
248	61.4	51.0	76.6
252	65.7	51.0	76.4

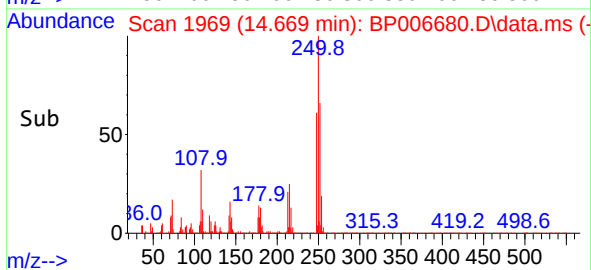



#77
Carbazole
Concen: 4.521 ng/ul
RT: 17.522 min Scan# 2454
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:167 Resp: 202437
Ion Ratio Lower Upper
167 100
166 22.0 17.6 26.4
139 14.6 11.9 17.9

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM




#78
Di-n-butylphthalate
Concen: 3.977 ng/ul
RT: 18.092 min Scan# 2551
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:149 Resp: 230280
Ion Ratio Lower Upper
149 100
150 9.4 7.3 10.9
104 6.2 4.8 7.2

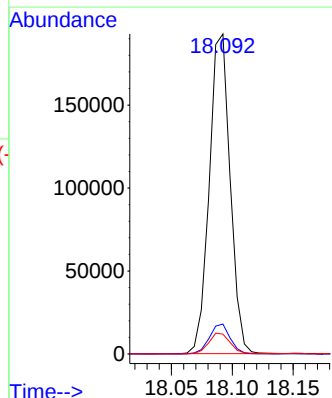



#80
Fluoranthene
Concen: 4.408 ng/u1
RT: 19.127 min Scan# 2727
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:202 Resp: 239869
Ion Ratio Lower Upper
202 100
101 14.0 11.0 16.4
100 10.6 8.3 12.5

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM

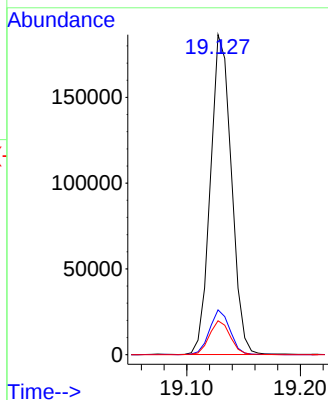


#82
Pyrene
Concen: 4.635 ng/u1
RT: 19.486 min Scan# 2788
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:202 Resp: 260530
Ion Ratio Lower Upper
202 100
101 15.1 12.6 19.0
100 12.5 10.6 15.8


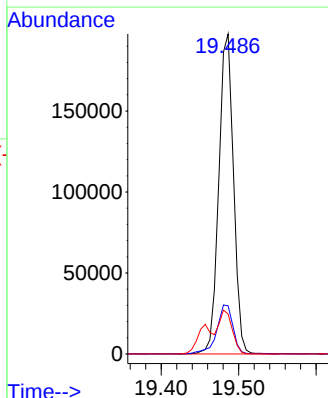






#83
Butylbenzylphthalate
Concen: 3.590 ng/ul
RT: 20.374 min Scan# 2939
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13





Tgt Ion:149 Resp: 99740
Ion Ratio Lower Upper
149 100
91 86.4 63.0 94.6
206 18.3 14.1 21.1



#84
3,3'-Dichlorobenzidine
Concen: 3.539 ng/ul
RT: 21.139 min Scan# 3069
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:252 Resp: 66573
Ion Ratio Lower Upper
252 100
254 62.8 51.6 77.4
126 15.3 10.7 16.1



Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06

Manual Integrations
APPROVED

mohammad
8/17/2021 1:21:25 PM







#85
Benzo(a)anthracene
Concen: 4.580 ng/ul
RT: 21.198 min Scan# 3079
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:	228	Resp:	245953
Ion	Ratio	Lower	Upper
228	100		
229	19.1	15.8	23.8
226	26.6	21.6	32.4

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#86
Bis(2-ethylhexyl)phthalate
Concen: 3.762 ng/ul
RT: 21.145 min Scan# 3070
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:	149	Resp:	161065
Ion	Ratio	Lower	Upper
149	100		
167	25.0	20.2	30.2
279	3.8	2.7	4.1

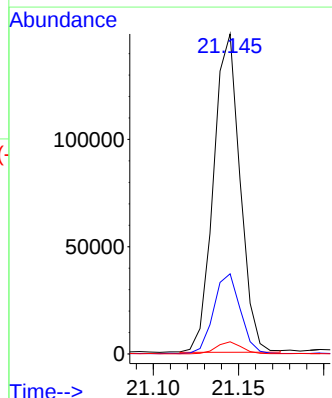



#87
Chrysene
Concen: 4.582 ng/ul
RT: 21.251 min Scan# 3088
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13





Tgt Ion:228 Resp: 237209

Ion	Ratio	Lower	Upper
228	100		
226	30.7	24.5	36.7
229	18.8	15.9	23.9

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#89
Di-n-octyl phthalate
Concen: 3.662 ng/ul
RT: 22.045 min Scan# 3223
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:149 Resp: 273309









#90
Benzo(b)fluoranthene
Concen: 4.433 ng/ul
RT: 22.827 min Scan# 3356
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13

Tgt Ion:252 Resp: 248600
Ion Ratio Lower Upper
252 100
253 21.8 17.7 26.5
125 13.0 10.1 15.1

Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Manual Integrations
APPROVED


mohammad
8/17/2021 1:21:25 PM



#91
Benzo(k)fluoranthene
Concen: 4.576 ng/ul
RT: 22.874 min Scan# 3364
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13


Tgt Ion:252 Resp: 248475
Ion Ratio Lower Upper
252 100
253 22.2 17.2 25.8
125 12.6 9.4 14.0

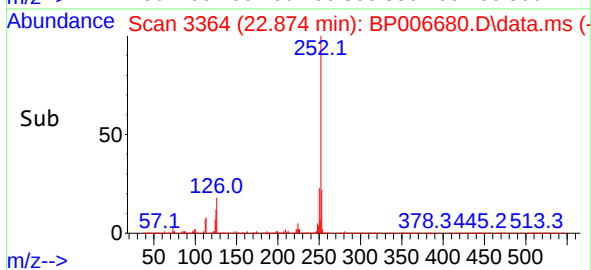



#93
Benzo(a)pyrene
Concen: 4.451 ng/ul
RT: 23.433 min Scan# 3459
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:252 Resp: 226147
Ion Ratio Lower Upper
252 100
253 22.5 17.6 26.4
125 14.8 11.3 16.9

Manual Integrations
APPROVED



mohammad
8/17/2021 1:21:25 PM

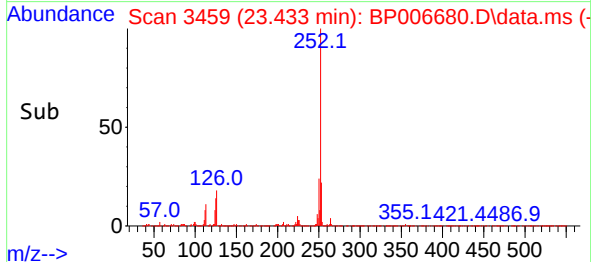


#94
Indeno(1,2,3-cd)pyrene
Concen: 4.466 ng/ul
RT: 25.921 min Scan# 3882
Delta R.T. -0.000 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Tgt Ion:276 Resp: 296666
Ion Ratio Lower Upper
276 100
138 29.1 21.8 32.8
277 25.2 19.9 29.9

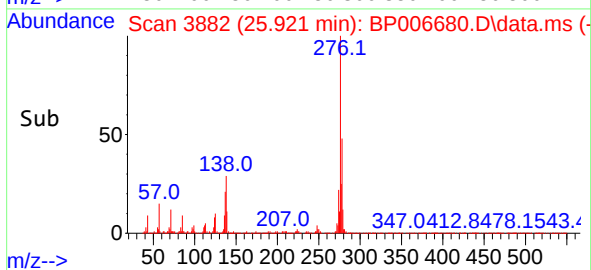



#95
Dibenzo(a,h)anthracene
Concen: 4.517 ng/ul
RT: 25.945 min Scan# 3886
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13




Instrument :
BNA_P
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion:278 Resp: 252052
Ion Ratio Lower Upper
278 100
139 19.7 15.4 23.2
279 25.0 19.0 28.4

Manual Integrations
APPROVED

mohammad
8/17/2021 1:21:25 PM

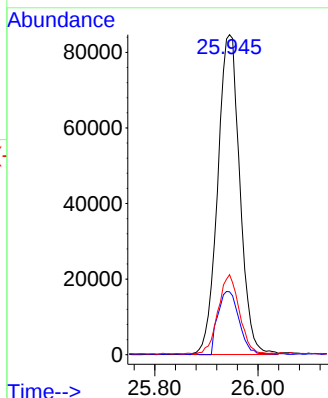

#96
Benzo(g,h,i)perylene
Concen: 4.495 ng/ul
RT: 26.656 min Scan# 4007
Delta R.T. 0.006 min
Lab File: BP006680.D
Acq: 16 Aug 2021 11:13



Tgt Ion:276 Resp: 247903
Ion Ratio Lower Upper
276 100
138 25.7 20.7 31.1
277 23.4 19.0 28.4

