

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
 Data File : BP011536.D
 Acq On : 23 Aug 2022 10:01
 Operator : CG/JU
 Sample : PB146666BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	10	13	27	rVB	26164	40775	2.59%	0.224%
2	3.475	80	83	102	rBV	284675	430690	27.37%	2.365%
3	3.775	130	134	141	rVB	26147	35813	2.28%	0.197%
4	6.399	578	580	584	rBV5	1245	1712	0.11%	0.009%
5	6.734	630	637	653	rBV	332346	525378	33.38%	2.885%
6	6.899	659	665	679	rVB	246876	375721	23.87%	2.063%
7	7.081	690	696	712	rBV	345054	522139	33.18%	2.867%
8	7.546	769	775	787	rVB	299934	475539	30.21%	2.611%
9	8.269	892	898	917	rBV	385242	623612	39.62%	3.424%
10	8.710	965	973	982	rBV	310341	514471	32.69%	2.825%
11	8.857	996	998	1004	rVB7	1101	1784	0.11%	0.010%
12	9.428	1086	1095	1109	rBV	261195	430212	27.33%	2.362%
13	9.963	1179	1186	1202	rBV	369045	615331	39.10%	3.379%
14	10.334	1242	1249	1258	rBV	405513	650646	41.34%	3.572%
15	10.487	1268	1275	1295	rBV	358899	636600	40.45%	3.495%
16	11.957	1517	1525	1531	rBV7	5165	11789	0.75%	0.065%
17	13.193	1733	1735	1739	rVB5	1286	2005	0.13%	0.011%
18	13.645	1804	1812	1823	rBV	706581	945039	60.05%	5.189%
19	13.910	1850	1857	1869	rBV2	707620	997664	63.39%	5.478%
20	14.222	1903	1910	1919	rBV	559027	794209	50.46%	4.361%
21	14.451	1942	1949	1978	rBV	266533	498730	31.69%	2.738%
22	15.228	2072	2081	2089	rBV	885006	1241918	78.91%	6.819%
23	15.363	2098	2104	2114	rBV	324003	441258	28.04%	2.423%
24	15.469	2118	2122	2128	rVV9	5549	10392	0.66%	0.057%
25	16.781	2340	2345	2352	rBV9	1612	3236	0.21%	0.018%
26	16.992	2375	2381	2392	rBV	676484	924287	58.73%	5.075%
27	17.092	2392	2398	2414	rVB2	1010015	1415782	89.96%	7.774%
28	17.610	2483	2486	2487	rBV3	1426	1611	0.10%	0.009%
29	17.663	2493	2495	2496	rBV2	1563	1580	0.10%	0.009%
30	17.681	2496	2498	2501	rVV4	1482	2025	0.13%	0.011%
31	18.316	2602	2606	2607	rBV4	1317	1755	0.11%	0.010%
32	18.645	2658	2662	2665	rBV5	1635	3018	0.19%	0.017%
33	18.933	2707	2711	2715	rBV4	11900	16376	1.04%	0.090%
34	18.998	2719	2722	2730	rVB2	11184	18287	1.16%	0.100%
35	19.357	2777	2783	2793	rBV	1245046	1573860	100.00%	8.642%
36	21.122	3078	3083	3090	rBV	792285	970688	61.68%	5.330%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
Data File : BP011536.D
Acq On : 23 Aug 2022 10:01
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Title : SVOA CALIBRATION

37	23.263	3441	3447	3454	rBV2	793611	1497538	95.15%	8.222%
38	23.410	3466	3472	3483	rVB2	512735	959233	60.95%	5.267%




Sum of corrected areas: 18212703

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
Data File : BP011536.D
Acq On : 23 Aug 2022 10:01
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

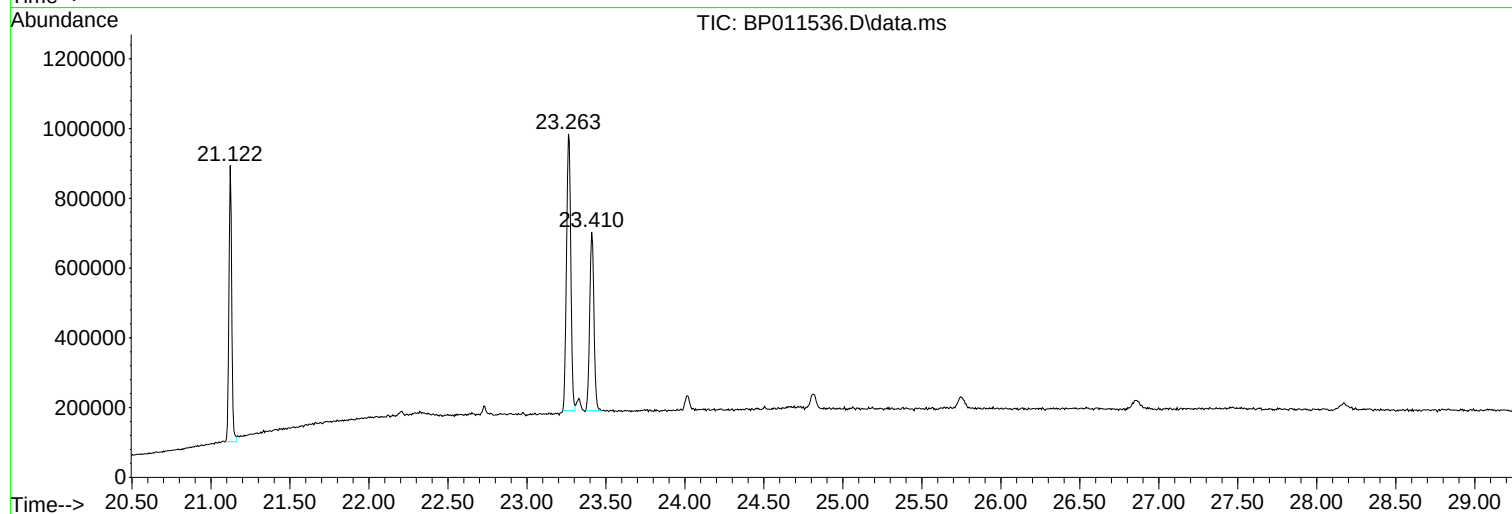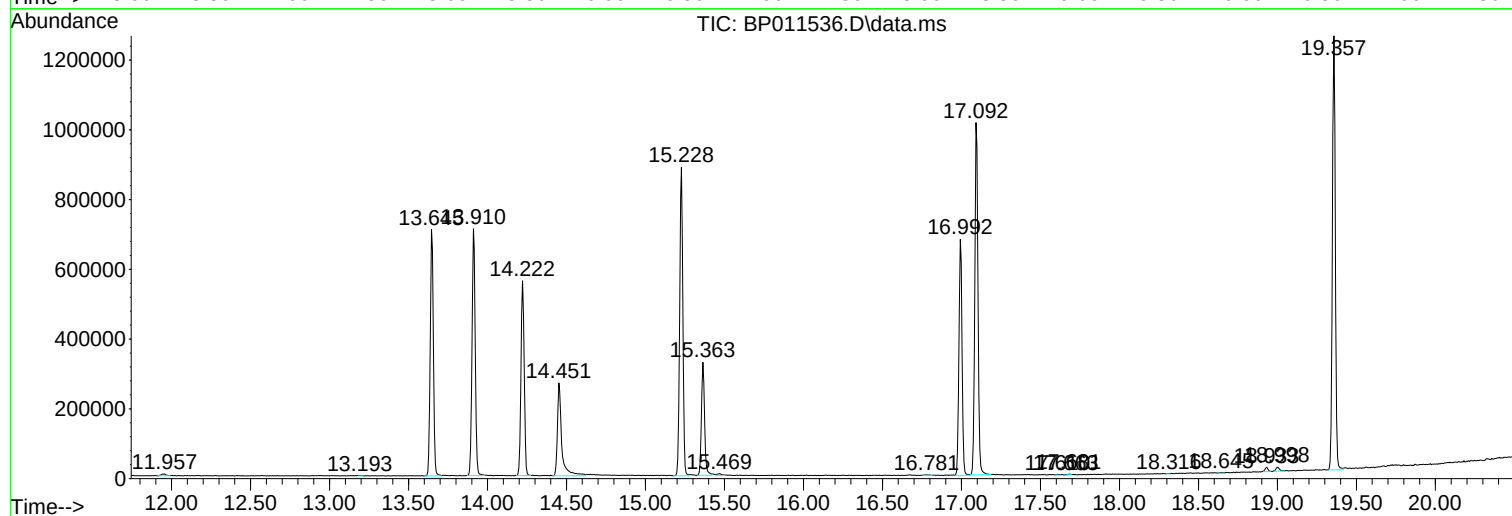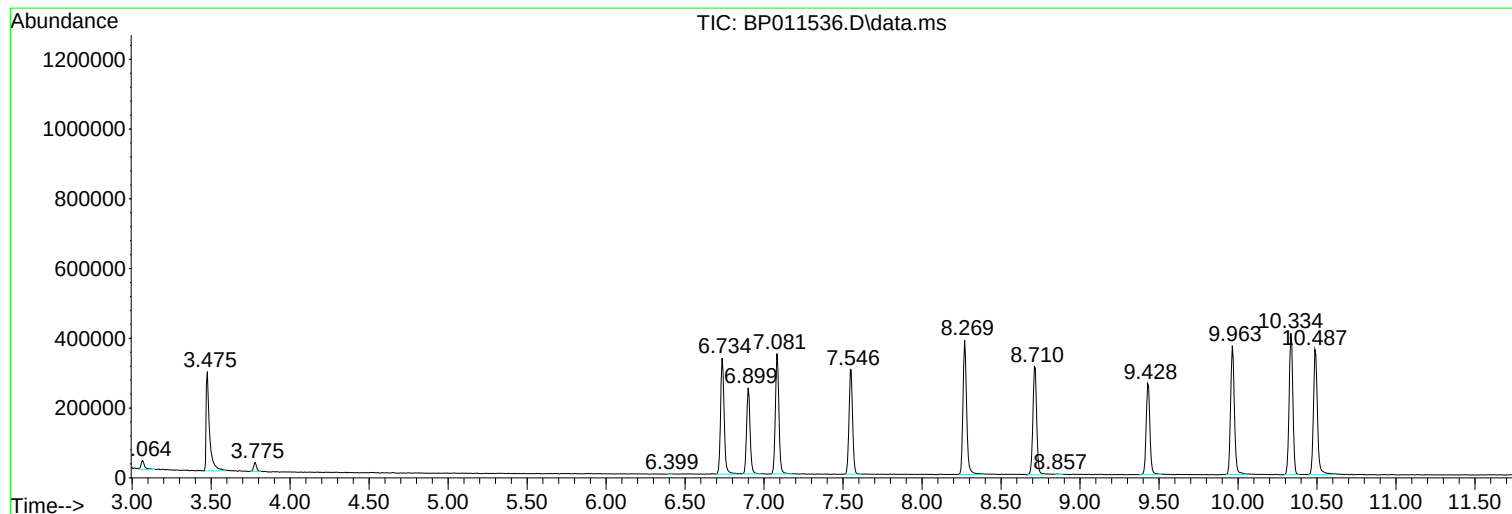

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
Data File : BP011536.D
Acq On : 23 Aug 2022 10:01
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
Data File : BP011536.D
Acq On : 23 Aug 2022 10:01
Operator : CG/JU
Sample : PB146666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc