

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
 Data File : BP011540.D
 Acq On : 23 Aug 2022 14:02
 Operator : CG/JU
 Sample : PB146668BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	10	13	20	rVB	35452	49154	3.17%	0.254%
2	3.475	79	83	98	rBV	354354	542997	35.00%	2.802%
3	3.775	130	134	141	rVB	30700	42156	2.72%	0.218%
4	6.187	539	544	550	rBV9	1873	3556	0.23%	0.018%
5	6.287	557	561	564	rBV5	1184	1790	0.12%	0.009%
6	6.393	576	579	583	rVB6	1253	2034	0.13%	0.010%
7	6.734	631	637	649	rBV	361199	579008	37.32%	2.988%
8	6.904	660	666	678	rVB	272293	419872	27.06%	2.167%
9	7.087	690	697	707	rBV	361217	576816	37.18%	2.977%
10	7.552	769	776	784	rBV	341651	516987	33.32%	2.668%
11	7.769	809	813	814	rBV4	1883	1693	0.11%	0.009%
12	8.275	892	899	910	rBV	417528	677425	43.67%	3.496%
13	8.481	932	934	939	rBV6	1450	1836	0.12%	0.009%
14	8.716	967	974	986	rBV	356572	571719	36.85%	2.951%
15	9.087	1031	1037	1039	rVV7	1273	1557	0.10%	0.008%
16	9.163	1049	1050	1054	rBV4	1545	1883	0.12%	0.010%
17	9.434	1088	1096	1107	rBV	303835	480481	30.97%	2.480%
18	9.822	1159	1162	1164	rBV3	1566	1787	0.12%	0.009%
19	9.875	1167	1171	1175	rVV7	1391	2344	0.15%	0.012%
20	9.969	1180	1187	1200	rVV	394731	663119	42.74%	3.422%
21	10.057	1200	1202	1205	rVB4	2022	1947	0.13%	0.010%
22	10.204	1226	1227	1232	rVB5	1416	1809	0.12%	0.009%
23	10.340	1241	1250	1257	rBV	429646	697239	44.94%	3.599%
24	10.493	1267	1276	1286	rBV	399922	680939	43.89%	3.514%
25	11.057	1370	1372	1375	rVB4	1703	1620	0.10%	0.008%
26	11.175	1385	1392	1393	rBV7	1539	3495	0.23%	0.018%
27	11.375	1422	1426	1427	rBV4	1485	1554	0.10%	0.008%
28	11.469	1439	1442	1448	rBV7	2301	6092	0.39%	0.031%
29	11.528	1450	1452	1458	rVB6	5577	8585	0.55%	0.044%
30	11.792	1493	1497	1500	rBV5	1243	2474	0.16%	0.013%
31	11.822	1500	1502	1508	rVB7	2807	3935	0.25%	0.020%
32	11.945	1518	1523	1532	rVB2	6078	11849	0.76%	0.061%
33	12.504	1614	1618	1619	rBV4	1904	1856	0.12%	0.010%
34	12.534	1619	1623	1624	rBV3	1955	2075	0.13%	0.011%
35	13.104	1715	1720	1721	rBV4	1913	2599	0.17%	0.013%
36	13.151	1725	1728	1731	rVB5	2298	3134	0.20%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
 Data File : BP011540.D
 Acq On : 23 Aug 2022 14:02
 Operator : CG/JU
 Sample : PB146668BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

37	13.463	1779	1781	1784	rBV3	1431	1899	0.12%	0.010%
38	13.504	1784	1788	1795	rVV9	2329	5057	0.33%	0.026%
39	13.575	1795	1800	1801	rVV5	3417	5143	0.33%	0.027%
40	13.651	1801	1813	1824	rVV	738607	1022855	65.93%	5.279%
41	13.739	1824	1828	1832	rVB7	1196	1812	0.12%	0.009%
42	13.916	1851	1858	1869	rVV	733413	1047785	67.54%	5.408%
43	14.175	1900	1902	1904	rBV3	2322	2513	0.16%	0.013%
44	14.228	1905	1911	1925	rVB	585529	850827	54.84%	4.391%
45	14.457	1944	1950	1965	rBV	301388	509725	32.86%	2.631%
46	14.675	1985	1987	1993	rVV7	2541	3555	0.23%	0.018%
47	14.751	1997	2000	2006	rVB7	1675	2878	0.19%	0.015%
48	15.033	2042	2048	2050	rBV6	2997	4199	0.27%	0.022%
49	15.086	2055	2057	2061	rVB5	3120	3234	0.21%	0.017%
50	15.145	2064	2067	2069	rBV4	1261	1679	0.11%	0.009%
51	15.233	2072	2082	2096	rVB	932045	1338483	86.28%	6.908%
52	15.369	2099	2105	2119	rBV	386178	513399	33.09%	2.650%
53	15.469	2119	2122	2129	rVB6	5017	7582	0.49%	0.039%
54	15.810	2178	2180	2184	rVV5	2144	3065	0.20%	0.016%
55	15.875	2187	2191	2192	rVV4	1401	2003	0.13%	0.010%
56	15.898	2192	2195	2199	rVV6	2406	4855	0.31%	0.025%
57	15.969	2202	2207	2213	rVB8	4127	8346	0.54%	0.043%
58	16.022	2213	2216	2220	rBV6	1390	2034	0.13%	0.010%
59	16.133	2224	2235	2241	rVV5	13917	27639	1.78%	0.143%
60	16.228	2248	2251	2254	rBV5	1407	2053	0.13%	0.011%
61	16.480	2286	2294	2300	rBV2	6248	11174	0.72%	0.058%
62	16.710	2330	2333	2337	rBV6	1613	2285	0.15%	0.012%
63	16.780	2339	2345	2352	rVV10	2882	6498	0.42%	0.034%
64	16.939	2366	2372	2376	rBV6	9028	16309	1.05%	0.084%
65	16.998	2376	2382	2391	rVV	668965	943675	60.83%	4.870%
66	17.104	2393	2400	2413	rVV	1024806	1446821	93.26%	7.467%
67	17.445	2456	2458	2461	rVV4	1475	2139	0.14%	0.011%
68	17.516	2465	2470	2473	rBV7	2119	4333	0.28%	0.022%
69	17.563	2473	2478	2485	rVB6	6001	10986	0.71%	0.057%
70	17.692	2496	2500	2507	rVB10	7214	11524	0.74%	0.059%
71	17.922	2535	2539	2541	rBV5	2840	4275	0.28%	0.022%
72	18.074	2562	2565	2567	rBV4	1797	2149	0.14%	0.011%
73	18.198	2584	2586	2590	rBV4	1283	1775	0.11%	0.009%
74	18.245	2592	2594	2597	rBV4	1458	1749	0.11%	0.009%
75	18.380	2613	2617	2622	rVV7	3883	7876	0.51%	0.041%
76	18.445	2624	2628	2633	rVV7	2915	4752	0.31%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
 Data File : BP011540.D
 Acq On : 23 Aug 2022 14:02
 Operator : CG/JU
 Sample : PB146668BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Title : SVOA CALIBRATION

77	18.492	2633	2636	2640	rVV5	2945	4129	0.27%	0.021%
78	18.580	2649	2651	2653	rBV3	1544	1704	0.11%	0.009%
79	18.663	2661	2665	2666	rBV3	1729	2040	0.13%	0.011%
80	18.939	2707	2712	2719	rBV4	14265	25814	1.66%	0.133%
81	19.010	2719	2724	2728	rBV	14655	19563	1.26%	0.101%
82	19.304	2772	2774	2775	rBV2	3030	2135	0.14%	0.011%
83	19.363	2779	2784	2793	rVV	1211725	1551401	100.00%	8.007%
84	21.133	3080	3085	3092	rBV	754390	936044	60.34%	4.831%
85	23.280	3443	3450	3456	rBV2	791106	1466181	94.51%	7.567%
86	23.427	3469	3475	3487	rVB2	495983	946365	61.00%	4.884%




Sum of corrected areas: 19375732

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
Data File : BP011540.D
Acq On : 23 Aug 2022 14:02
Operator : CG/JU
Sample : PB146668BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

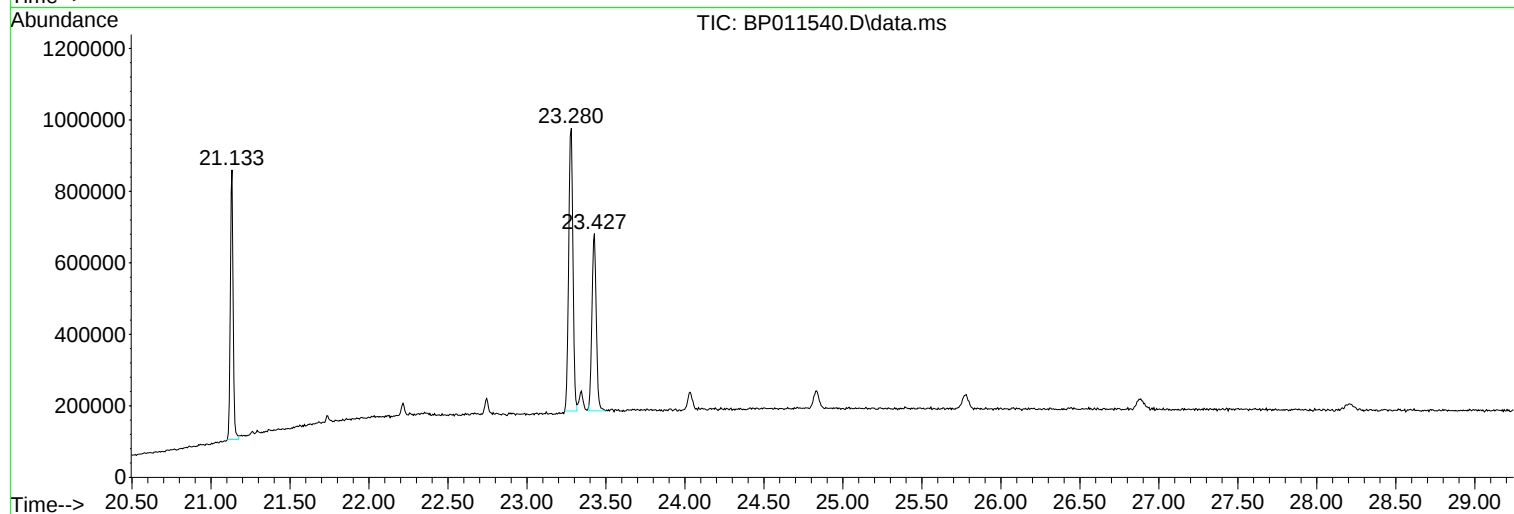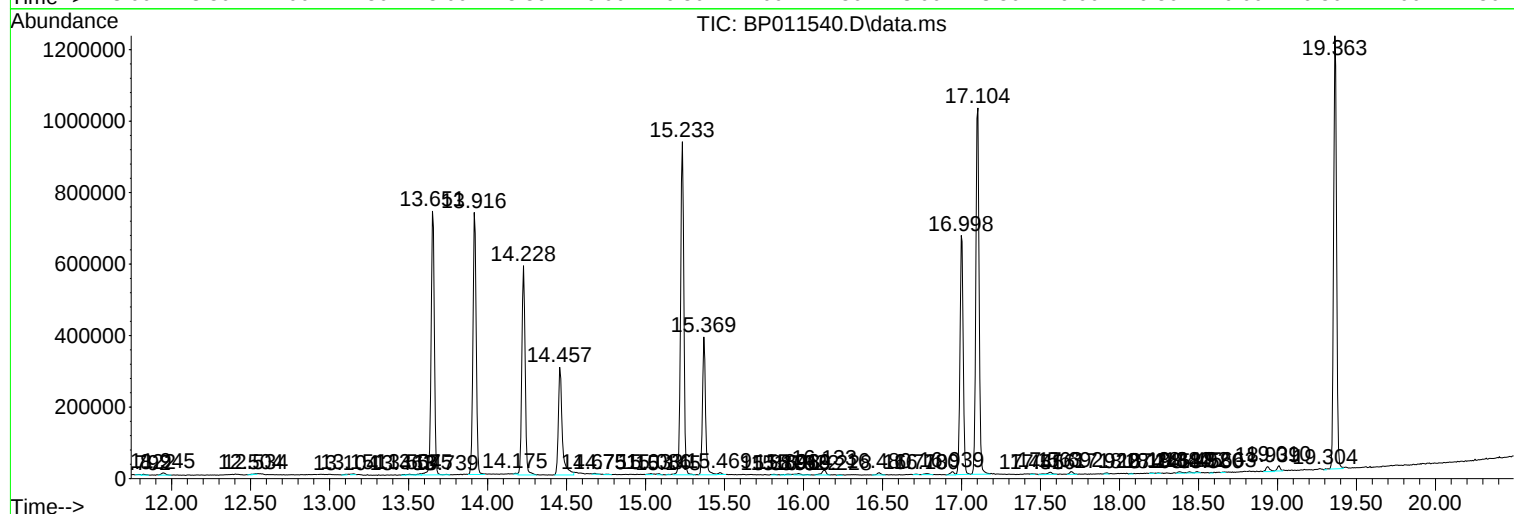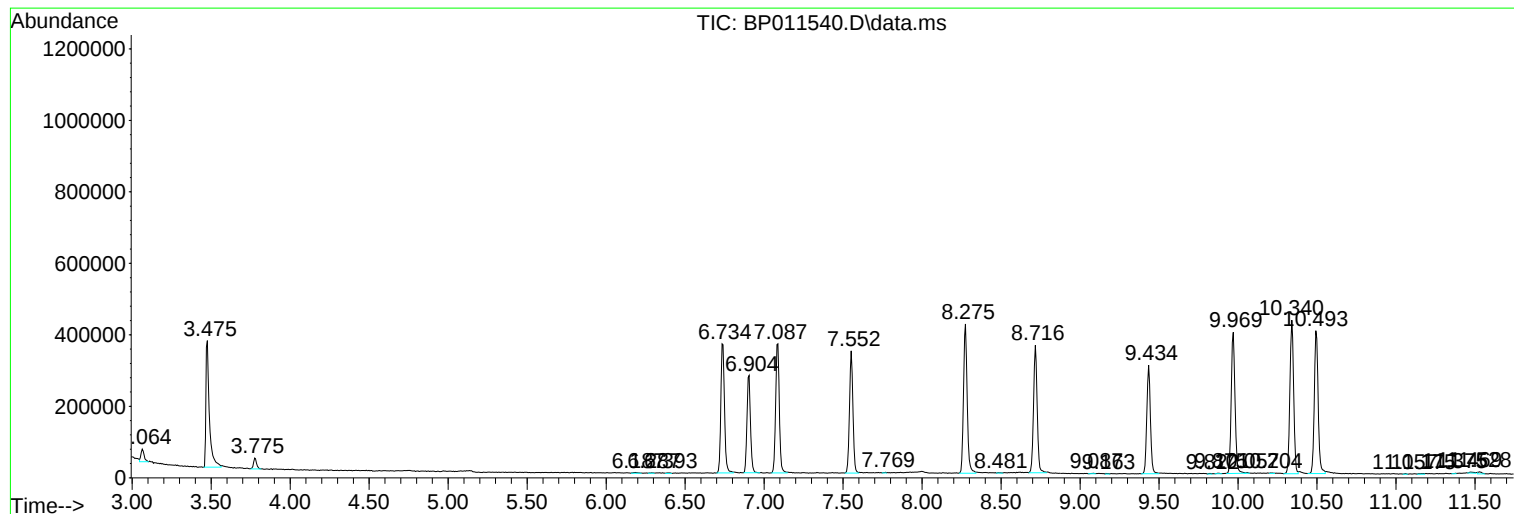

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
Data File : BP011540.D
Acq On : 23 Aug 2022 14:02
Operator : CG/JU
Sample : PB146668BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082322\
Data File : BP011540.D
Acq On : 23 Aug 2022 14:02
Operator : CG/JU
Sample : PB146668BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc