
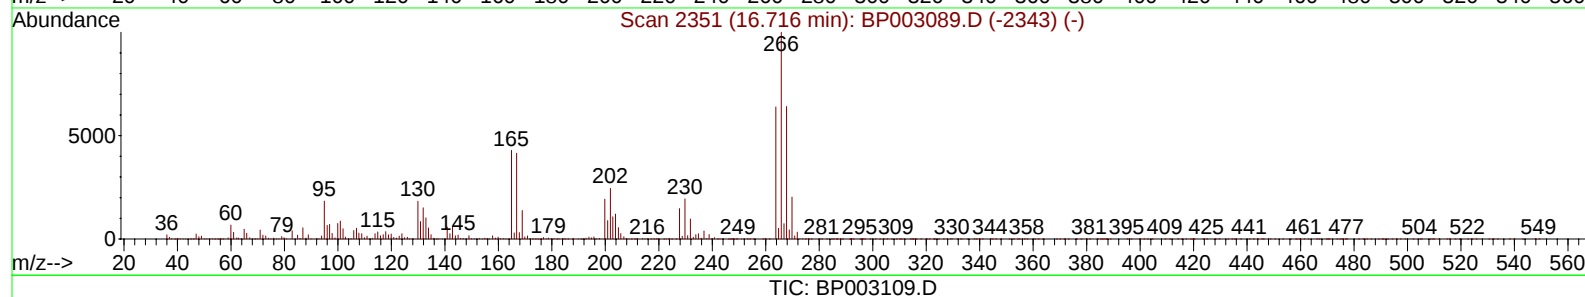
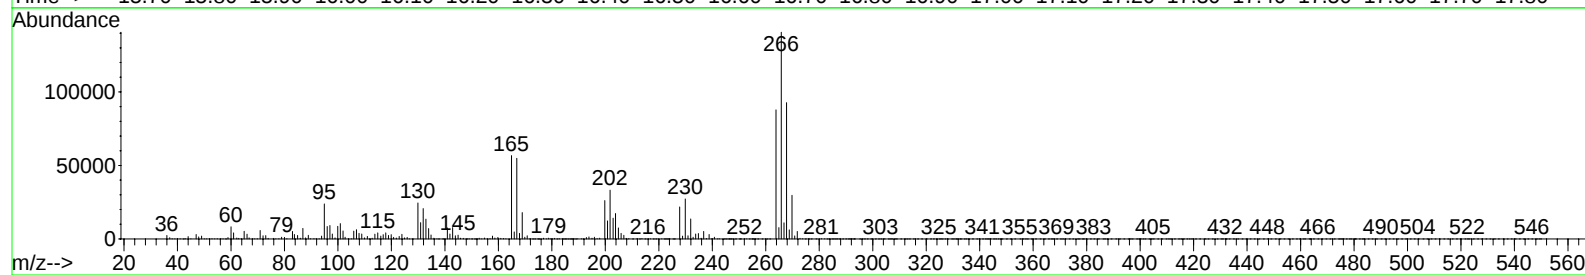


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082620\
 Data File : BP003109.D
 Acq On : 26 Aug 2020 11:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 18:10:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 24 15:32:08 2020
 Response via : Initial Calibration

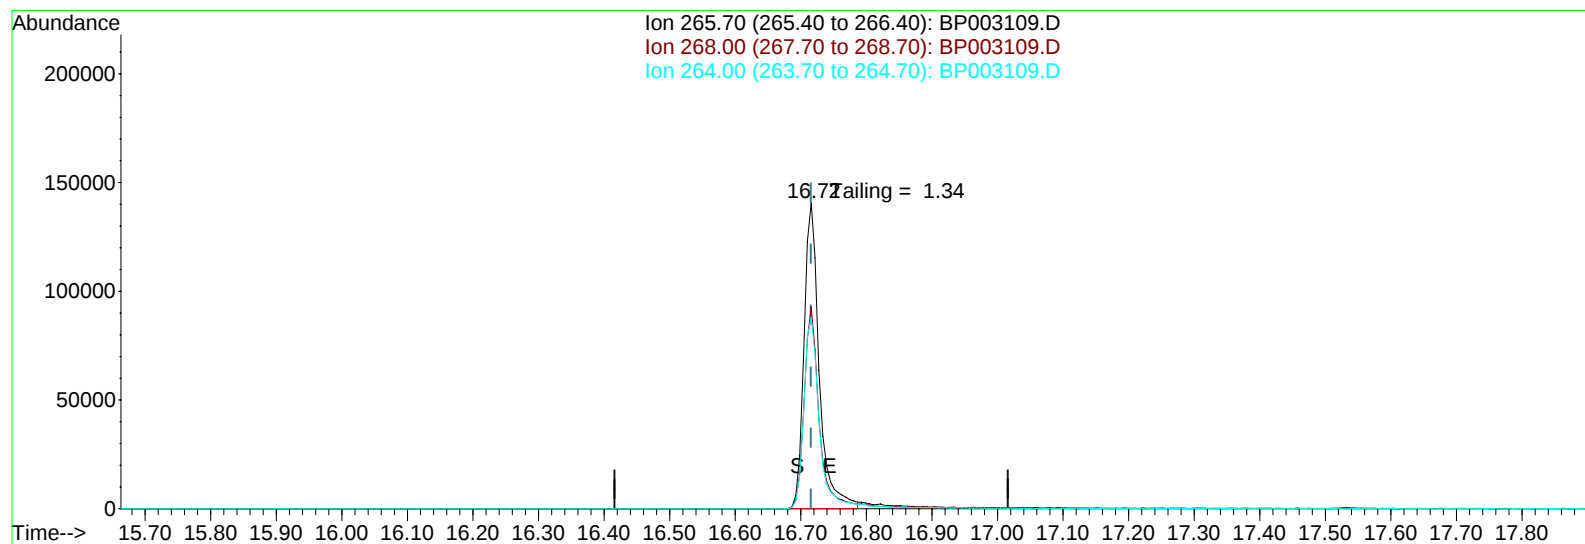

(70) Pentachlorophenol (C)




16.716min (+0.000) 1808995.62ng

response 238698

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	65.95
264.00	63.80	62.49
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP082620\
 Data File : BP003109.D
 Acq On : 26 Aug 2020 11:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 18:10:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 24 15:32:08 2020
 Response via : Initial Calibration

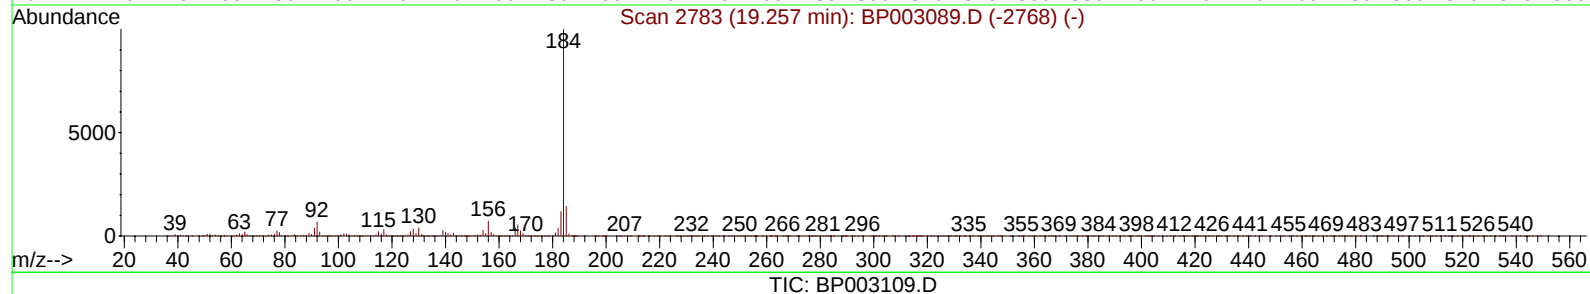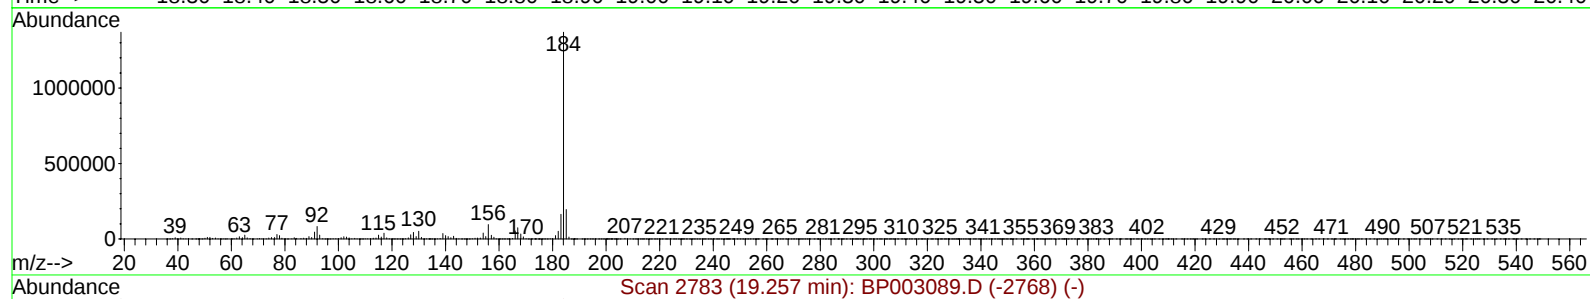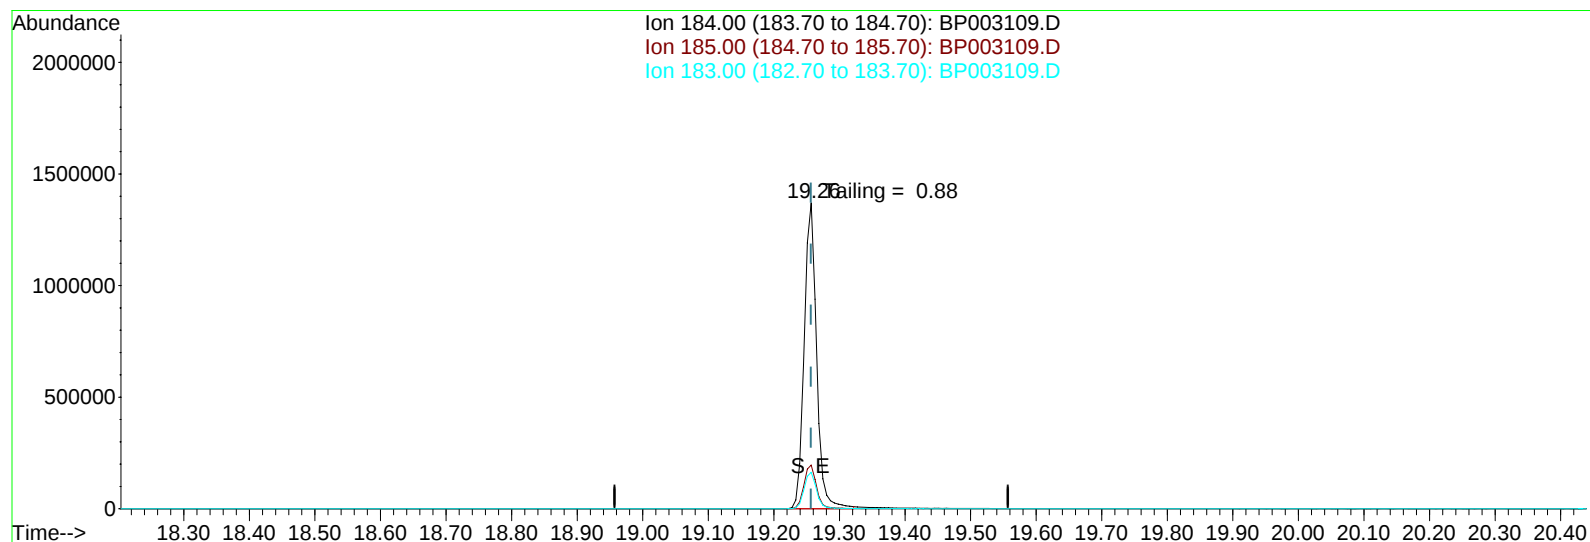

(77) Benzidine

19.257min (+0.000) 606332.98ng

response 1829218

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.28
183.00	11.80	11.93
0.00	0.00	0.00