


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082620\
 Data File : BP003109.D
 Acq On : 26 Aug 2020 11:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 15:32:08 2020

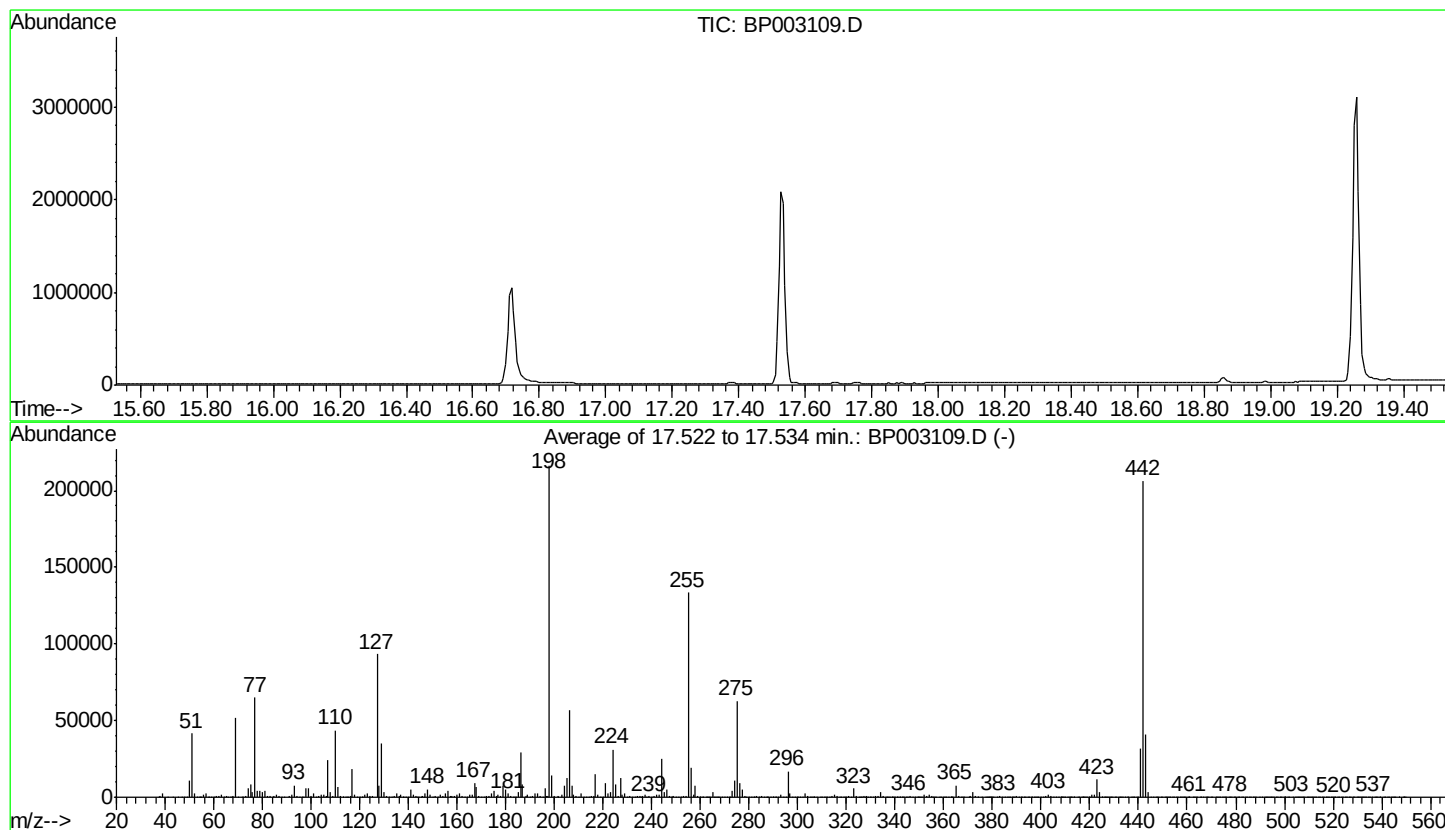

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.2	41430	PASS
68	69	0.00	2	1.9	998	PASS
69	198	0.00	100	23.8	51580	PASS
70	69	0.00	2	0.6	324	PASS
127	198	10	80	43.2	93371	PASS
197	198	0.00	2	0.2	529	PASS
198	198	100	100	100.0	216298	PASS
199	198	5	9	6.7	14596	PASS
275	198	10	60	29.1	62917	PASS
365	198	1	100	3.6	7812	PASS
441	198	0.01	100	14.6	31484	PASS
442	198	50	100	95.5	206642	PASS
443	442	15	24	19.8	40848	PASS