
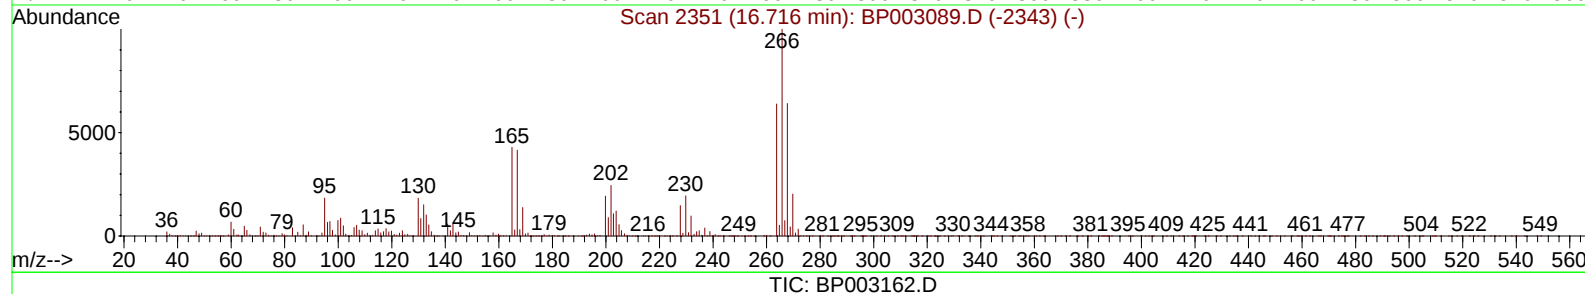
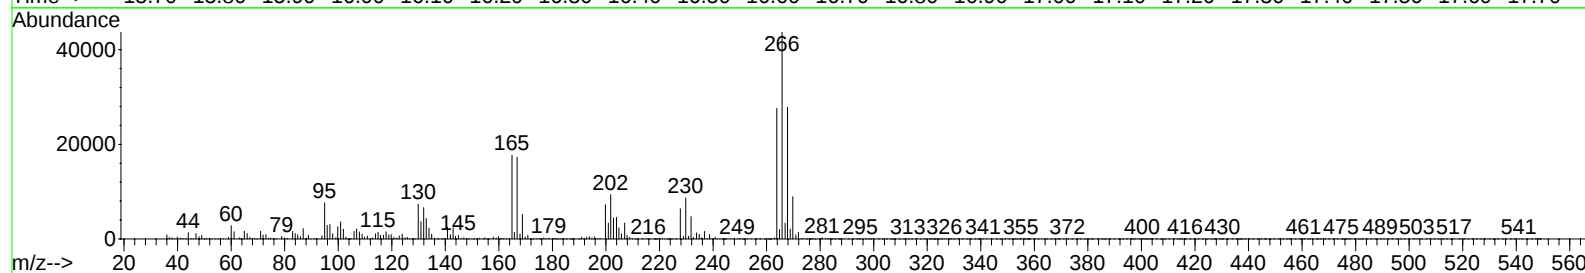


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090120\
Data File : BP003162.D
Acq On : 01 Sep 2020 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 18:29:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 01 14:37:05 2020
Response via : Initial Calibration

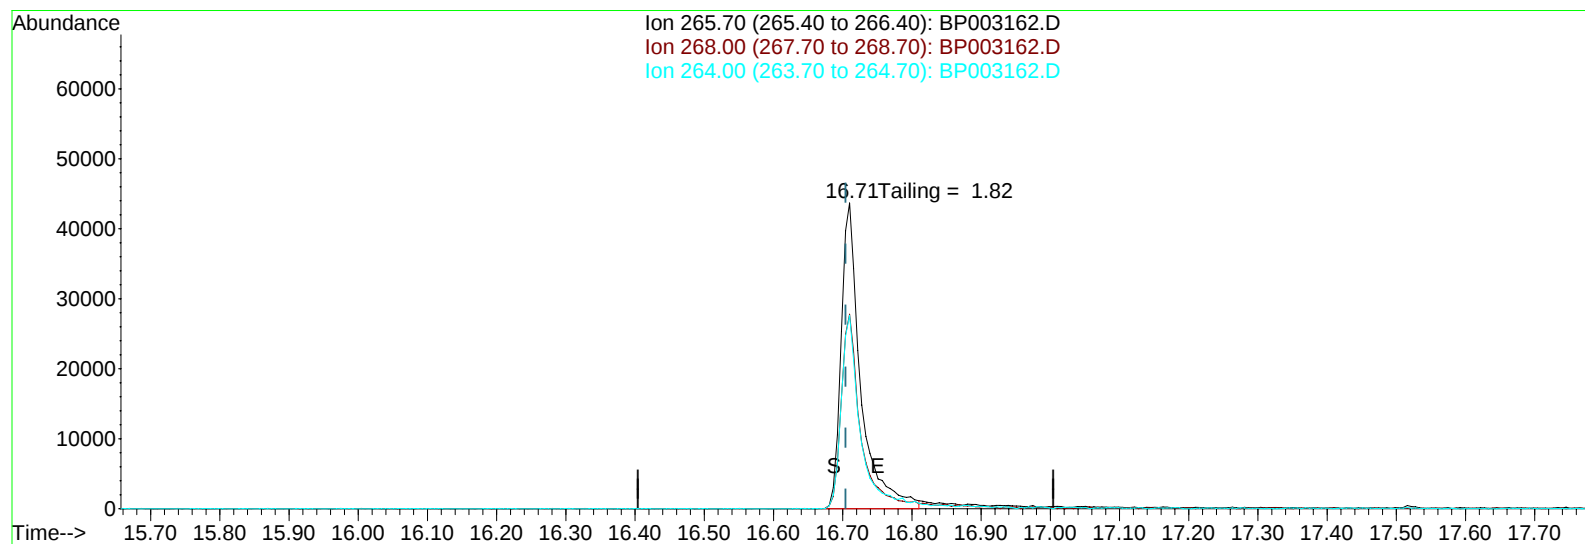

(70) Pentachlorophenol (C)




16.710min (+0.006) 1018906.04ng

response 83228

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.65
264.00	63.30	63.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090120\
 Data File : BP003162.D
 Acq On : 01 Sep 2020 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 01 18:29:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

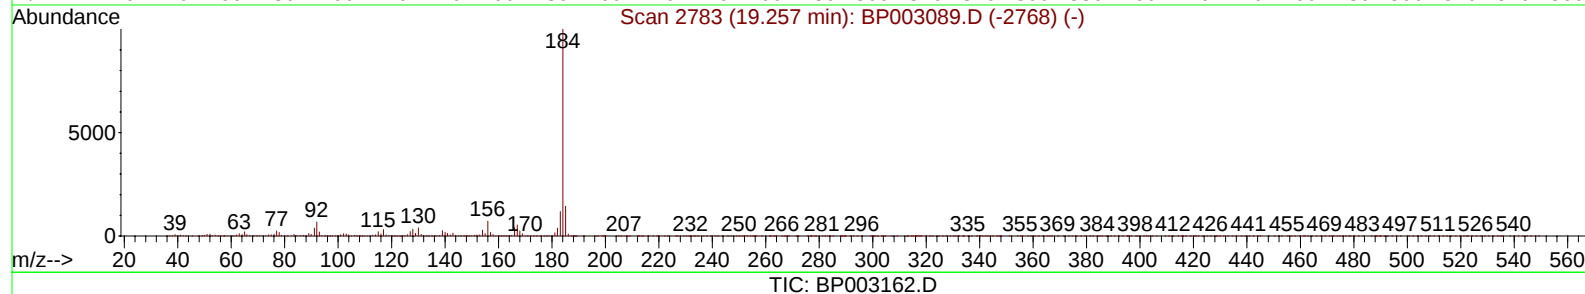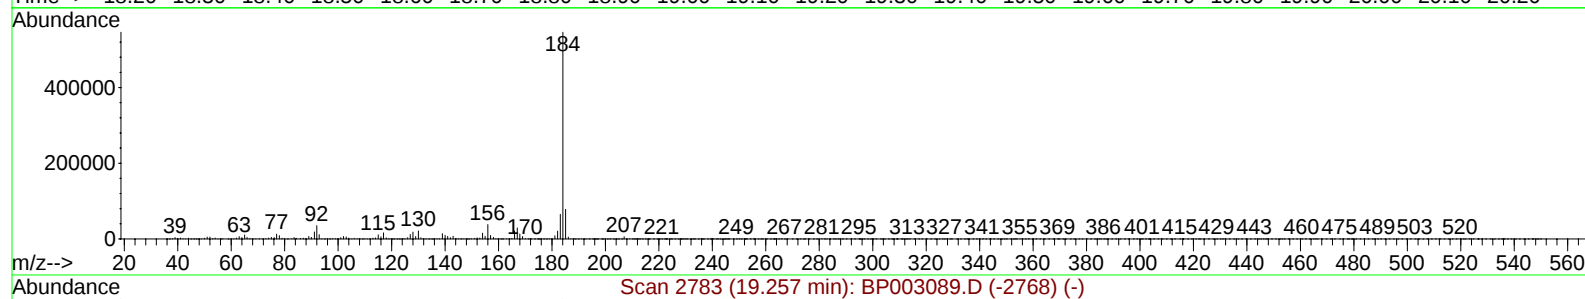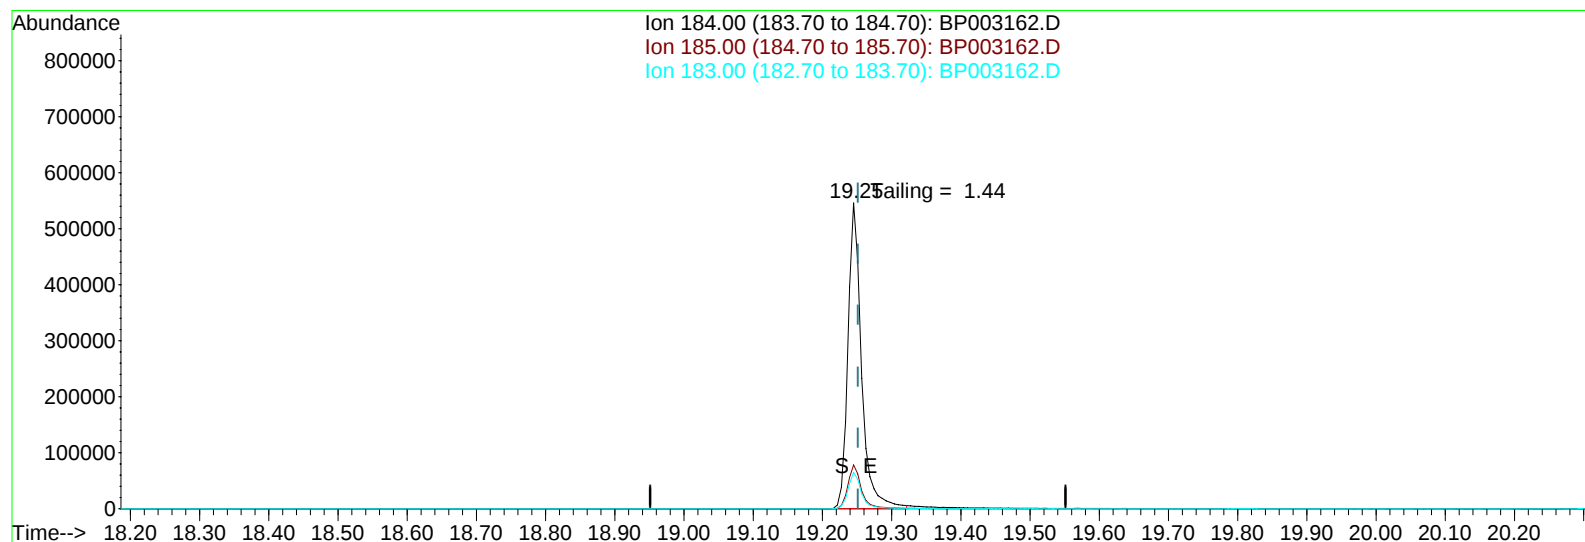

(77) Benzidine

19.245min (-0.006) 1154671.54ng

response 738919

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.35
183.00	12.00	11.93
0.00	0.00	0.00