

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090120\
 Data File : BP003164.D
 Acq On : 01 Sep 2020 13:26
 Operator : CG/JU
 Sample : PB131322BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131322BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	397	404	421	rBV	2732020	3914562	41.59%	9.125%
2	6.840	664	672	686	rBV	2308535	3721948	39.55%	8.676%
3	7.651	801	810	824	rBV	663609	1062006	11.28%	2.475%
4	8.798	996	1005	1020	rBV	1574451	2634438	27.99%	6.141%
5	10.434	1275	1283	1298	rBV	802952	1411167	14.99%	3.289%
6	12.922	1697	1706	1720	rBV	4445376	7008835	74.47%	16.337%
7	14.298	1932	1940	1960	rBV	1200630	1820803	19.35%	4.244%
8	15.792	2187	2194	2223	rBV	2872278	4408229	46.84%	10.275%
9	17.051	2402	2408	2422	rBV	1349395	2016805	21.43%	4.701%
10	19.633	2841	2847	2864	rBV	7396195	9411163	100.00%	21.937%
11	20.939	3065	3069	3077	rVV	169314	219495	2.33%	0.512%
12	21.145	3099	3104	3114	rBV	1869115	2433263	25.86%	5.672%
13	21.263	3120	3124	3131	rBV	80050	121183	1.29%	0.282%
14	23.386	3477	3485	3496	rBV2	1425679	2717446	28.87%	6.334%


Sum of corrected areas: 42901343

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090120\
Data File : BP003164.D
Acq On : 01 Sep 2020 13:26
Operator : CG/JU
Sample : PB131322BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131322BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

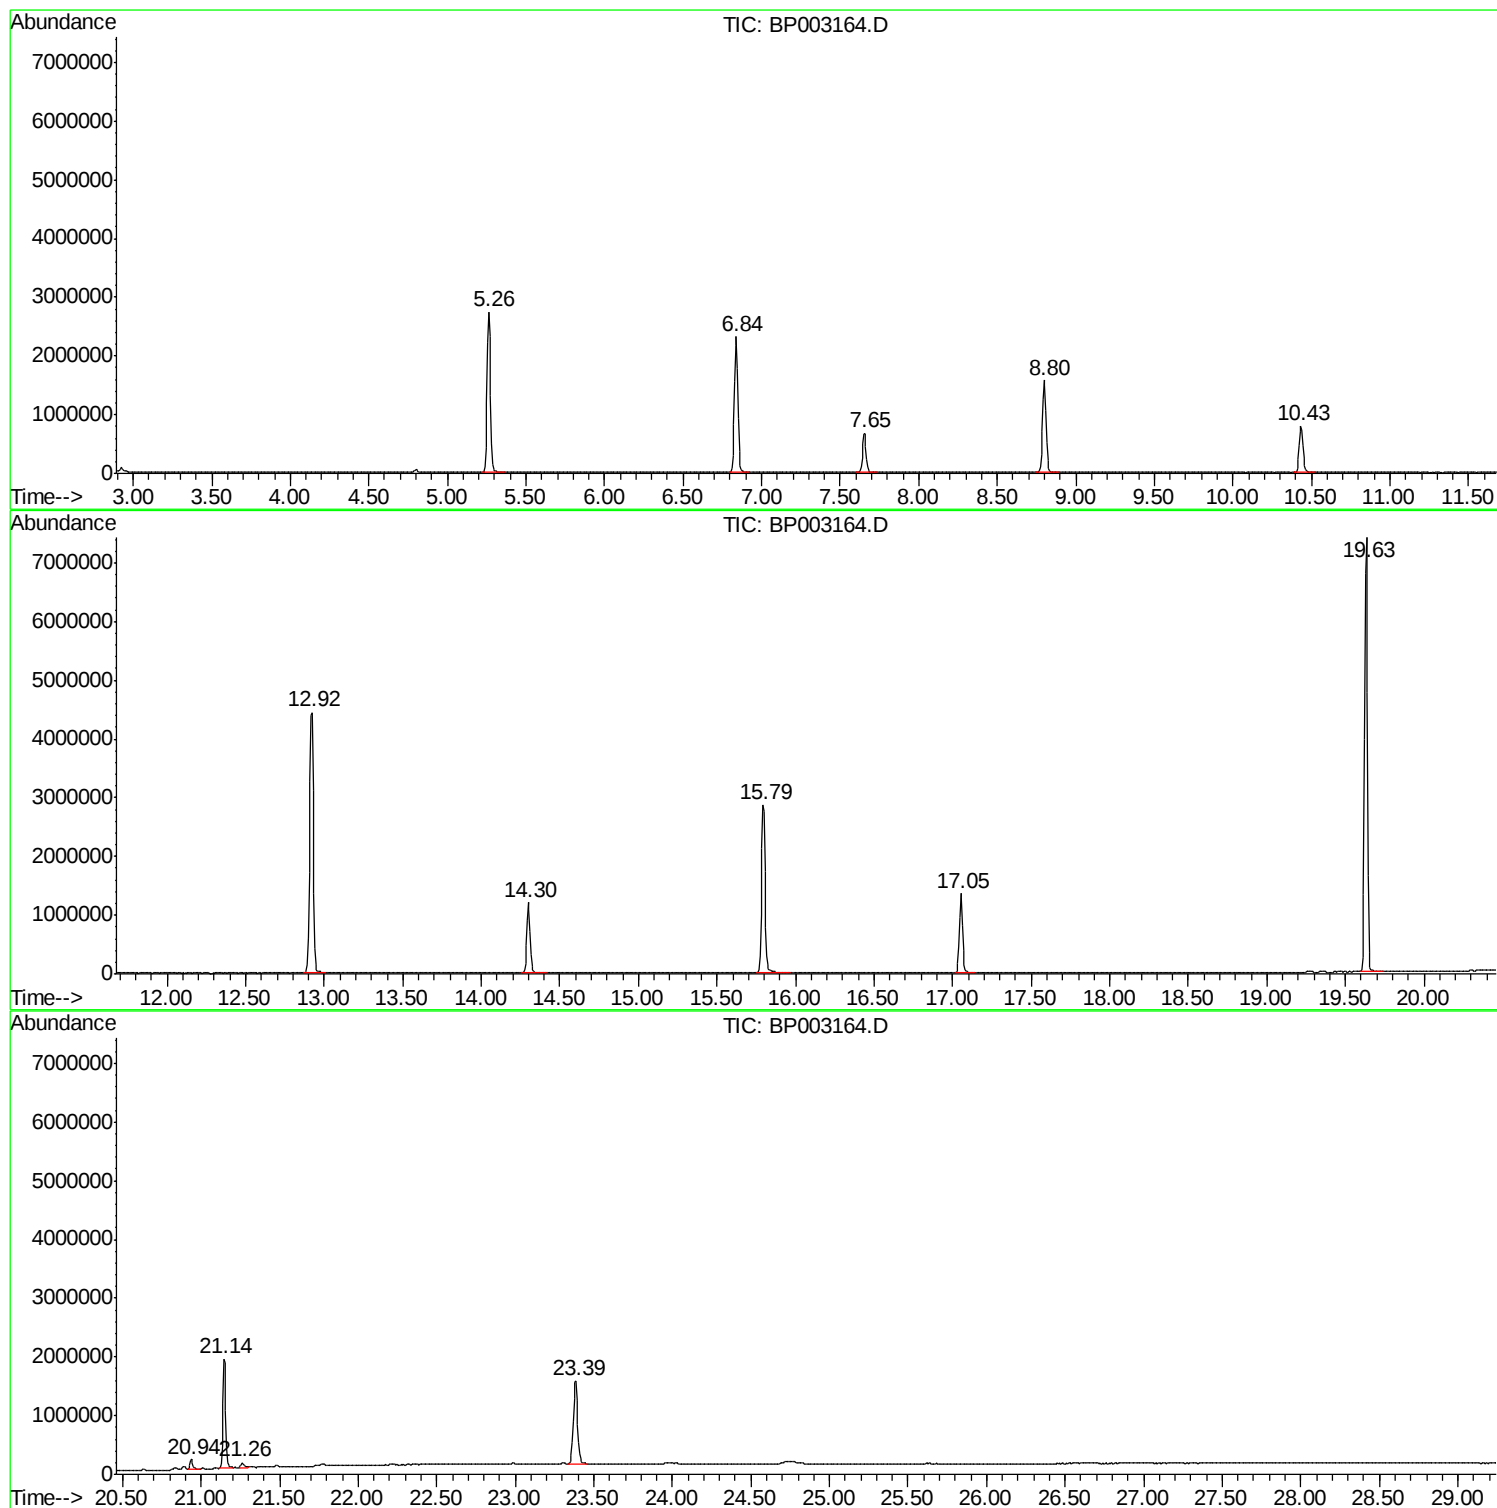

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090120\
Data File : BP003164.D
Acq On : 01 Sep 2020 13:26
Operator : CG/JU
Sample : PB131322BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131322BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090120\
Data File : BP003164.D
Acq On : 01 Sep 2020 13:26
Operator : CG/JU
Sample : PB131322BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131322BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc