


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP090120\
 Data File : BP003162.D
 Acq On : 01 Sep 2020 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

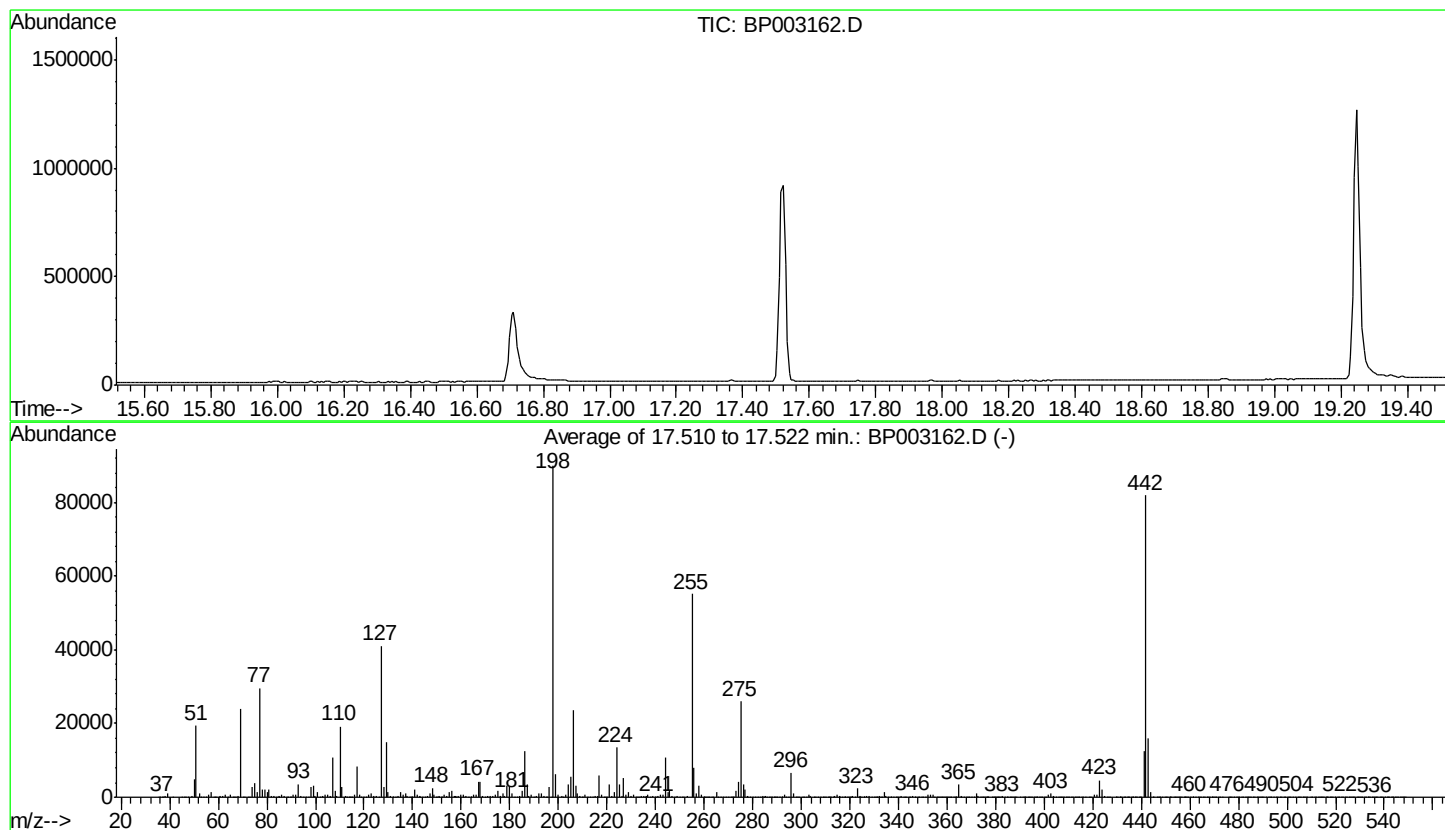

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	19354	PASS
68	69	0.00	2	2.0	473	PASS
69	198	0.00	100	26.5	23865	PASS
70	69	0.00	2	0.5	131	PASS
127	198	10	80	45.7	41146	PASS
197	198	0.00	2	0.2	147	PASS
198	198	100	100	100.0	90016	PASS
199	198	5	9	7.0	6290	PASS
275	198	10	60	28.8	25909	PASS
365	198	1	100	3.8	3389	PASS
441	198	0.01	100	14.0	12583	PASS
442	198	50	100	91.1	81970	PASS
443	442	15	24	19.4	15865	PASS