
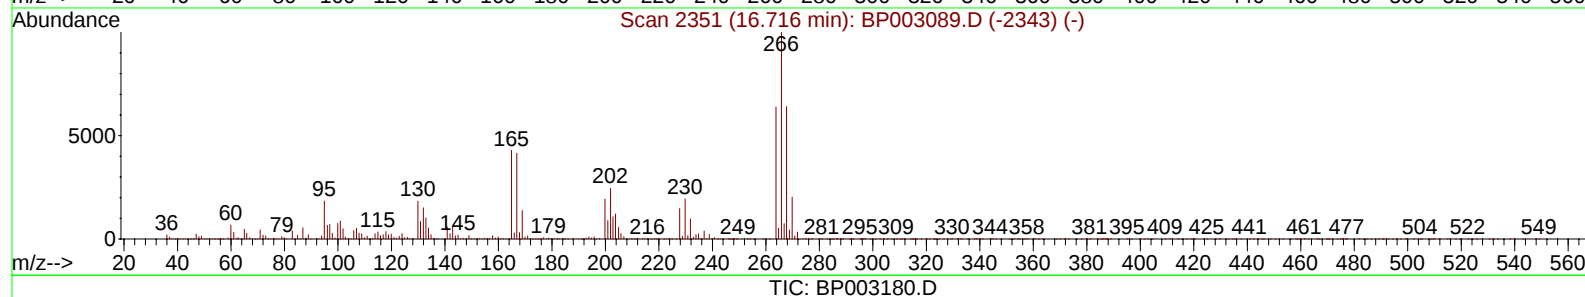
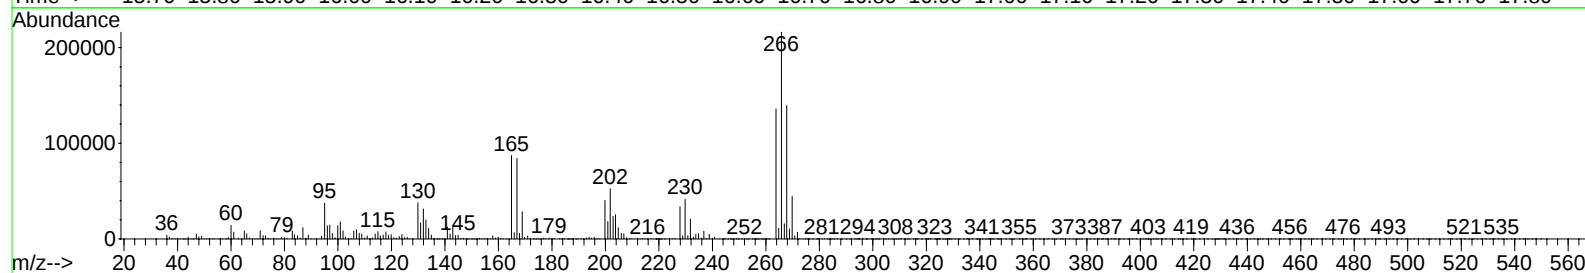


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP090220\
 Data File : BP003180.D
 Acq On : 02 Sep 2020 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 18:31:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

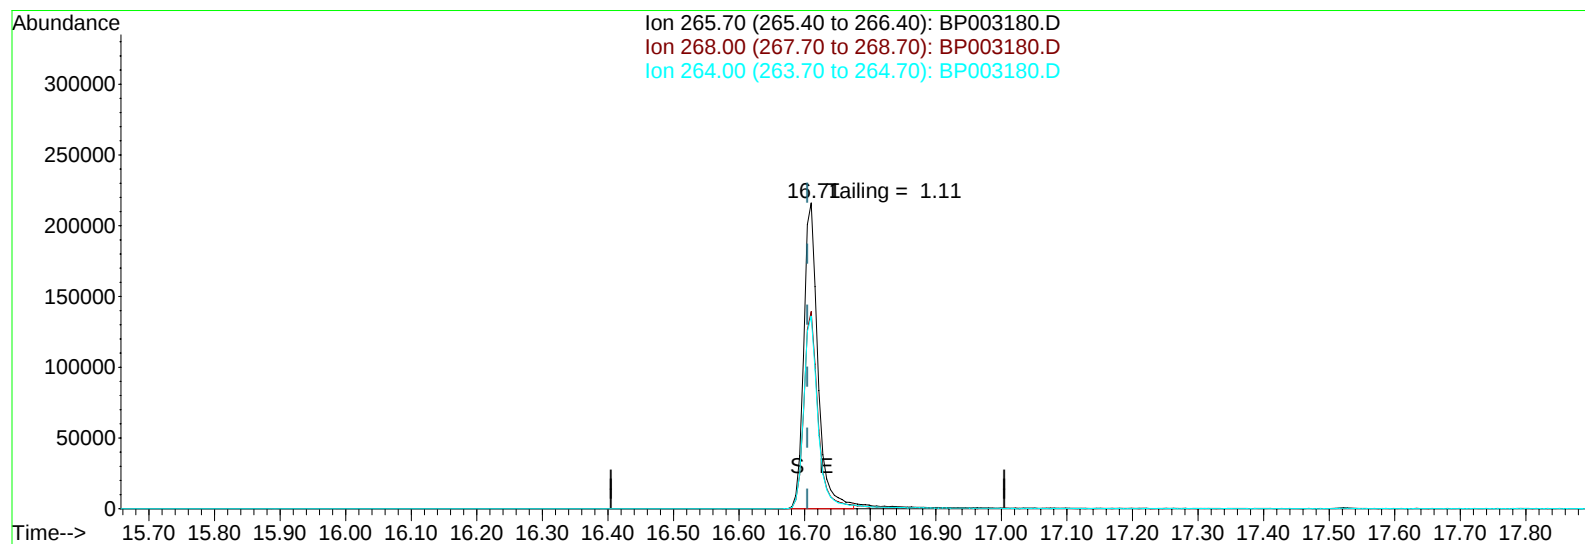

(70) Pentachlorophenol (C)

16.710min (+0.006) 119048.46ng

response 337359

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.48
264.00	63.30	62.94
0.00	0.00	0.00

