


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP090220\  
 Data File : BP003180.D  
 Acq On : 02 Sep 2020 11:14  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Sep 01 14:37:05 2020

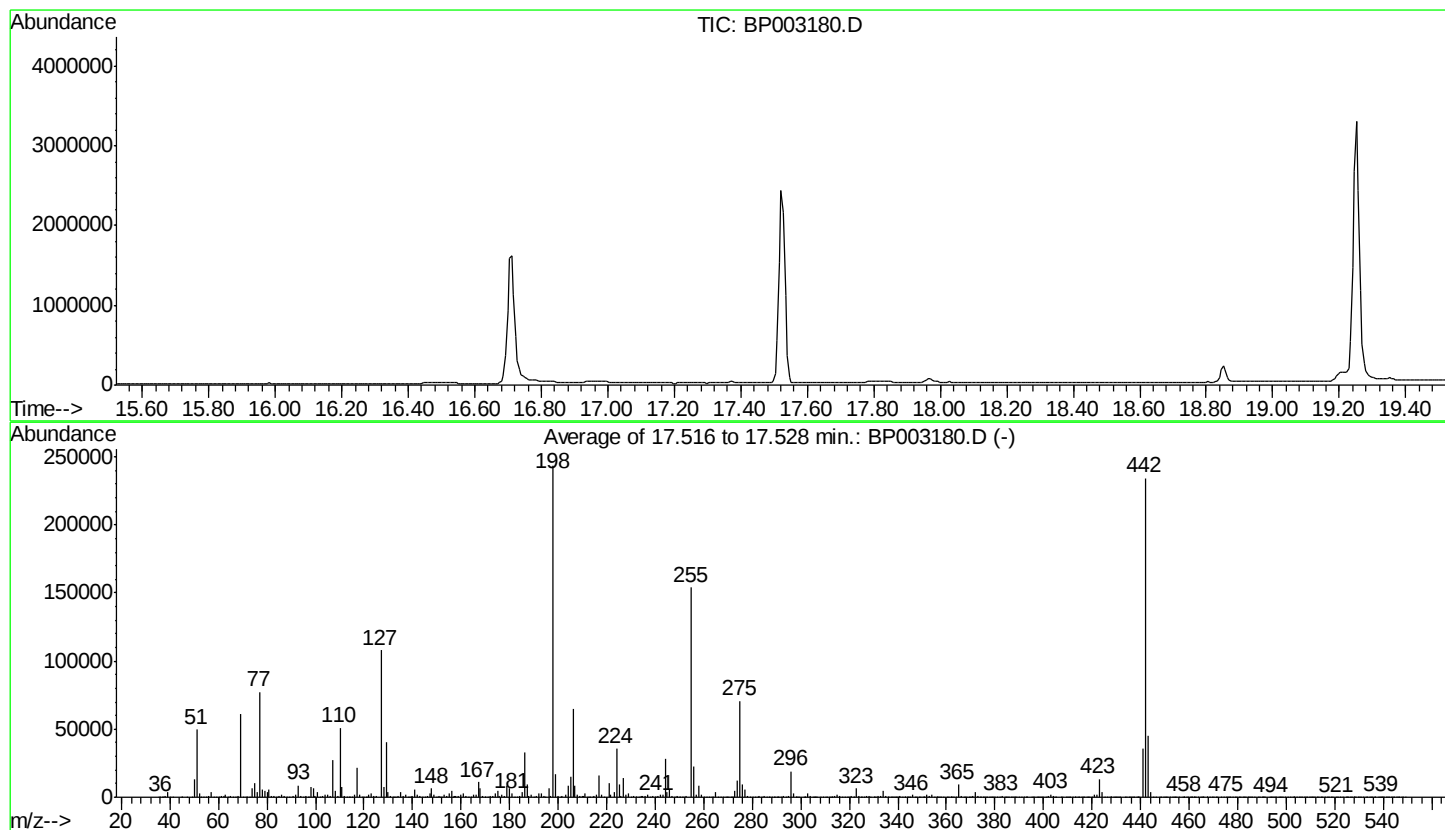

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 20.4      | 49673   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 1107    | PASS             |
| 69          | 198          | 0.00         | 100          | 25.0      | 60842   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 219     | PASS             |
| 127         | 198          | 10           | 80           | 44.3      | 107820  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 587     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 243470  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 16577   | PASS             |
| 275         | 198          | 10           | 60           | 29.0      | 70698   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 9038    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.6      | 35581   | PASS             |
| 442         | 198          | 50           | 100          | 96.3      | 234405  | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 45282   | PASS             |