
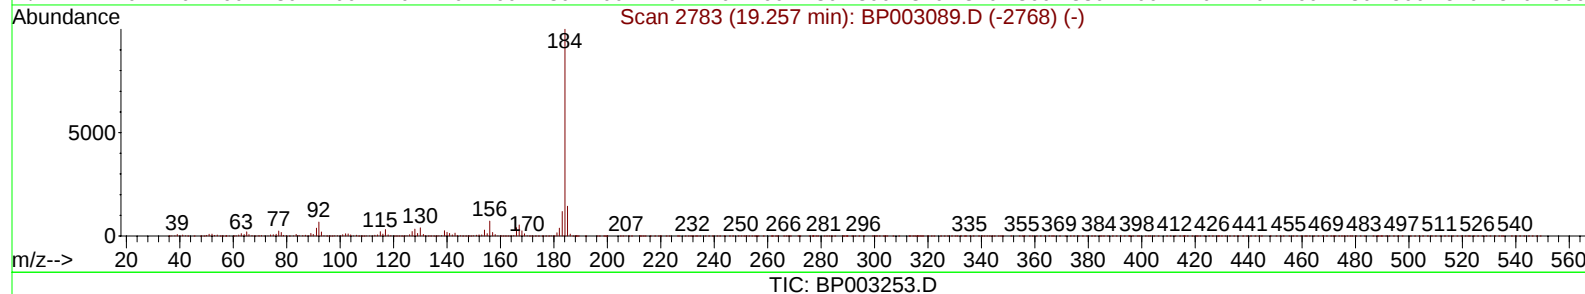
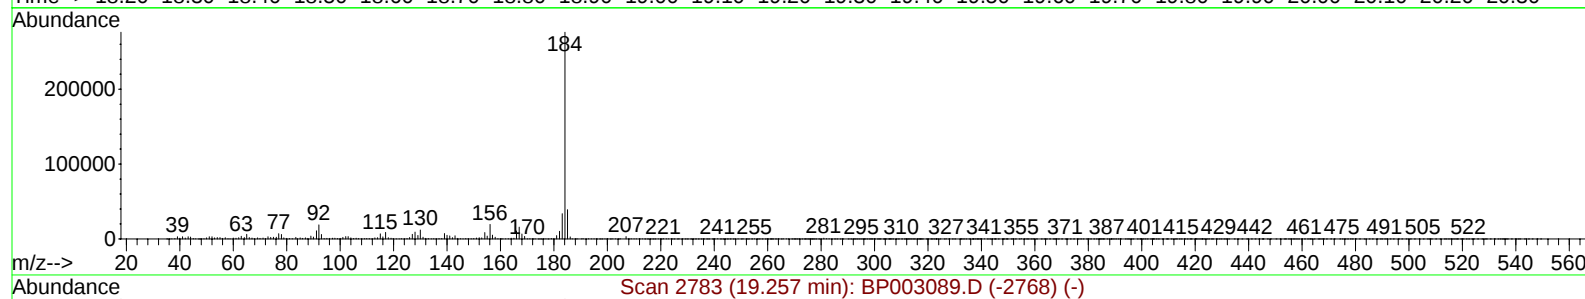


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
 Data File : BP003253.D
 Acq On : 11 Sep 2020 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 11:07:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

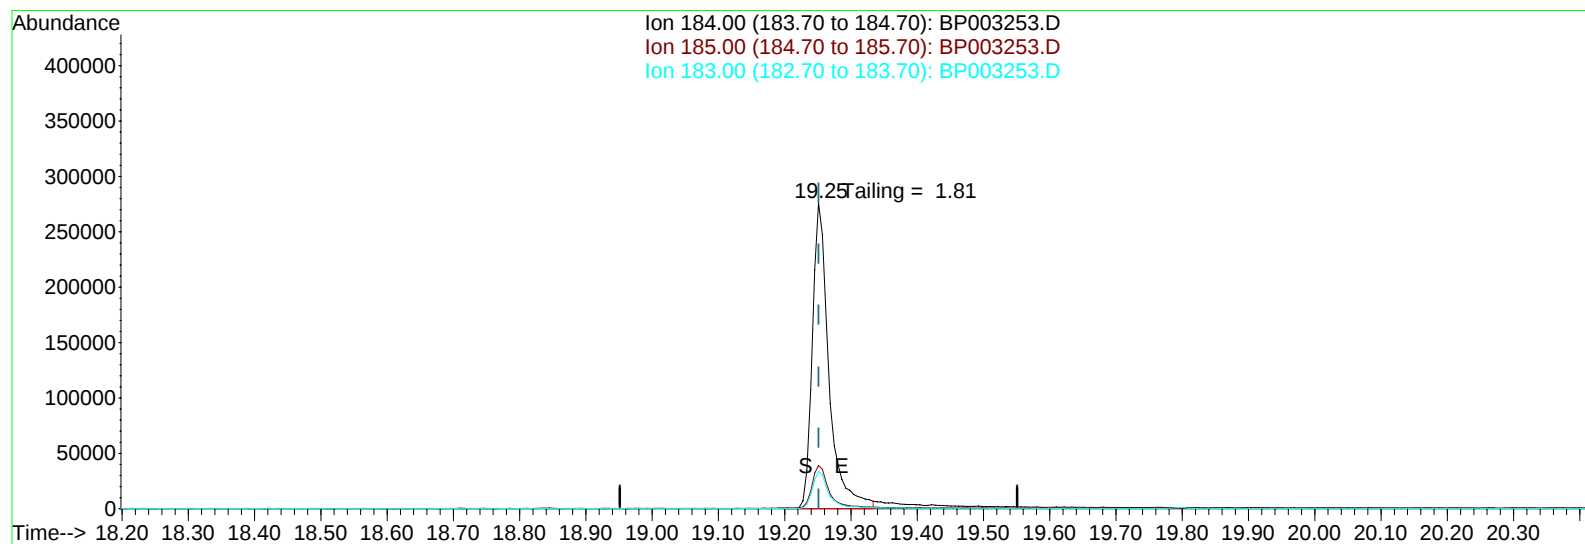

(77) Benzidine




19.251min (-0.000) 8394.44ng

response 499589

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.15
183.00	12.00	12.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
 Data File : BP003253.D
 Acq On : 11 Sep 2020 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 11:07:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 01 14:37:05 2020
 Response via : Initial Calibration

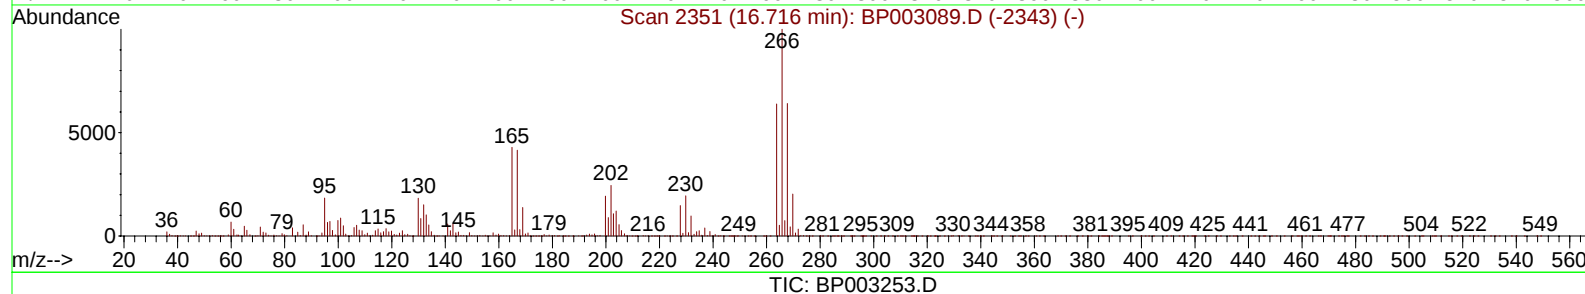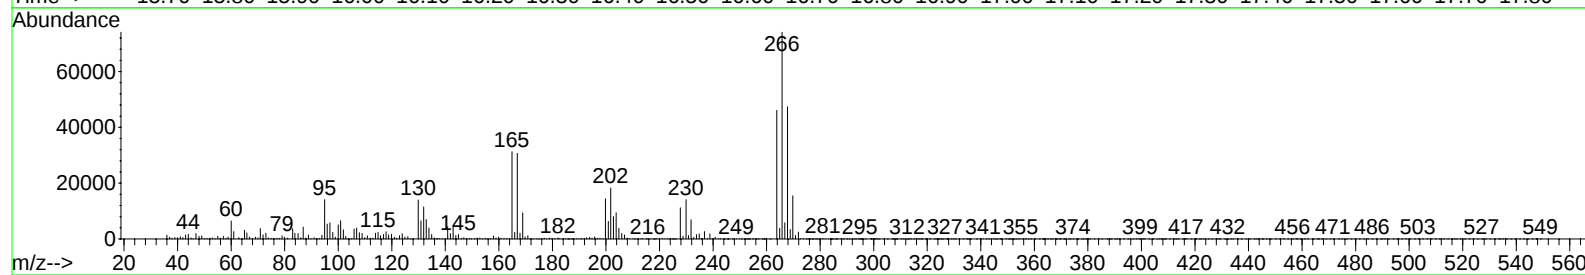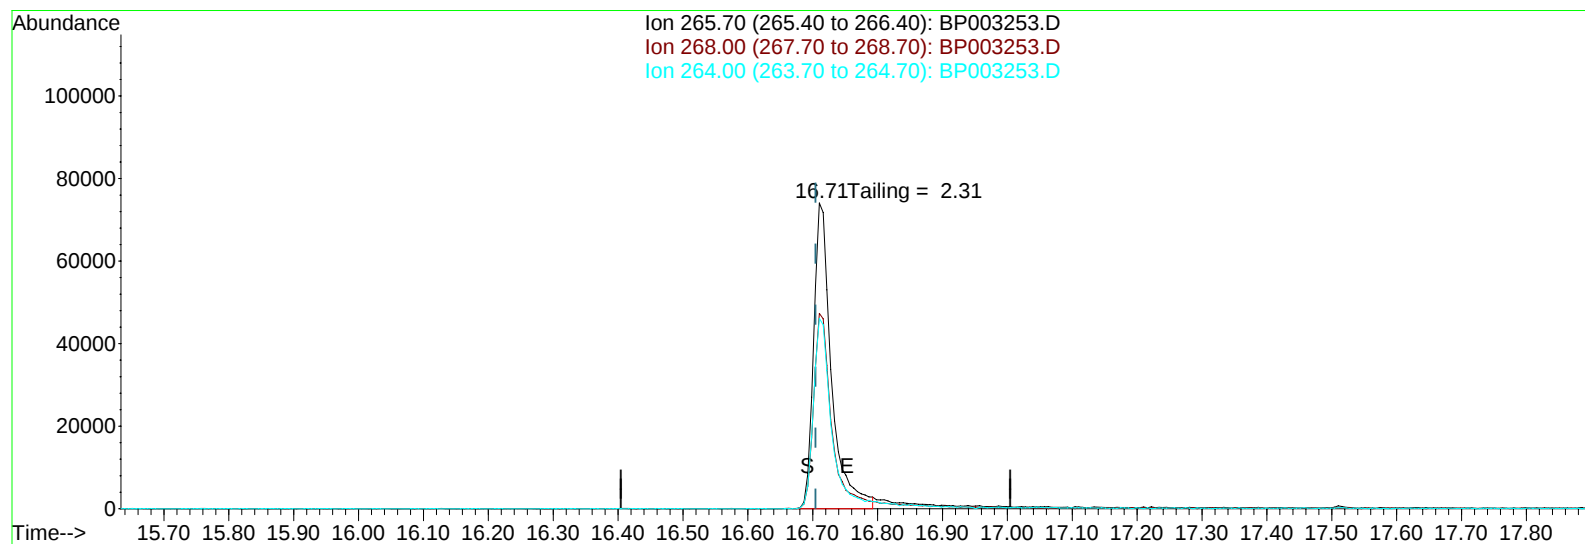

(70) Pentachlorophenol (C)

16.710min (+0.006) 39404.88ng

response 151033

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.91
264.00	63.30	62.27
0.00	0.00	0.00