

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
 Data File : BP003255.D
 Acq On : 11 Sep 2020 12:00
 Operator : CG/JU
 Sample : PB131525BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB131525BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.264	397	404	421	rBV	2482281	3832122	35.53%	8.217%
2	6.840	664	672	688	rBV	2238661	3753238	34.80%	8.048%
3	7.646	801	809	823	rBV	692307	1077885	9.99%	2.311%
4	8.793	994	1004	1021	rBV	1600148	2836546	26.30%	6.083%
5	10.428	1273	1282	1302	rBV	785477	1533995	14.22%	3.289%
6	12.910	1696	1704	1728	rBV	4654101	7566566	70.15%	16.225%
7	14.293	1932	1939	1959	rVB2	1243574	2080670	19.29%	4.462%
8	15.792	2186	2194	2217	rBV	2983606	5339215	49.50%	11.449%
9	17.045	2401	2407	2422	rBV	1544939	2490516	23.09%	5.341%
10	19.622	2840	2845	2861	rBV	7892689	10785901	100.00%	23.129%
11	20.933	3064	3068	3075	rBV	98358	149389	1.39%	0.320%
12	21.145	3098	3104	3117	rBV	1950519	2755996	25.55%	5.910%
13	23.380	3477	3484	3497	rVB2	1130213	2432334	22.55%	5.216%




Sum of corrected areas: 46634373

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
Data File : BP003255.D
Acq On : 11 Sep 2020 12:00
Operator : CG/JU
Sample : PB131525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131525BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

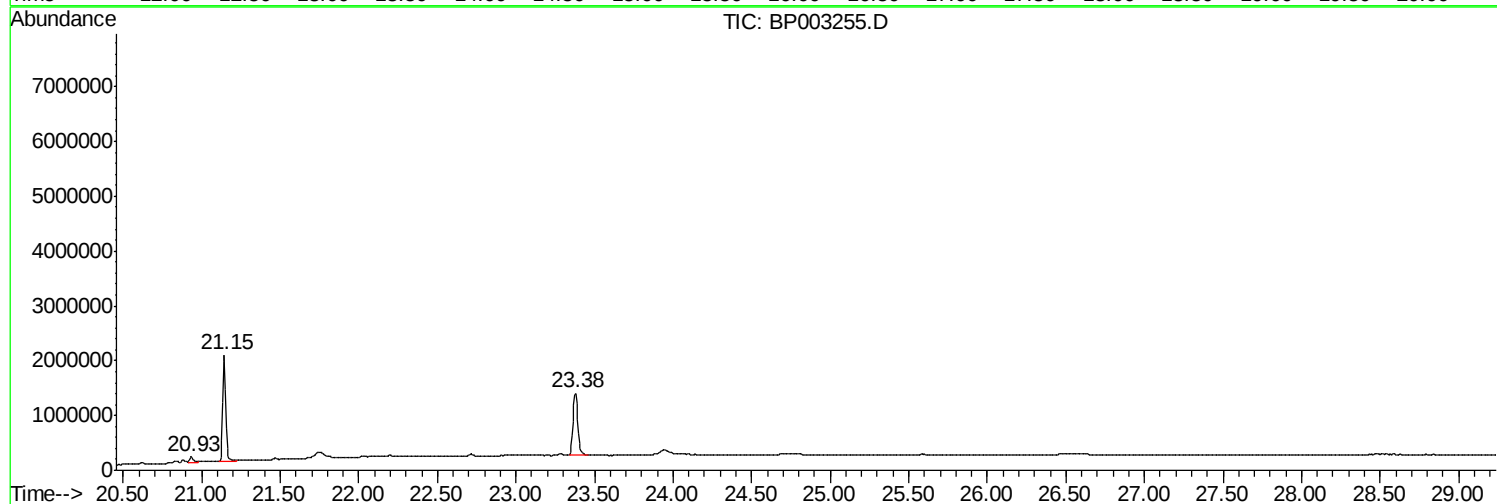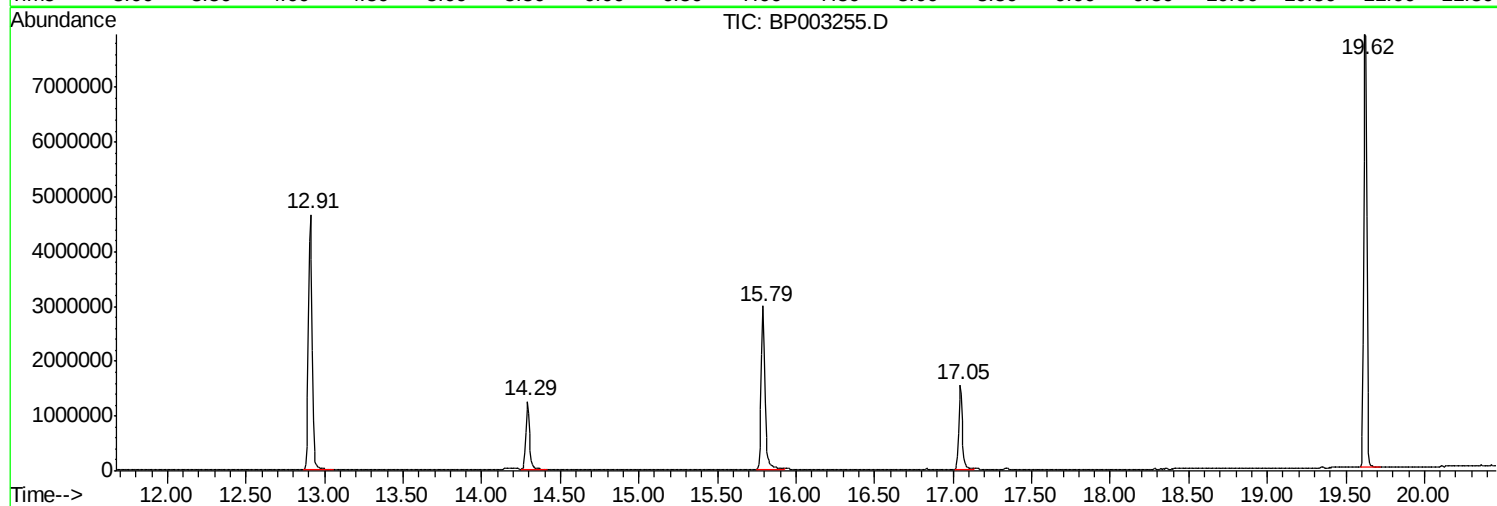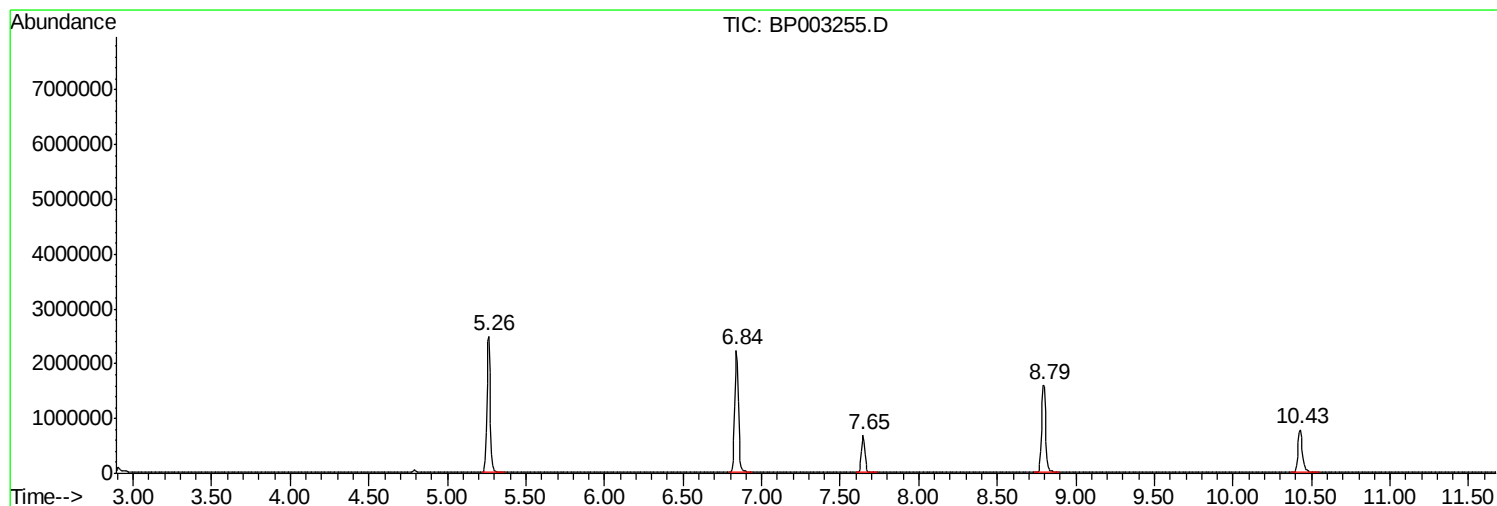

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091120\
Data File : BP003255.D
Acq On : 11 Sep 2020 12:00
Operator : CG/JU
Sample : PB131525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131525BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091120\
Data File : BP003255.D
Acq On : 11 Sep 2020 12:00
Operator : CG/JU
Sample : PB131525BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB131525BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc