

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\  
 Data File : BP003258.D  
 Acq On : 11 Sep 2020 13:43  
 Operator : CG/JU  
 Sample : PB131546BL  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB131546BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.258       | 396           | 403         | 423          | rBV      | 1615492        | 2467715       | 34.17%          | 6.689%        |
| 2         | 6.840       | 663           | 672         | 693          | rBV      | 1355585        | 2334813       | 32.33%          | 6.329%        |
| 3         | 7.646       | 801           | 809         | 827          | rBV      | 601885         | 950494        | 13.16%          | 2.577%        |
| 4         | 7.963       | 855           | 863         | 874          | rBV      | 2324887        | 3794774       | 52.54%          | 10.286%       |
| 5         | 8.793       | 996           | 1004        | 1026         | rBV      | 1393228        | 2473655       | 34.25%          | 6.705%        |
| 6         | 10.428      | 1274          | 1282        | 1300         | rBV      | 601394         | 1231434       | 17.05%          | 3.338%        |
| 7         | 12.910      | 1696          | 1704        | 1730         | rBV      | 3817142        | 6452118       | 89.33%          | 17.490%       |
| 8         | 14.292      | 1932          | 1939        | 1958         | rVB      | 864438         | 1558717       | 21.58%          | 4.225%        |
| 9         | 15.792      | 2187          | 2194        | 2224         | rBV      | 1470264        | 2916280       | 40.38%          | 7.905%        |
| 10        | 17.045      | 2400          | 2407        | 2423         | rBV      | 952780         | 1701508       | 23.56%          | 4.612%        |
| 11        | 19.622      | 2839          | 2845        | 2860         | rBV      | 5698439        | 7222773       | 100.00%         | 19.579%       |
| 12        | 20.933      | 3065          | 3068        | 3074         | rBV      | 69599          | 110426        | 1.53%           | 0.299%        |
| 13        | 21.145      | 3099          | 3104        | 3114         | rBV      | 1176826        | 1673575       | 23.17%          | 4.537%        |
| 14        | 23.380      | 3477          | 3484        | 3503         | rVB2     | 885548         | 2002602       | 27.73%          | 5.428%        |


Sum of corrected areas: 36890884

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\  
Data File : BP003258.D  
Acq On : 11 Sep 2020 13:43  
Operator : CG/JU  
Sample : PB131546BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB131546BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

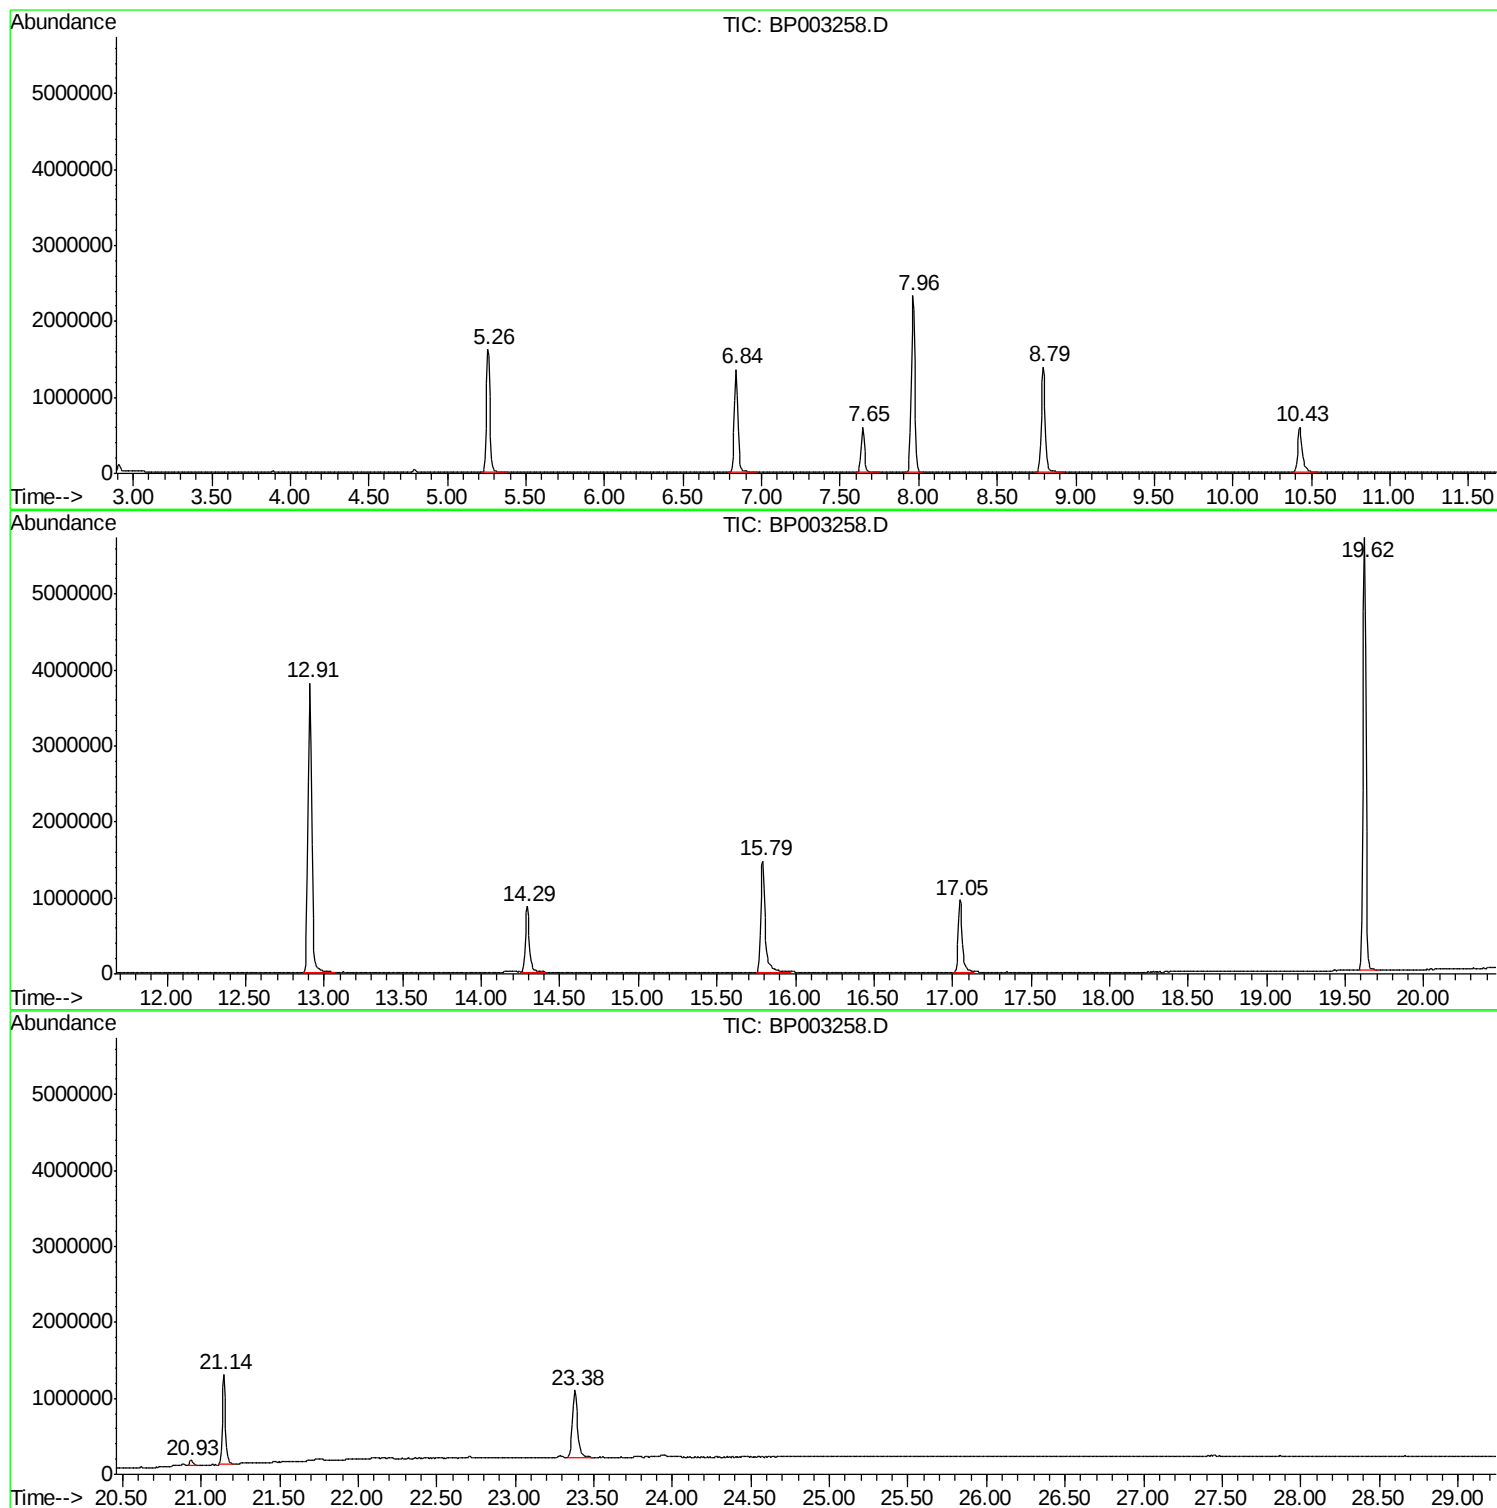

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP091120\  
Data File : BP003258.D  
Acq On : 11 Sep 2020 13:43  
Operator : CG/JU  
Sample : PB131546BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB131546BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP091120\  
Data File : BP003258.D  
Acq On : 11 Sep 2020 13:43  
Operator : CG/JU  
Sample : PB131546BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB131546BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP082420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |