

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
Data File : BP003263.D
Acq On : 11 Sep 2020 16:43
Operator : CG/JU
Sample : L3943-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
357

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	396	404	422	rBV	1717430	2604805	33.56%	6.933%
2	6.846	665	673	697	rBV	1490667	2631384	33.90%	7.004%
3	7.646	800	809	819	rBV	660206	1027049	13.23%	2.734%
4	8.793	994	1004	1026	rBV	1063484	1916591	24.69%	5.102%
5	10.428	1272	1282	1300	rBV	759095	1452664	18.71%	3.867%
6	12.910	1696	1704	1725	rBV	3248609	5243266	67.54%	13.956%
7	13.751	1841	1847	1867	rBV	370099	672823	8.67%	1.791%
8	14.292	1932	1939	1972	rVB	1257797	2066549	26.62%	5.501%
9	15.792	2187	2194	2217	rBV	2249016	3928840	50.61%	10.458%
10	17.045	2401	2407	2421	rBV	1553445	2420431	31.18%	6.443%
11	19.622	2839	2845	2856	rBV	6076479	7762743	100.00%	20.663%
12	20.869	3053	3057	3065	rBV	399955	559549	7.21%	1.489%
13	21.139	3098	3103	3114	rBV	2006678	2714786	34.97%	7.226%
14	22.321	3301	3304	3312	rVB	170717	223125	2.87%	0.594%
15	23.374	3477	3483	3500	rVB2	1199961	2344500	30.20%	6.241%


Sum of corrected areas: 37569105

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
Data File : BP003263.D
Acq On : 11 Sep 2020 16:43
Operator : CG/JU
Sample : L3943-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
357

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

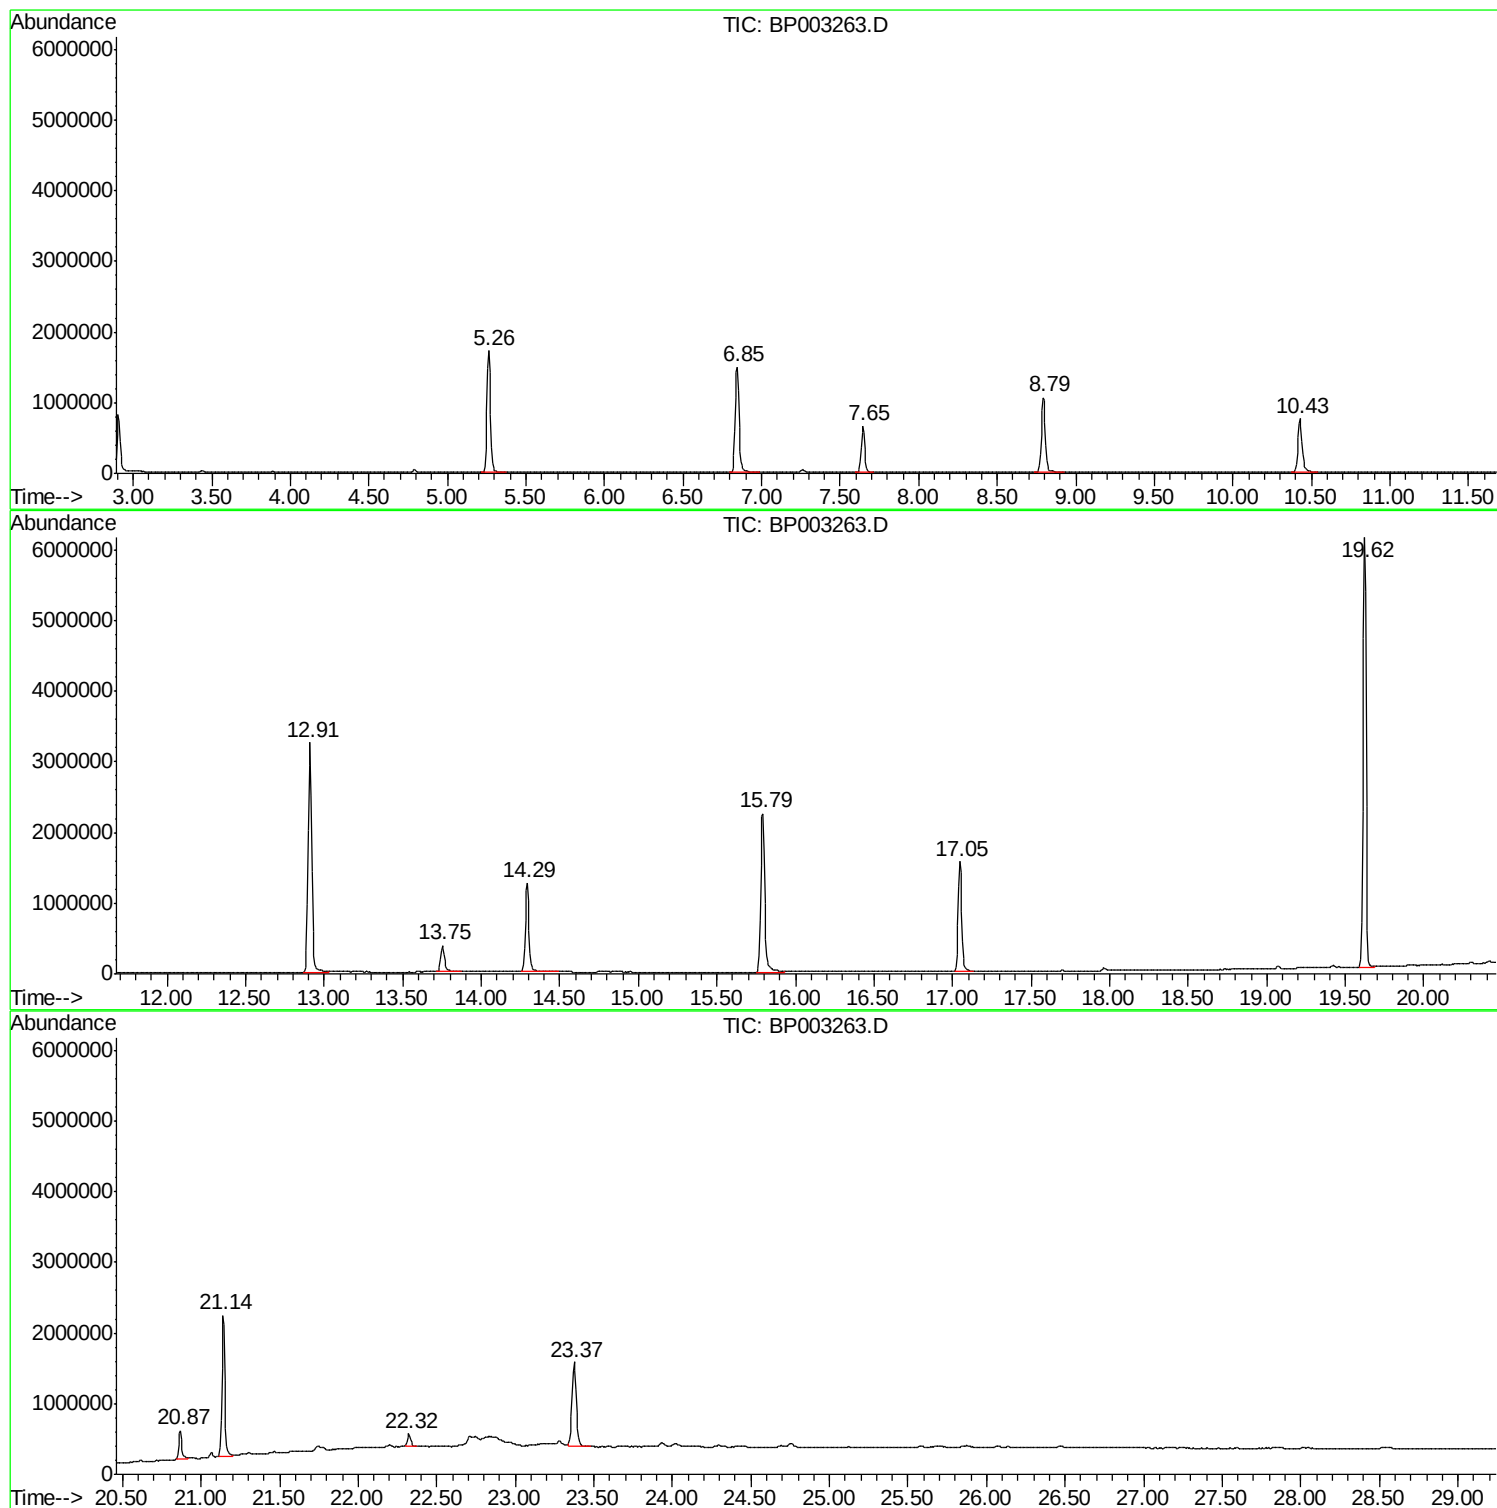

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
Data File : BP003263.D
Acq On : 11 Sep 2020 16:43
Operator : CG/JU
Sample : L3943-02
Misc :
ALS Vial : 11 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
357

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Behenic alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.
20.87	4.12 ng	559549	Chrysene-d12		21.14
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Behenic alcohol	326	C22H46O	000661-19-8	95
2	n-Tetracosanol-1	354	C24H50O	000506-51-4	95
3	1-Heptacosanol	396	C27H56O	002004-39-9	95
4	n-Nonadecanol-1	284	C19H40O	001454-84-8	94
5	Nonadecyl trifluoroacetate	380	C21H39F3O2	1000351-76-3	93

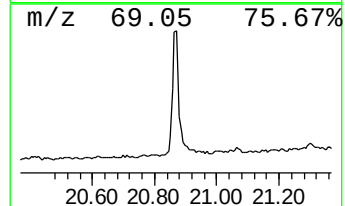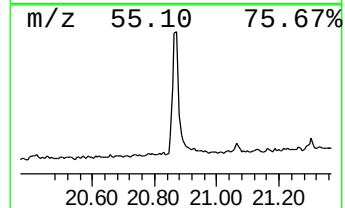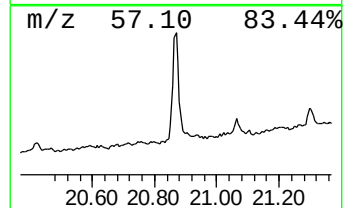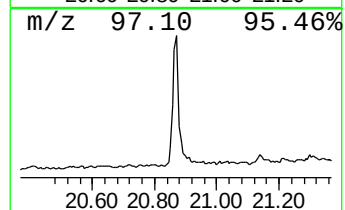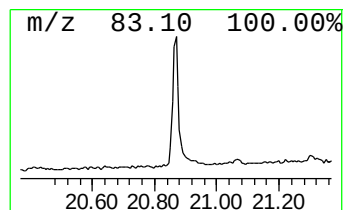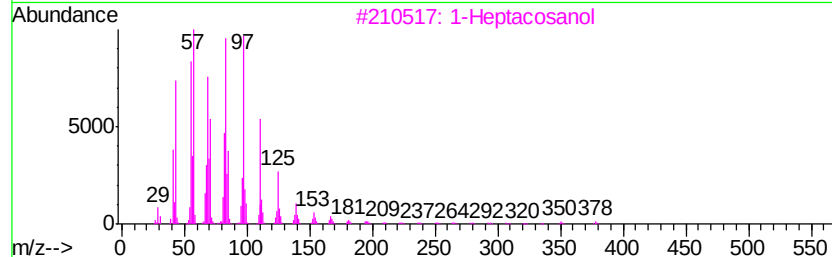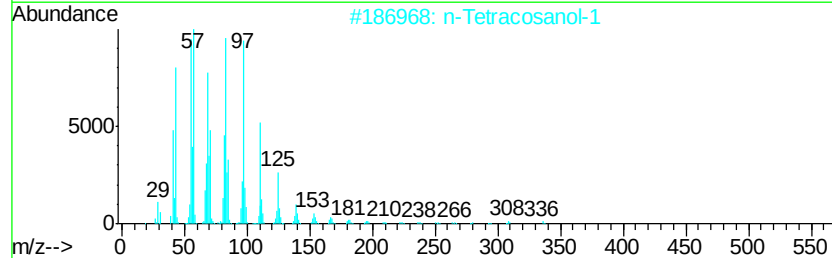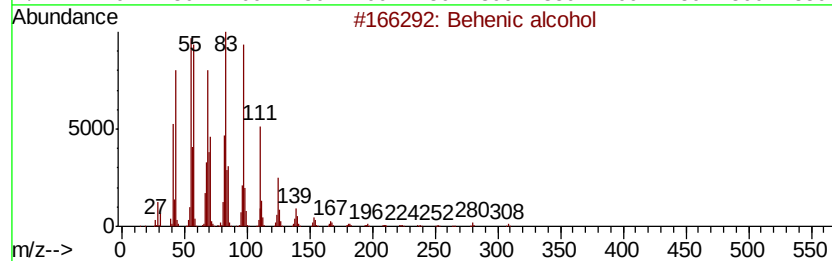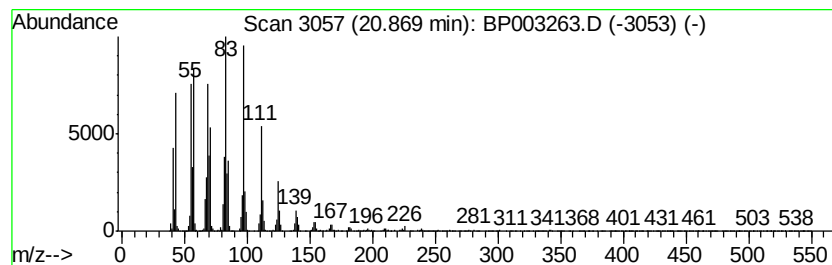

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP091120\
Data File : BP003263.D
Acq On : 11 Sep 2020 16:43
Operator : CG/JU
Sample : L3943-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
357

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Behenic alcohol	20.87	4.1 ng		559549	5	21.14	2714790	20.0