


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP091120\
 Data File : BP003253.D
 Acq On : 11 Sep 2020 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 01 14:37:05 2020

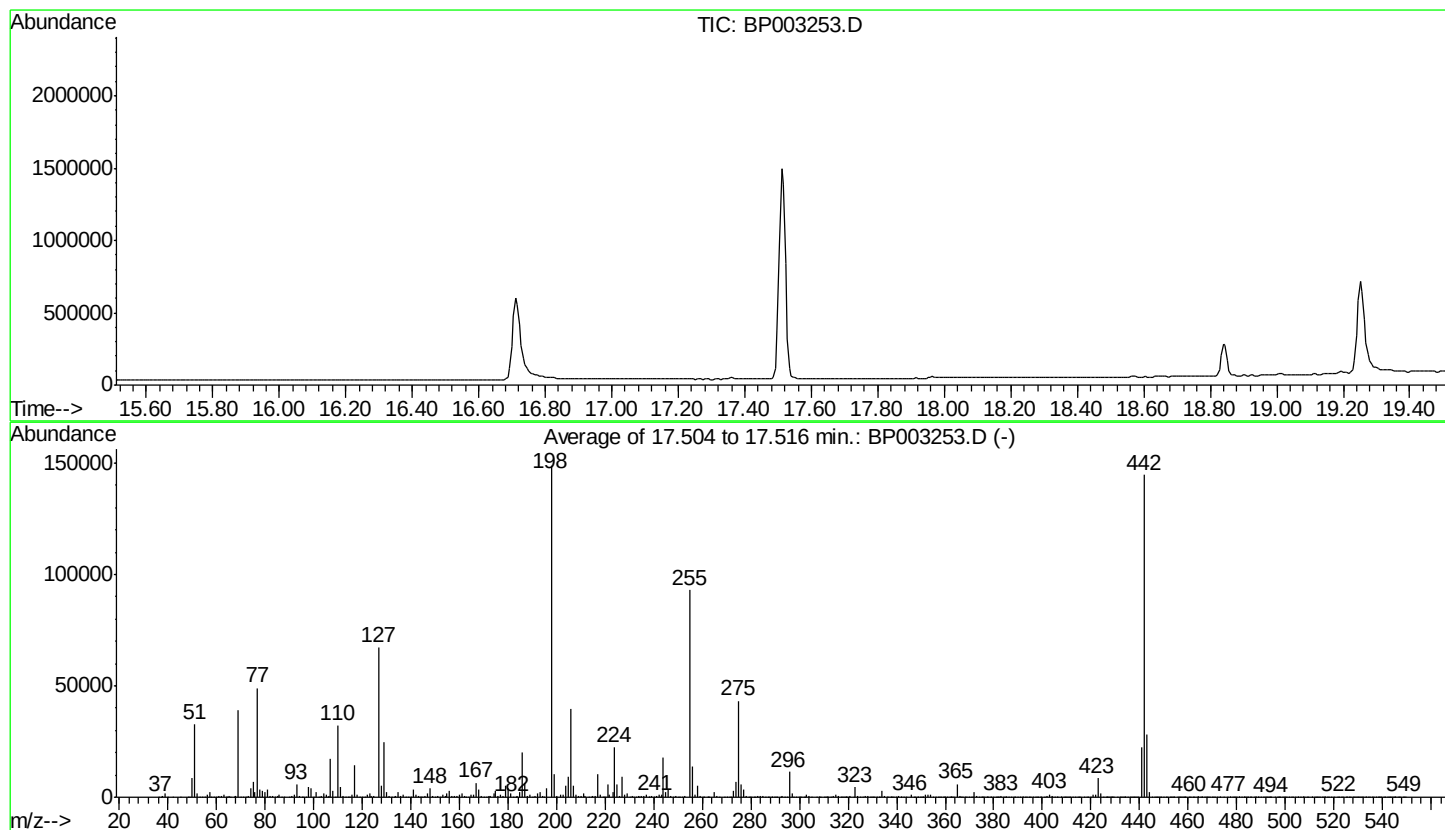

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.9	32602	PASS
68	69	0.00	2	0.9	364	PASS
69	198	0.00	100	26.1	38868	PASS
70	69	0.00	2	0.2	74	PASS
127	198	10	80	45.2	67244	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148920	PASS
199	198	5	9	7.1	10500	PASS
275	198	10	60	29.2	43416	PASS
365	198	1	100	3.9	5806	PASS
441	198	0.01	100	15.2	22584	PASS
442	198	50	100	97.2	144824	PASS
443	442	15	24	19.4	28157	PASS