



2-Nitrophenol

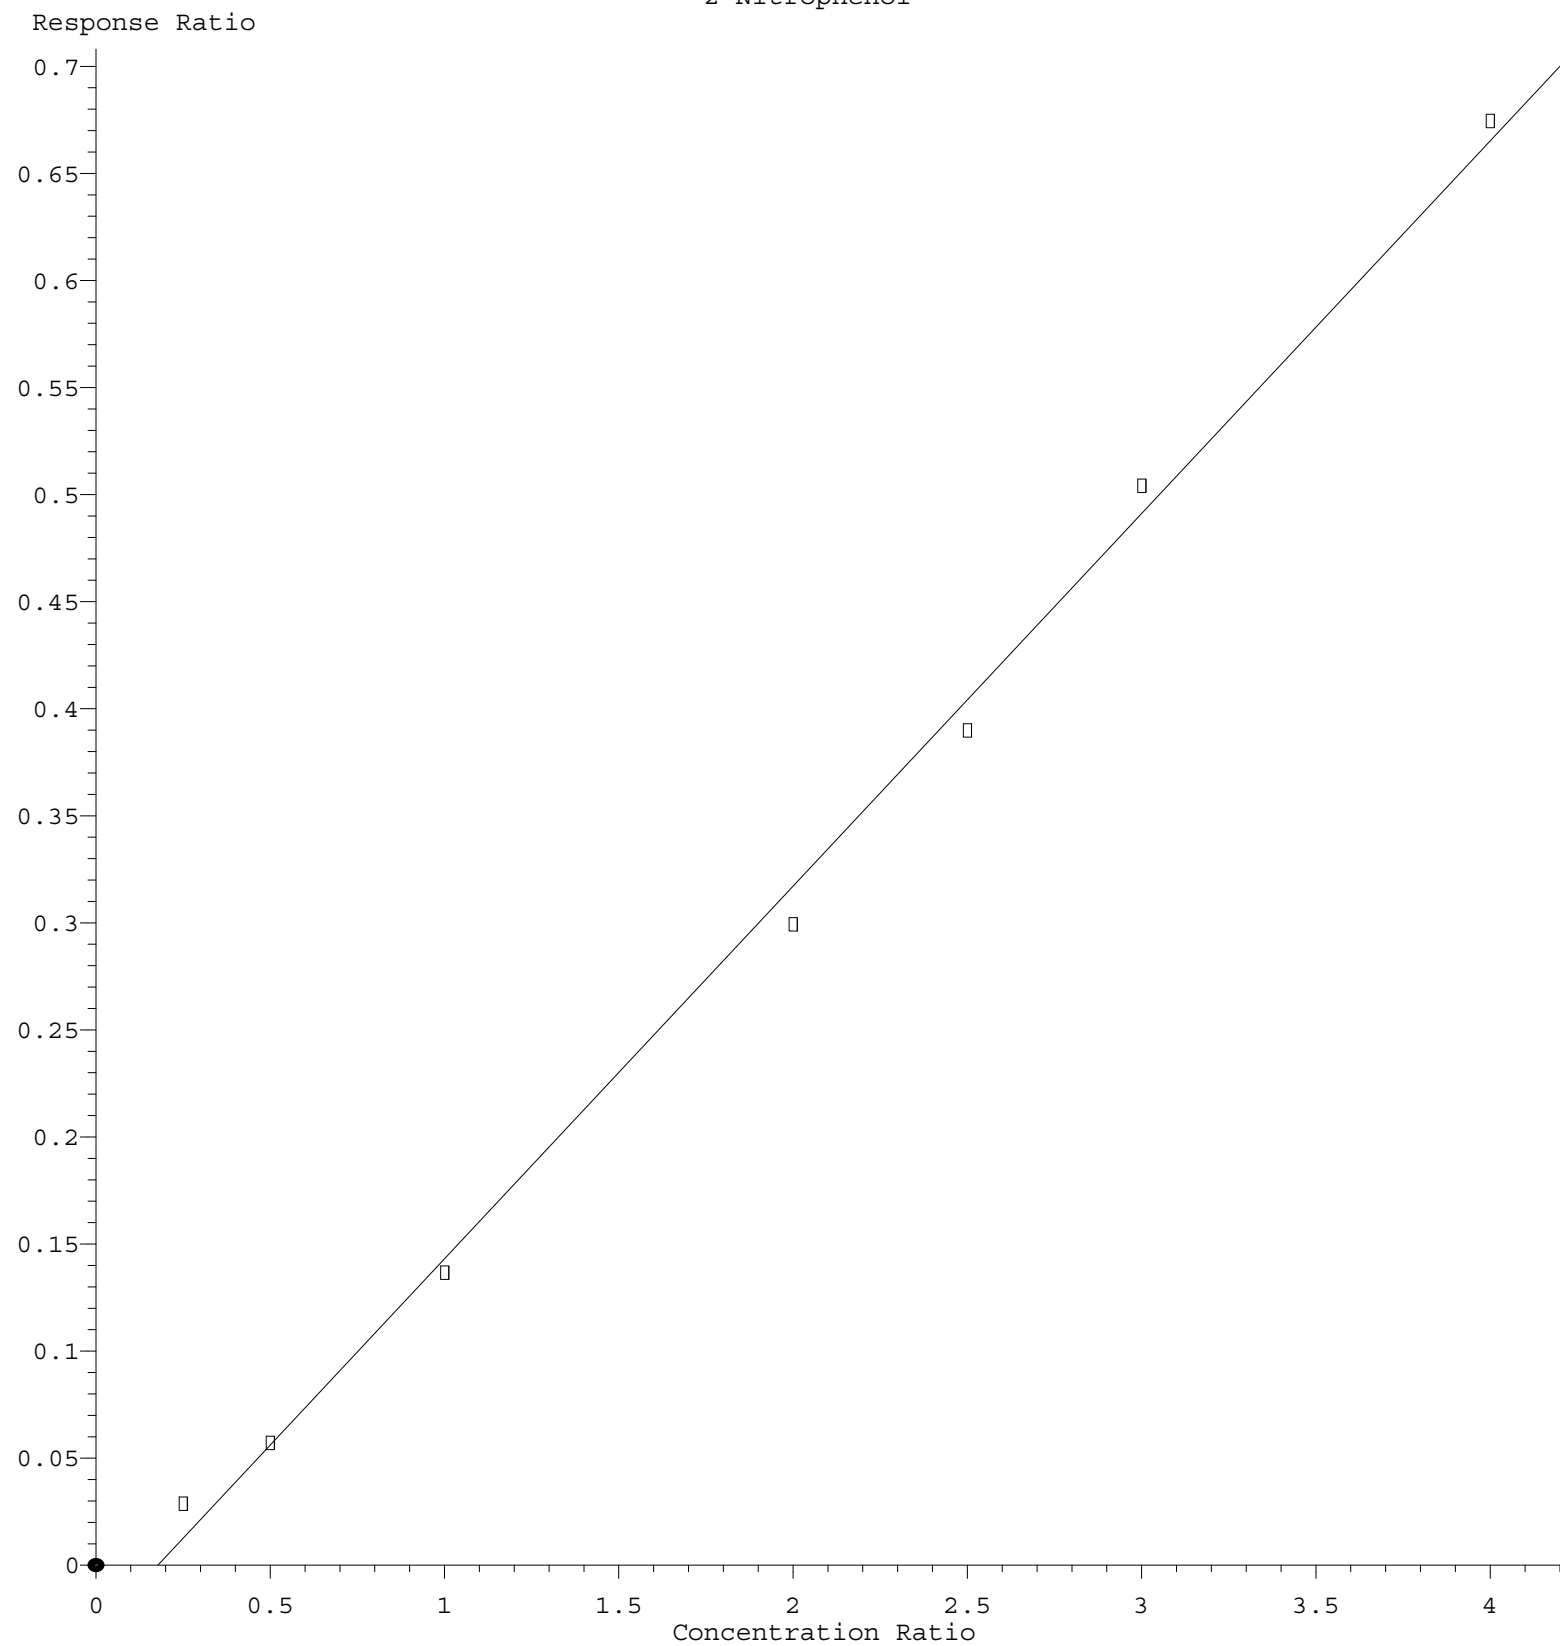

Response = $1.741e-001 * \text{Amt} - 3.105e-002$
 Coef of Det (r^2) = 0.996908 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091422.M
 Calibration Table Last Updated: Wed Sep 14 19:12:50 2022

Benzoic acid

Response Ratio

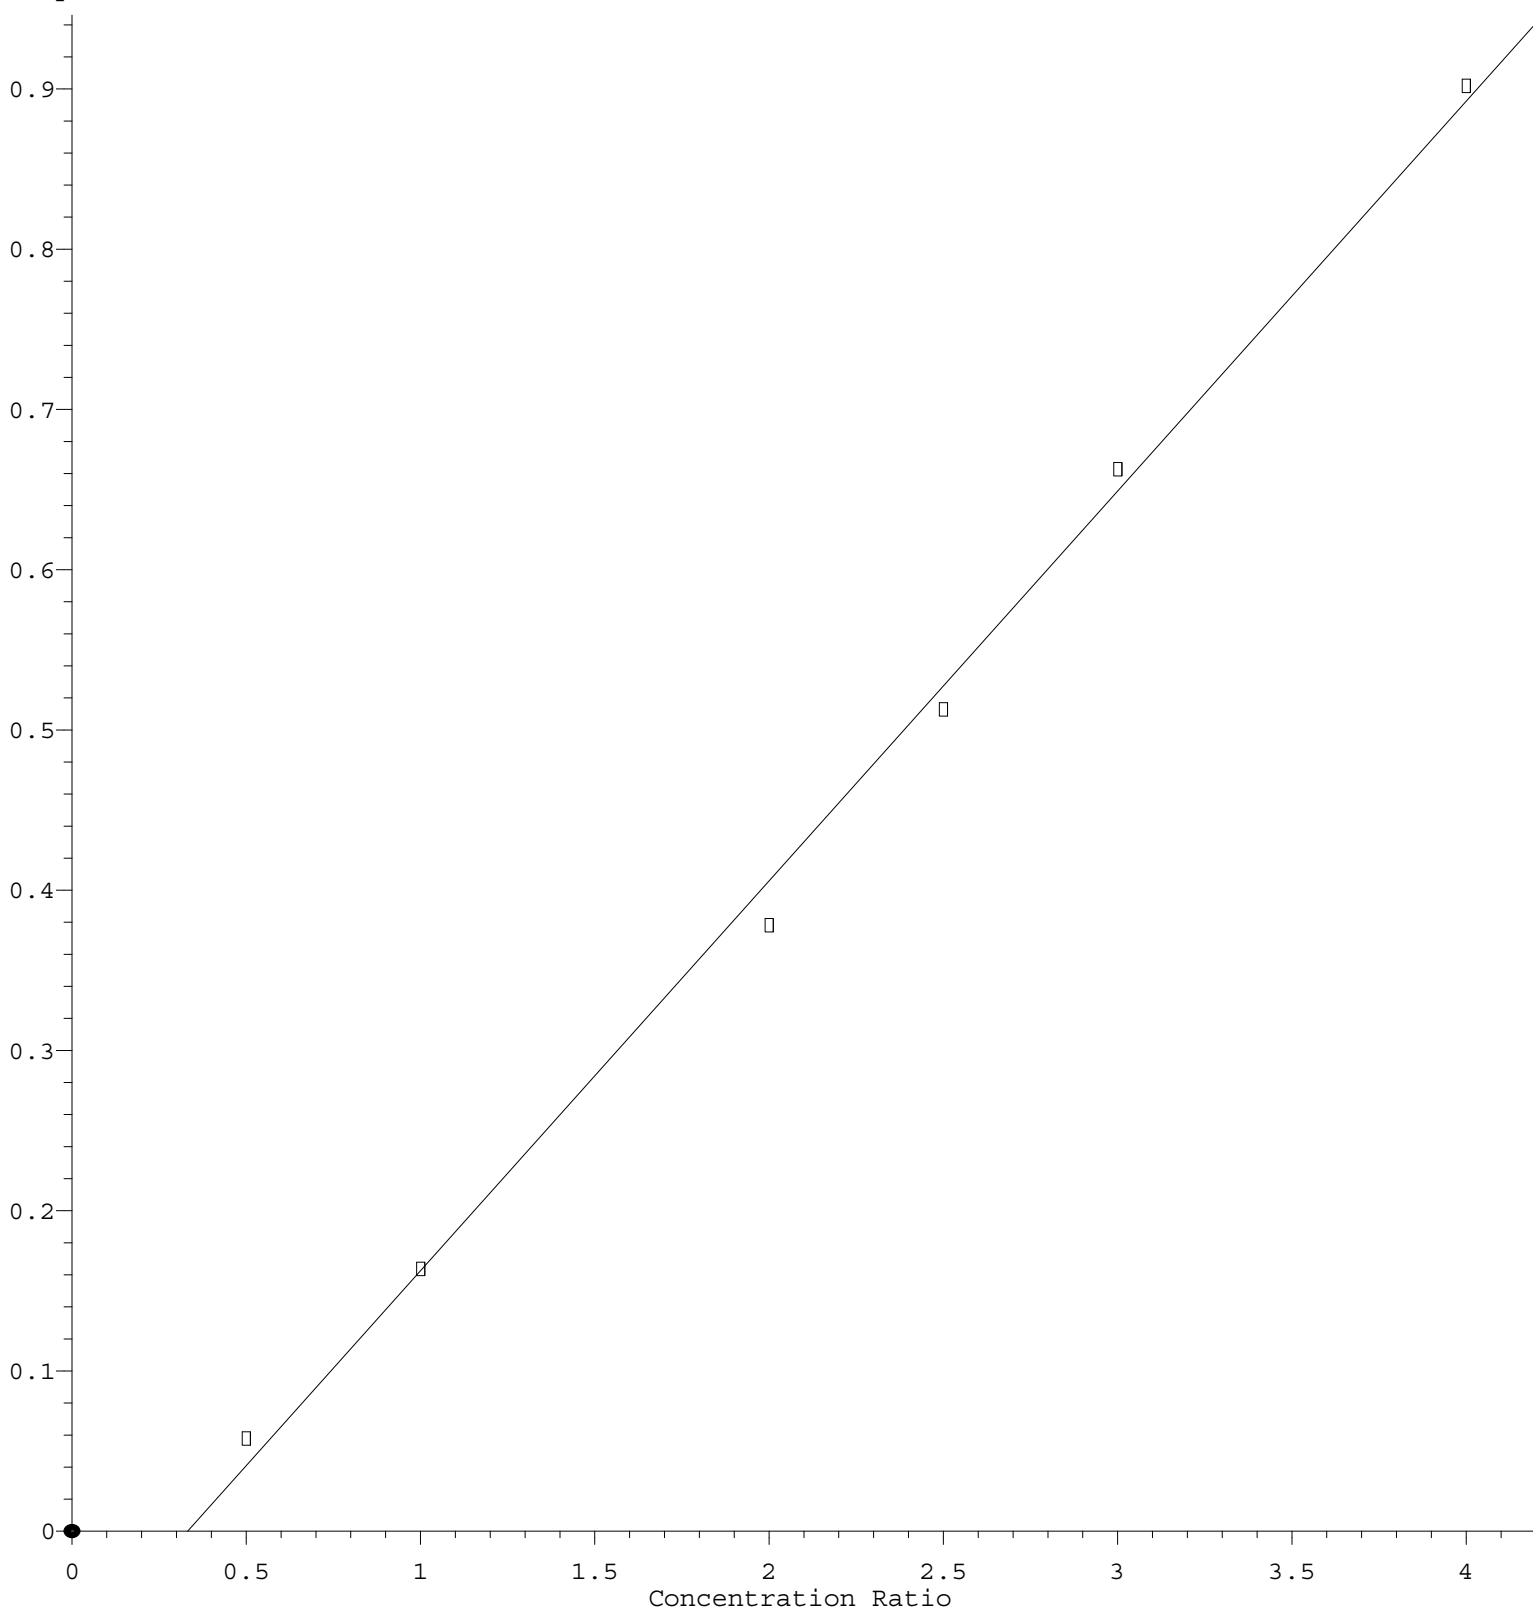

$$\text{Response} = 2.431\text{e-}001 * \text{Amt} - 8.067\text{e-}002$$


Coef of Det (r^2) = 0.996878 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091422.M

Calibration Table Last Updated: Wed Sep 14 19:12:50 2022

3-Nitroaniline

Response Ratio

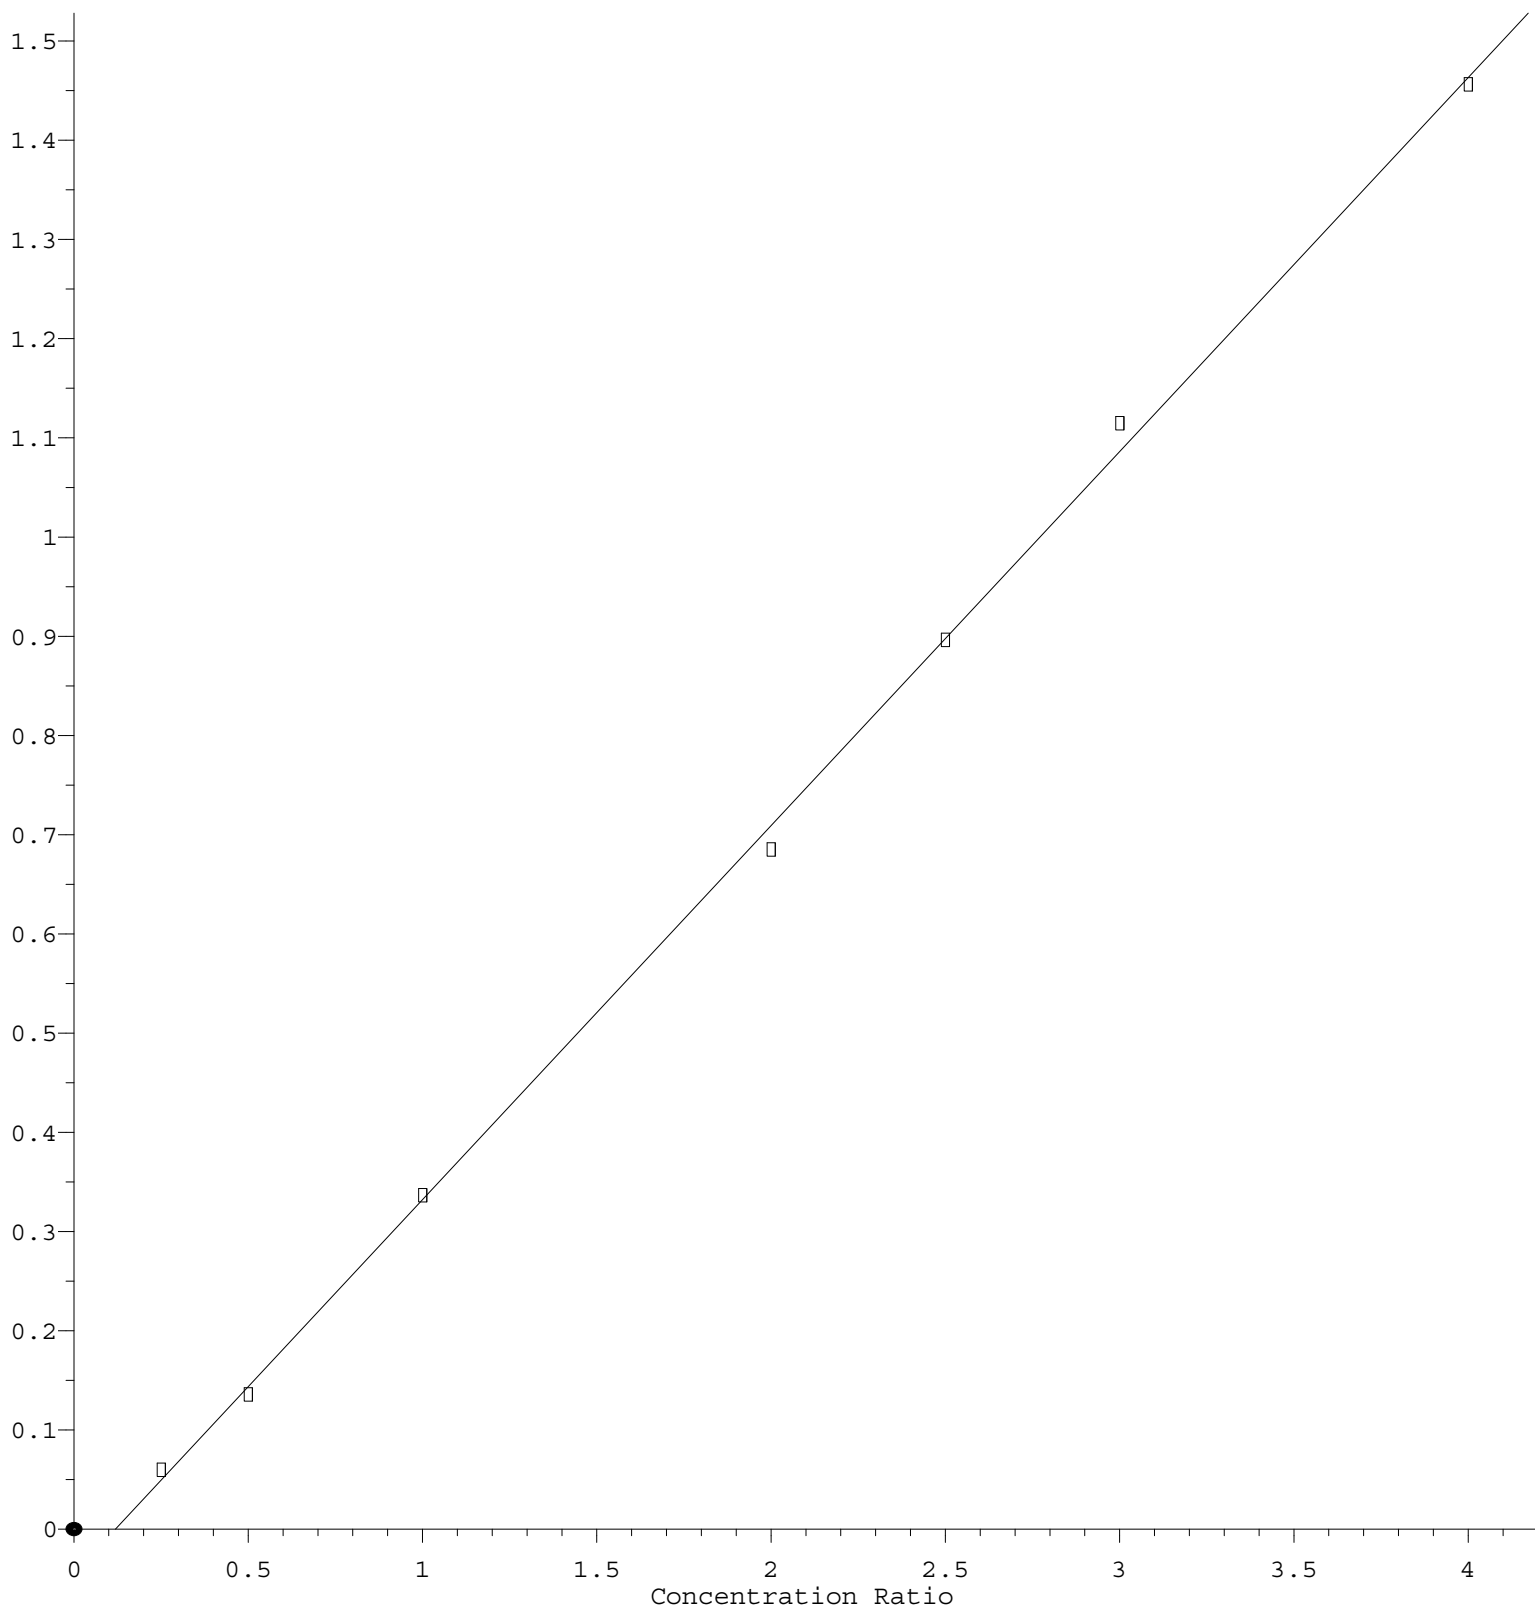


$$\text{Response} = 3.773\text{e-}001 * \text{Amt} - 4.500\text{e-}002$$

Coef of Det (r^2) = 0.999003 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091422.M

Calibration Table Last Updated: Wed Sep 14 19:12:50 2022


2,4-Dinitrophenol

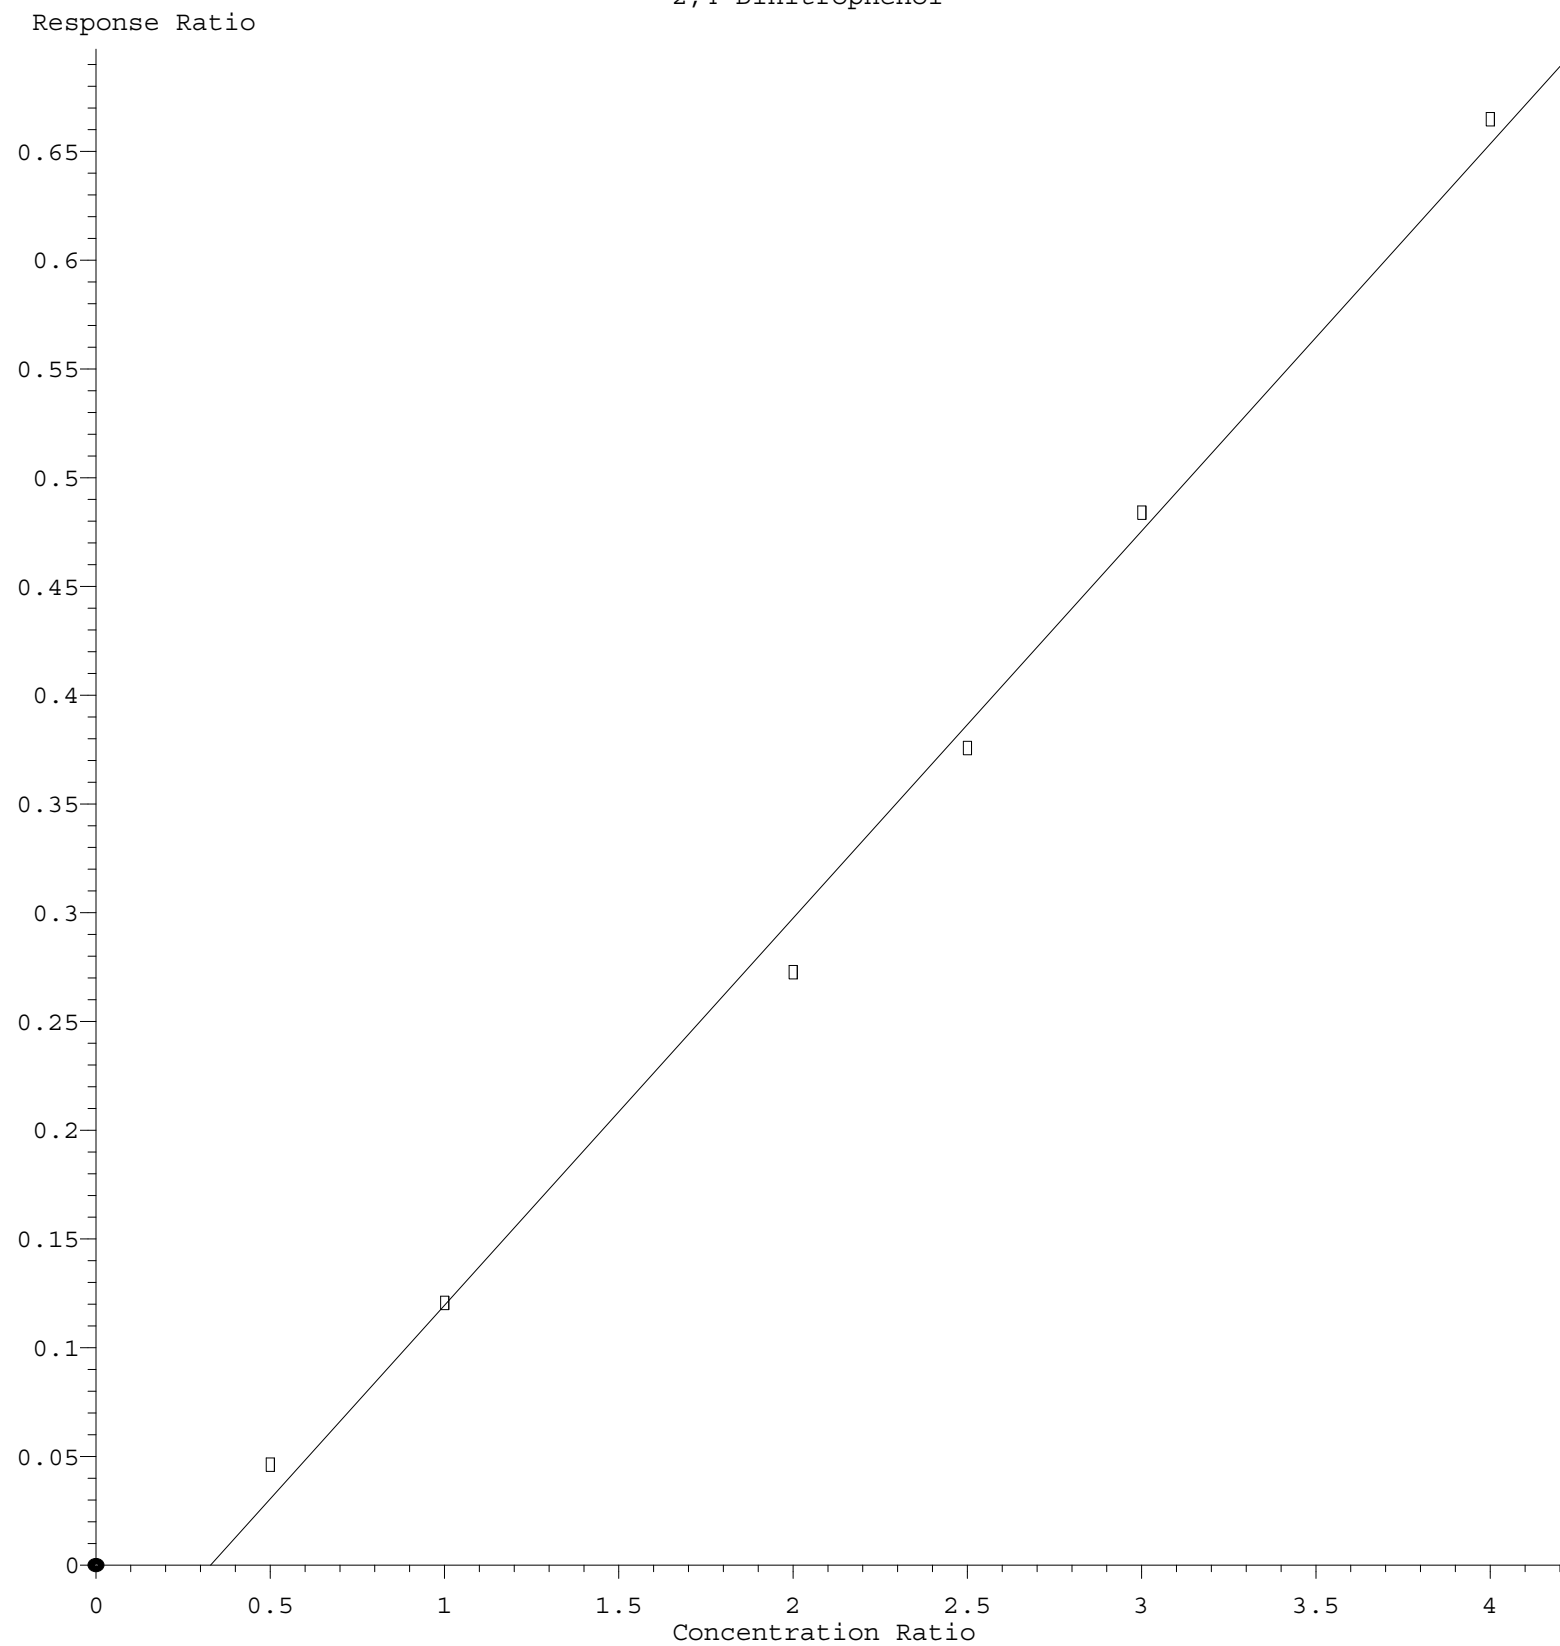

Response = $1.781e-001 * \text{Amt} - 5.860e-002$
 Coef of Det (r^2) = 0.995557 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091422.M
 Calibration Table Last Updated: Wed Sep 14 19:12:50 2022

2,4-Dinitrotoluene

Response Ratio

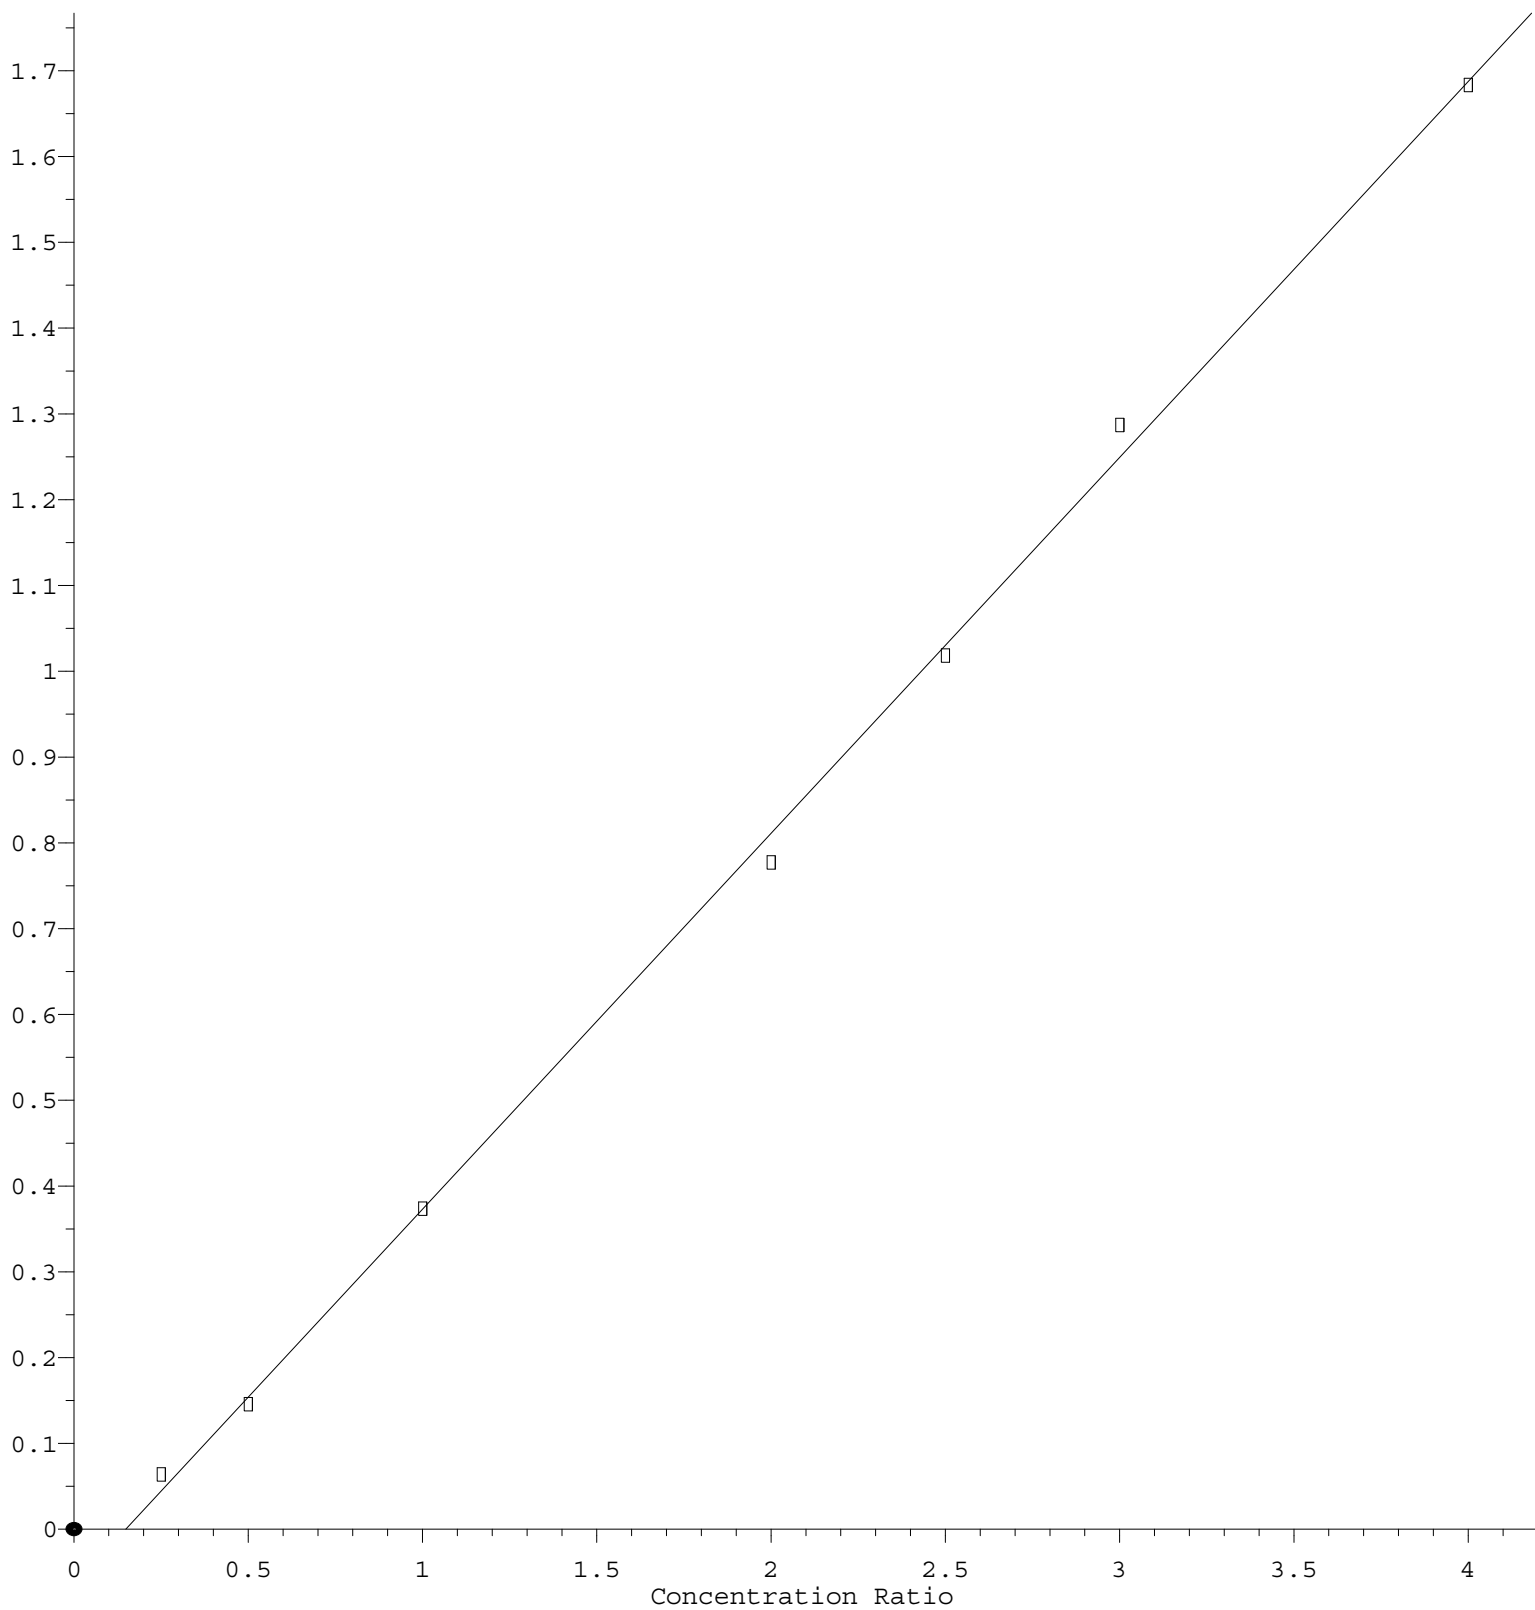


$$\text{Response} = 4.383\text{e-}001 * \text{Amt} - 6.548\text{e-}002$$

Coef of Det (r^2) = 0.998561 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091422.M

Calibration Table Last Updated: Wed Sep 14 19:12:50 2022


4,6-Dinitro-2-methylphenol

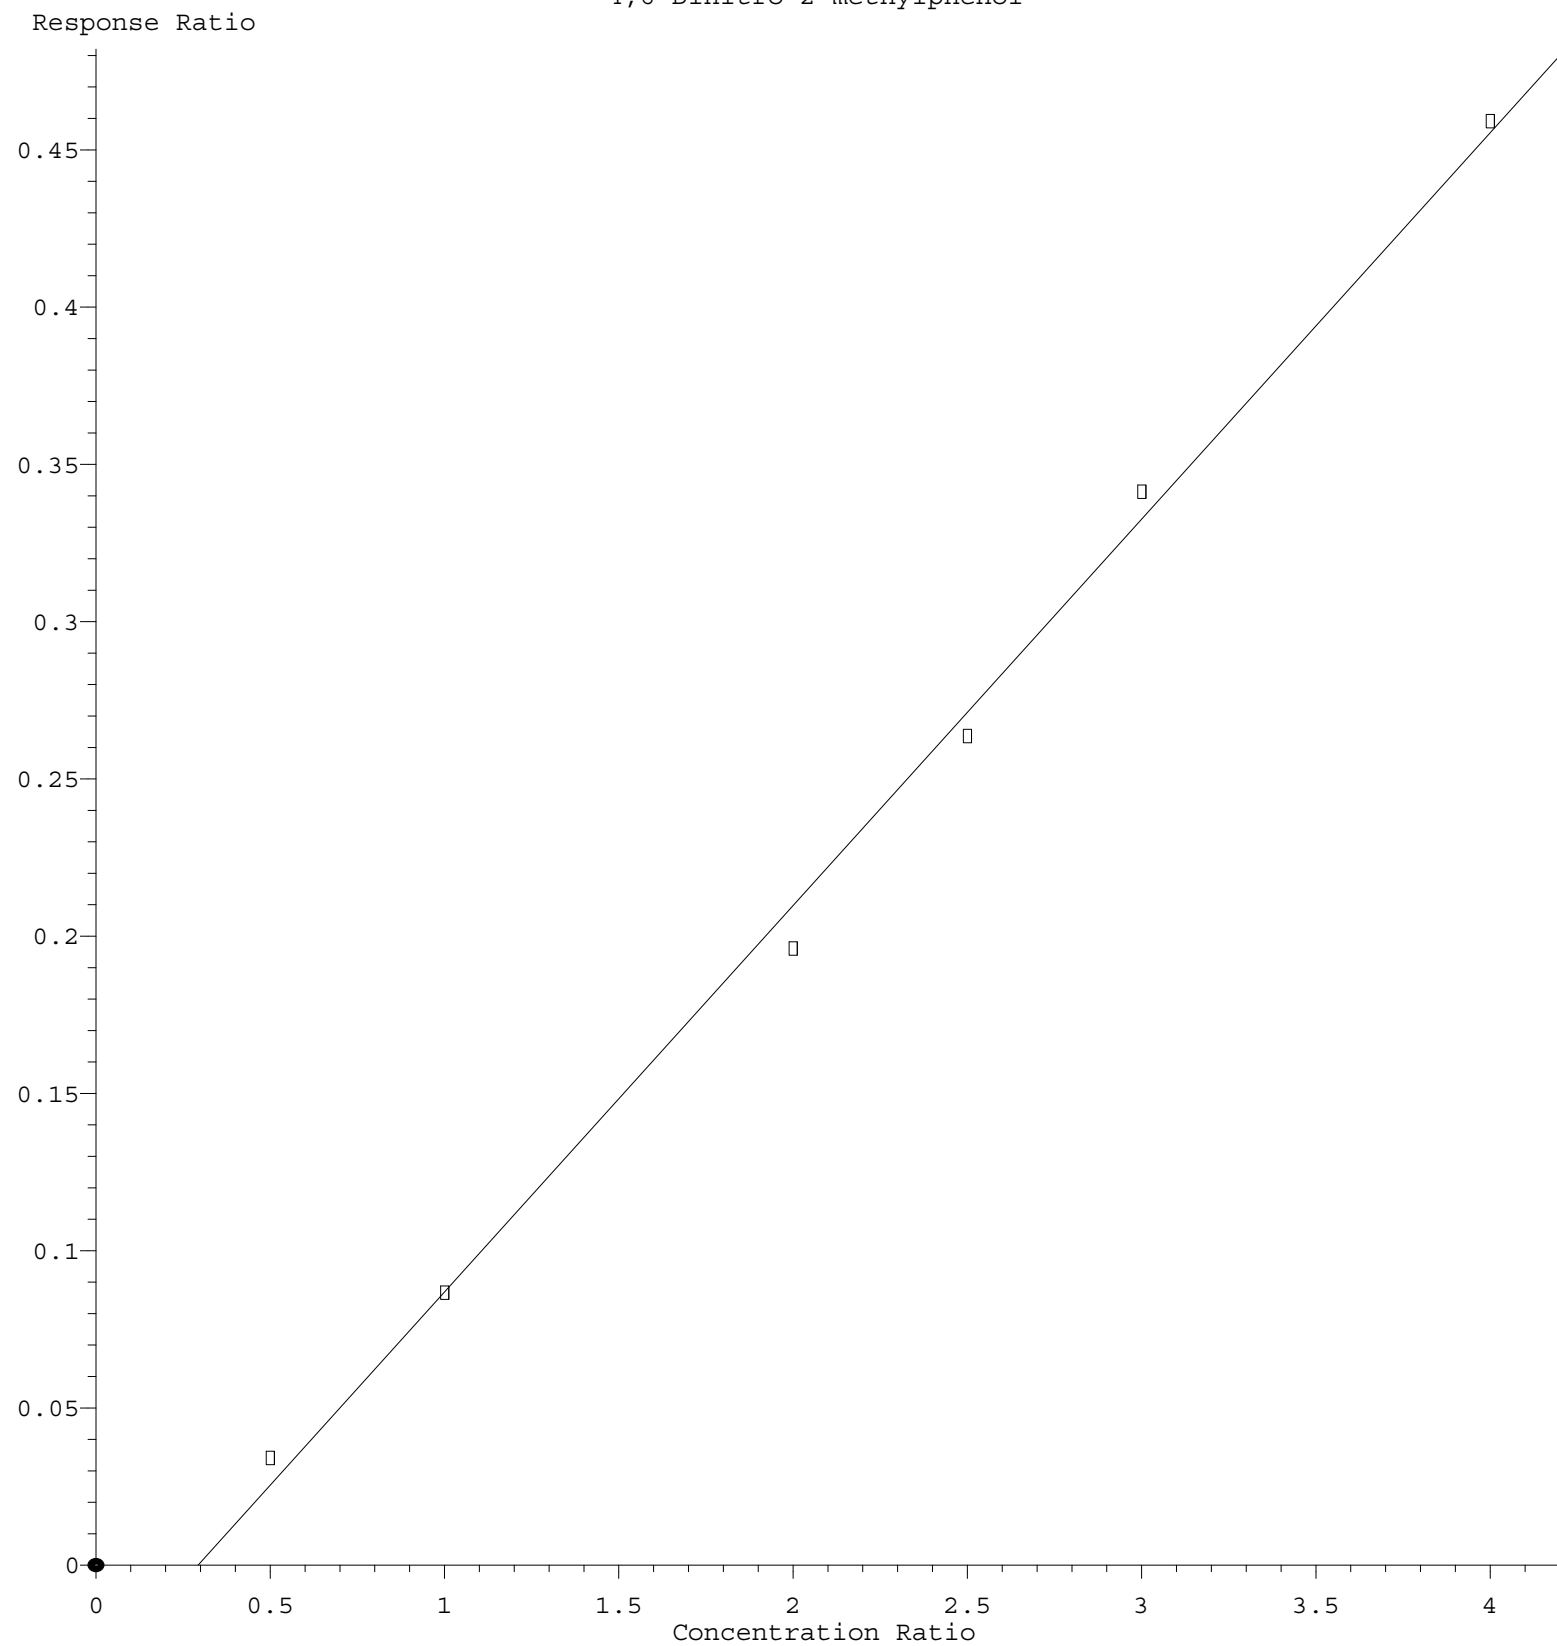

Response = $1.228 \times 10^{-1} \times \text{Amt} - 3.594 \times 10^{-2}$
Coef of Det (r^2) = 0.996761 Curve Fit: Linear
Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091422.M
Calibration Table Last Updated: Wed Sep 14 19:12:50 2022

4-Nitroaniline

Response Ratio

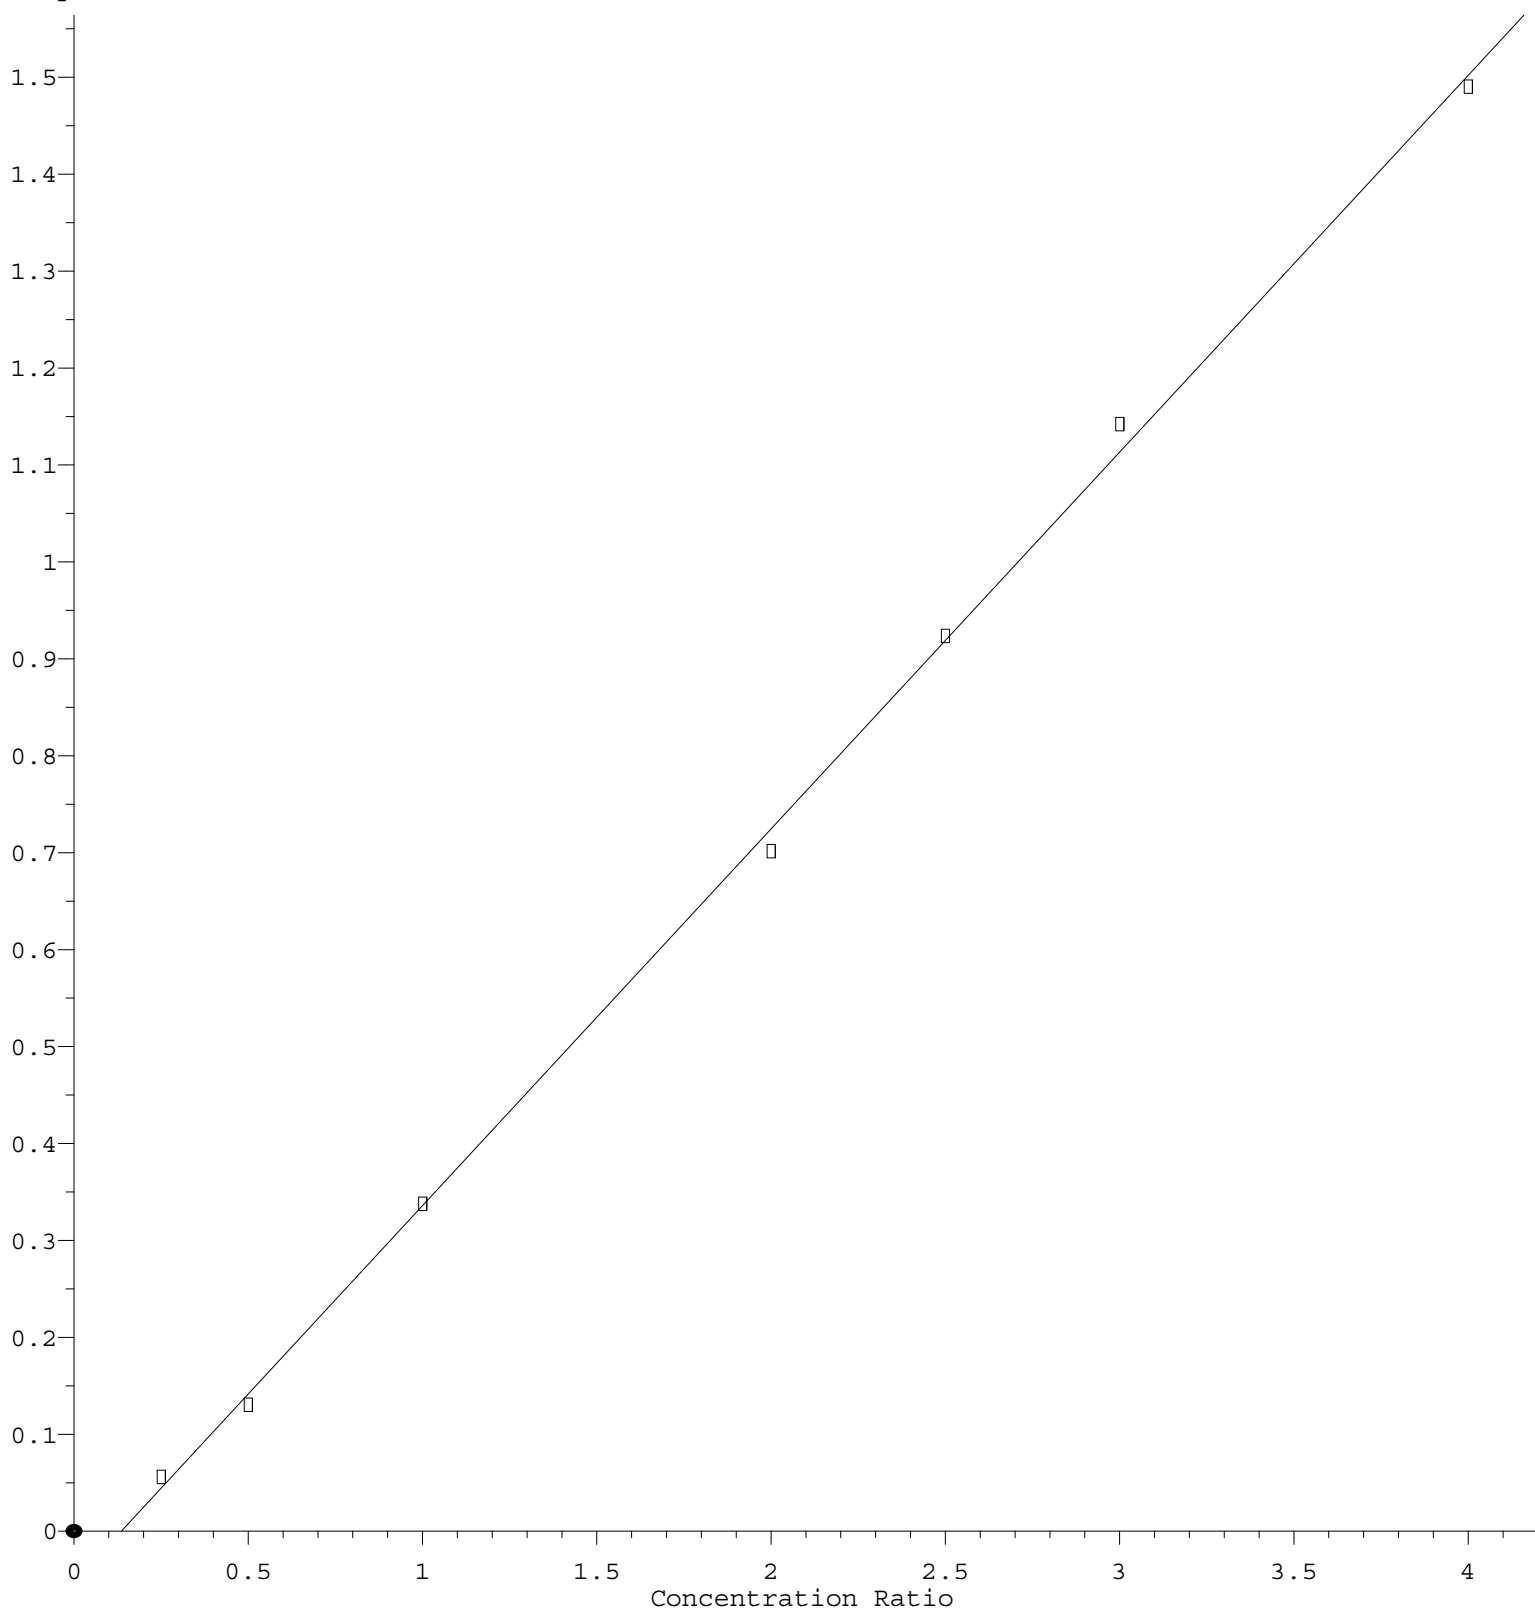

$$\text{Response} = 3.889\text{e-}001 * \text{Amt} - 5.305\text{e-}002$$

Coef of Det (r^2) = 0.998976 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP091422.M

Calibration Table Last Updated: Wed Sep 14 19:12:50 2022