
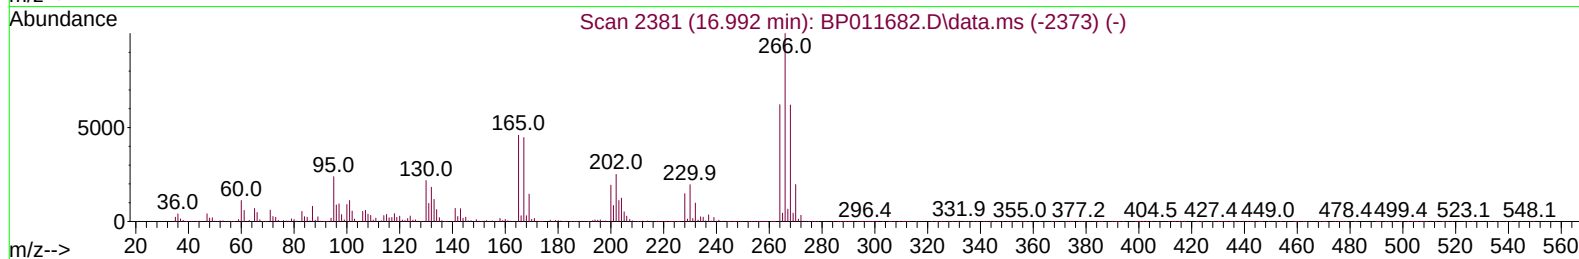
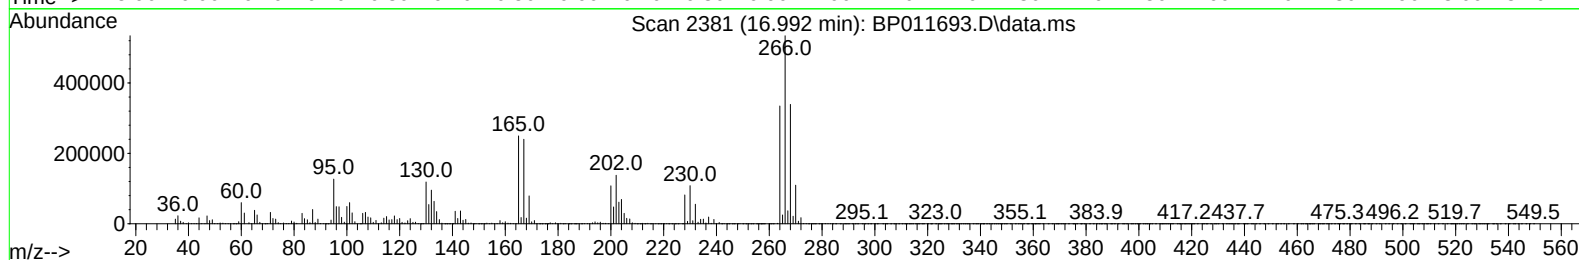


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091422\
Data File : BP011693.D
Acq On : 14 Sep 2022 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 16:24:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 16:19:53 2022
Response via : Initial Calibration

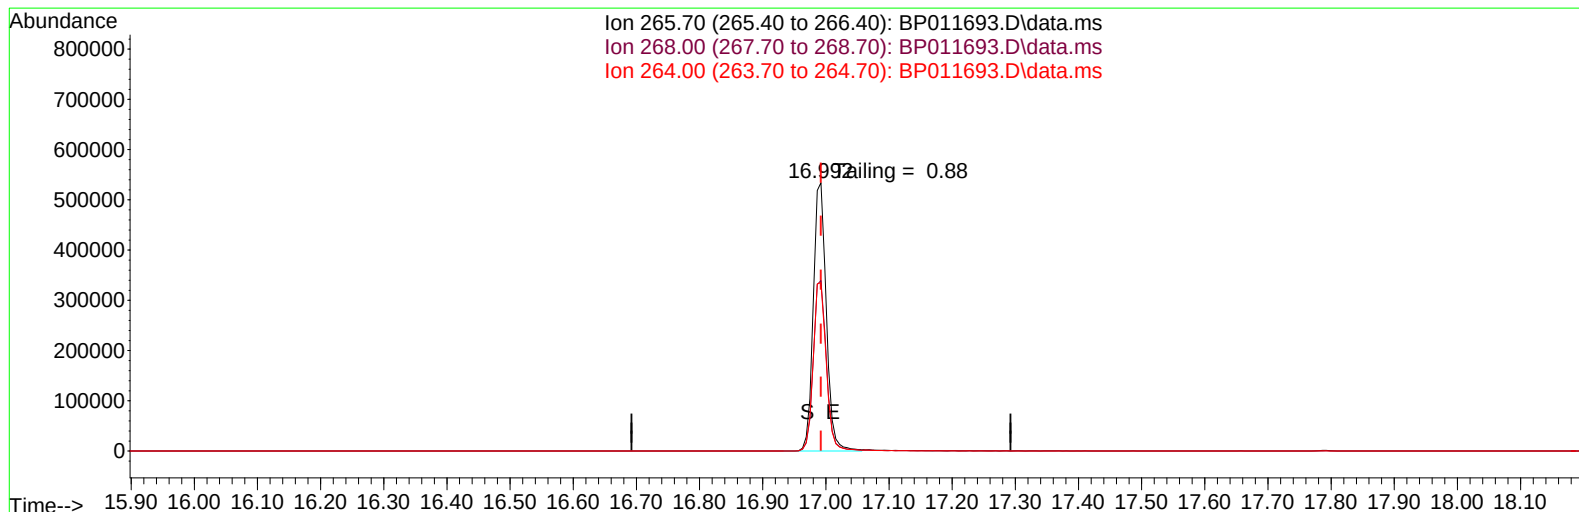

TIC: BP011693.D\data.ms

(70) Pentachlorophenol (C)




16.992min (-0.000) 373392.89 ng

response 774698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.50
264.00	63.00	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091422\
 Data File : BP011693.D
 Acq On : 14 Sep 2022 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 16:24:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 16:19:53 2022
 Response via : Initial Calibration

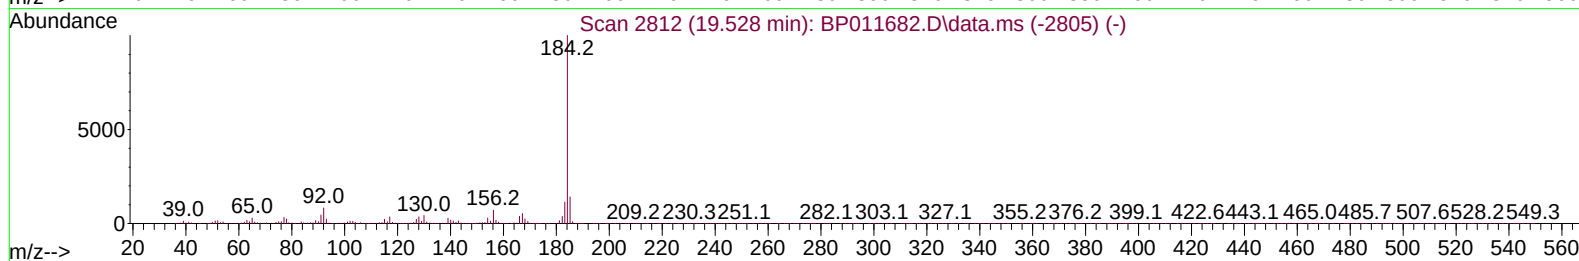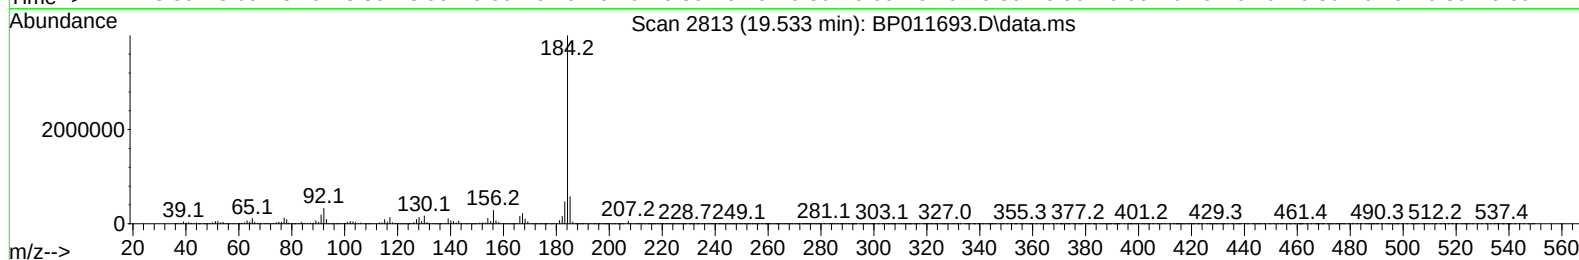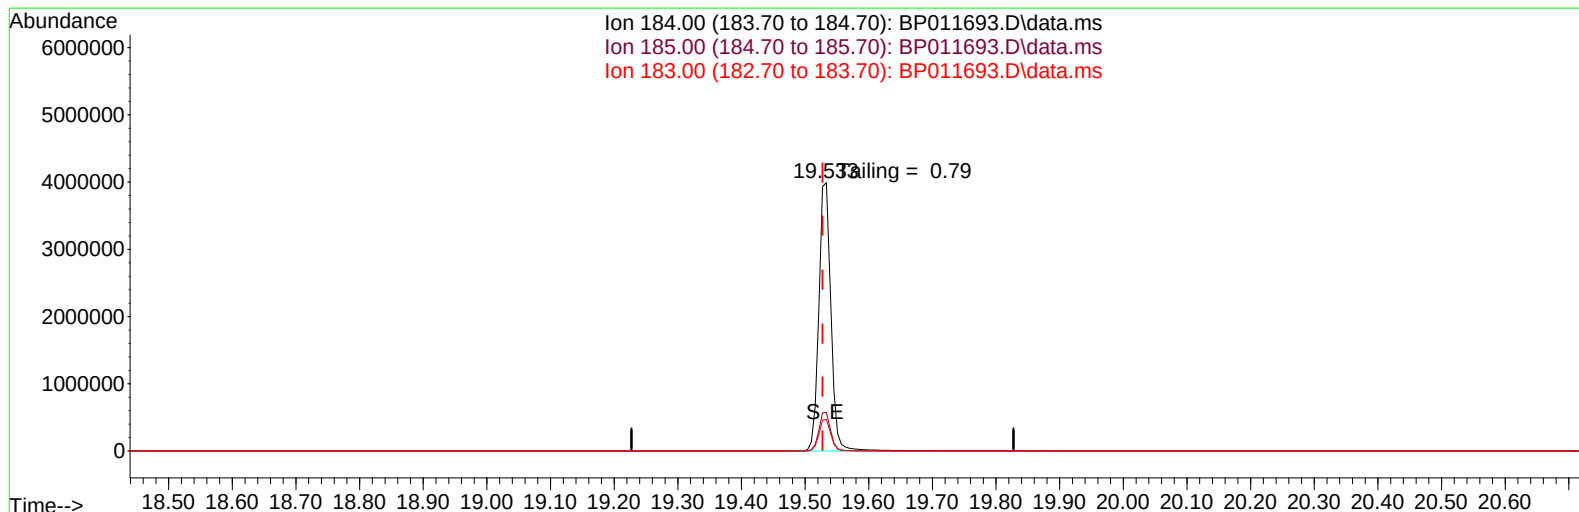

TIC: BP011693.D\data.ms

(77) Benzidine**19.533min (+ 0.006) 5101042.46 ng****response 5265308**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.39
183.00	11.30	11.79
0.00	0.00	0.00