


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091422\
 Data File : BP011693.D
 Acq On : 14 Sep 2022 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 19:12:50 2022

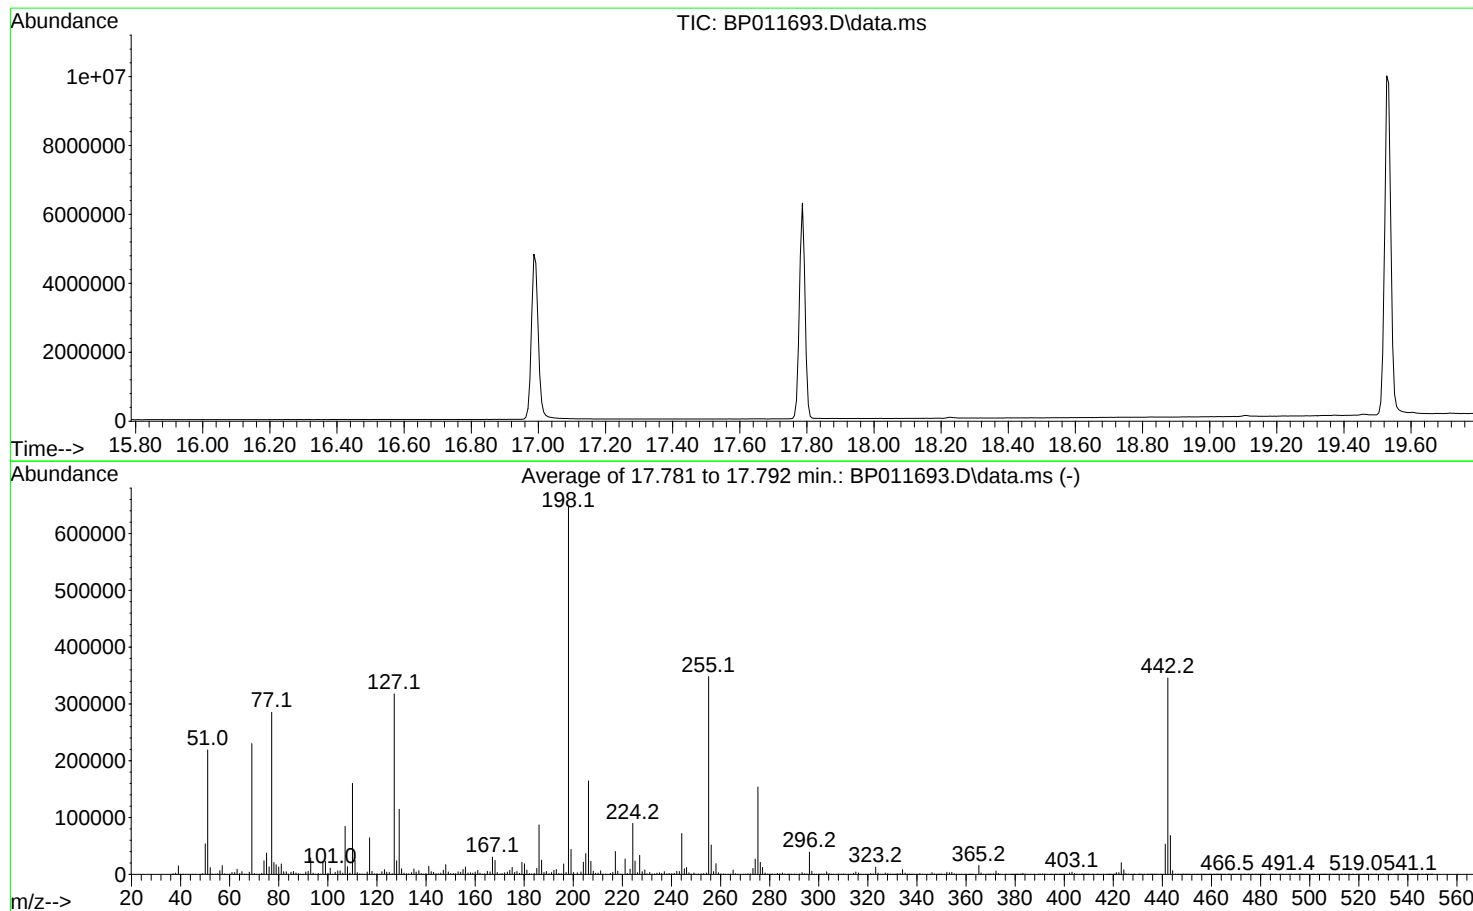


AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	219074	PASS
68	69	0.00	2	1.6	3710	PASS
69	198	0.00	100	35.5	230045	PASS
70	69	0.00	2	0.6	1287	PASS
127	198	10	80	49.0	317577	PASS
197	198	0.00	2	0.5	3259	PASS
198	198	100	100	100.0	647793	PASS
199	198	5	9	6.7	43725	PASS
275	198	10	60	23.7	153653	PASS
365	198	1	100	2.4	15601	PASS
441	198	0.01	100	8.2	53141	PASS
442	442	100	100	100.0	345550	PASS
443	442	15	24	19.8	68341	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091422\
 Data File : BP011693.D
 Acq On : 14 Sep 2022 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 14 16:24:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 16:19:53 2022
 Response via : Initial Calibration

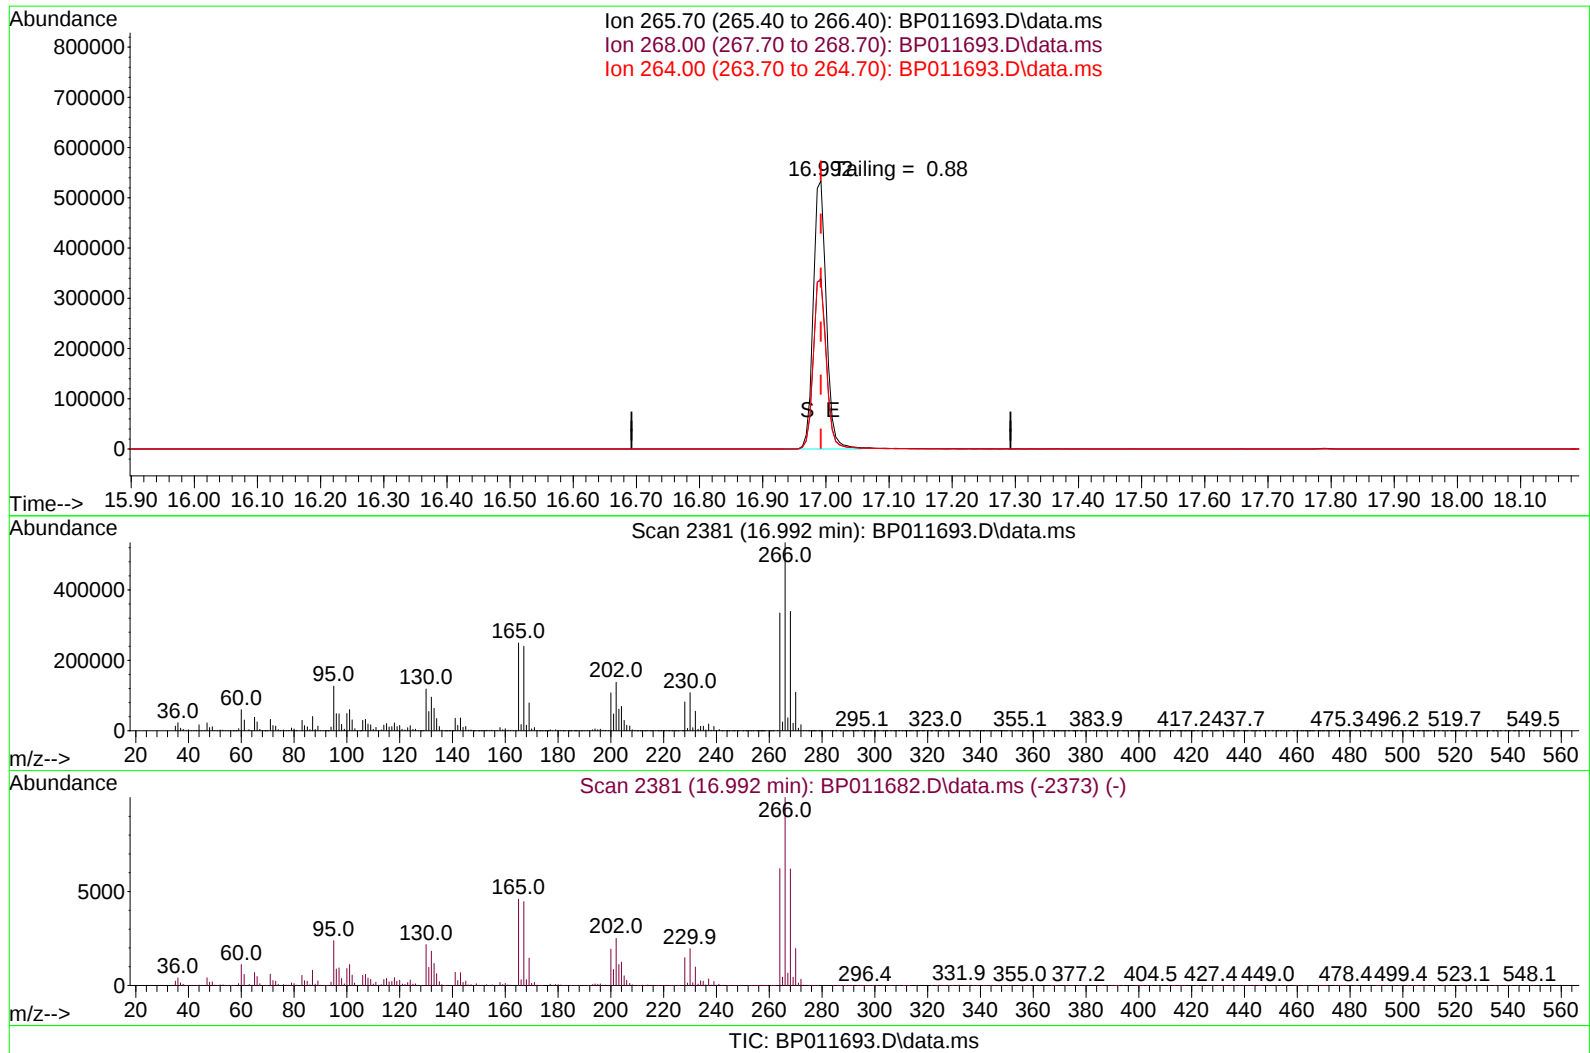

(70) Pentachlorophenol (C)

16.992min (-0.000) 373392.89 ng




response 774698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.50
264.00	63.00	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091422\
 Data File : BP011693.D
 Acq On : 14 Sep 2022 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 14 16:24:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 16:19:53 2022
 Response via : Initial Calibration

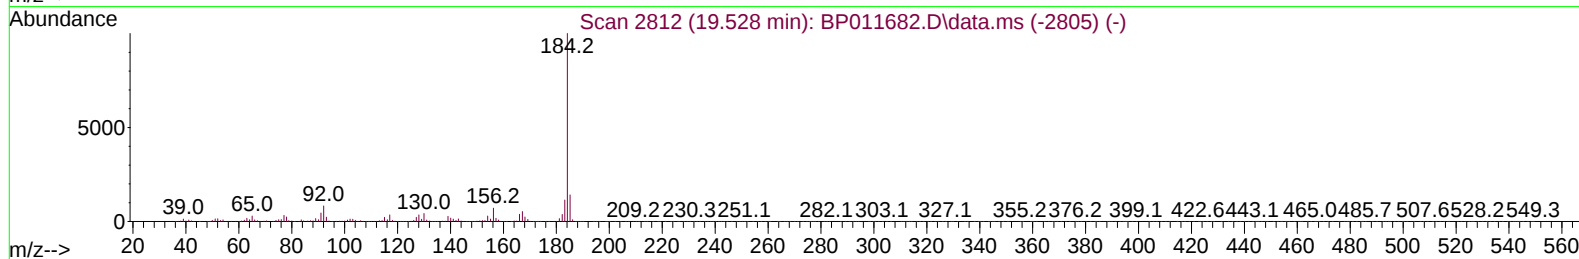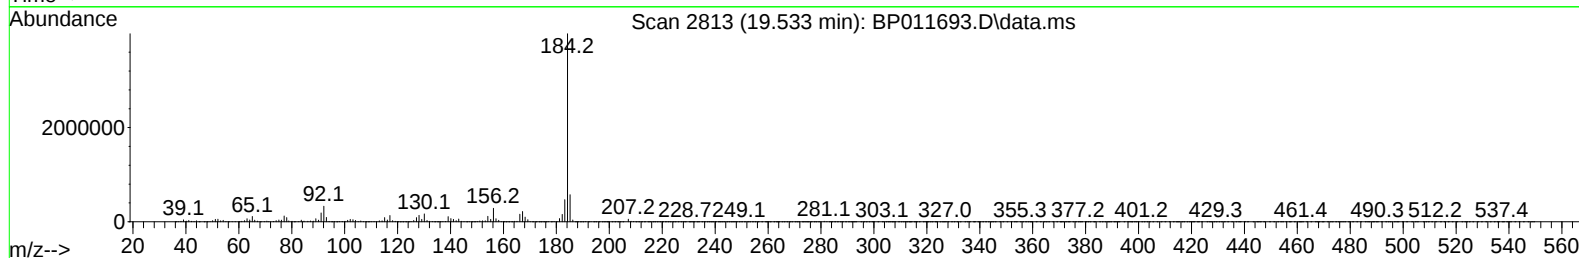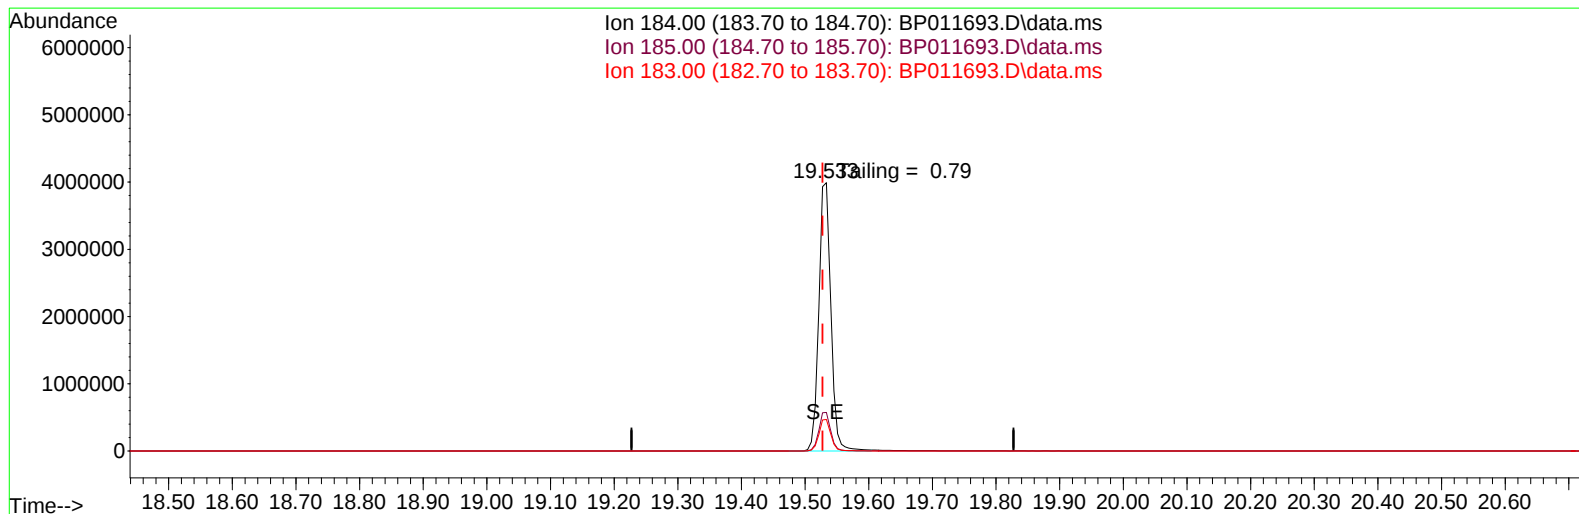

TIC: BP011693.D\data.ms

(77) Benzidine

19.533min (+ 0.006) 5101042.46 ng

response 5265308

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.39
183.00	11.30	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2022	BNA_P	<u>BP011693.D</u>
Compound Name	Response	Retention Time
DDT	2297536	20.73
DDD	14556	20.3
DDE	2283	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16839	2314375	0.73

Instrument :
BNA_P
ClientSampleId :
DFTPP