
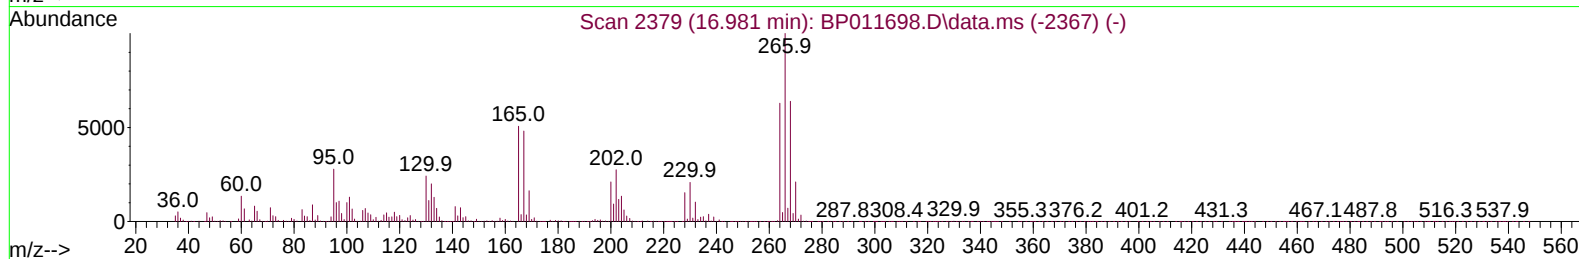
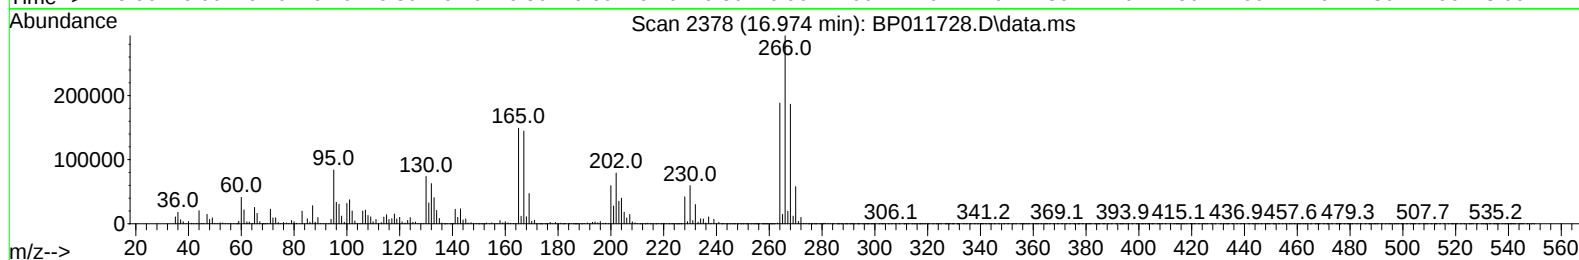


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
 Data File : BP011728.D
 Acq On : 19 Sep 2022 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 18:04:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 19:12:50 2022
 Response via : Initial Calibration

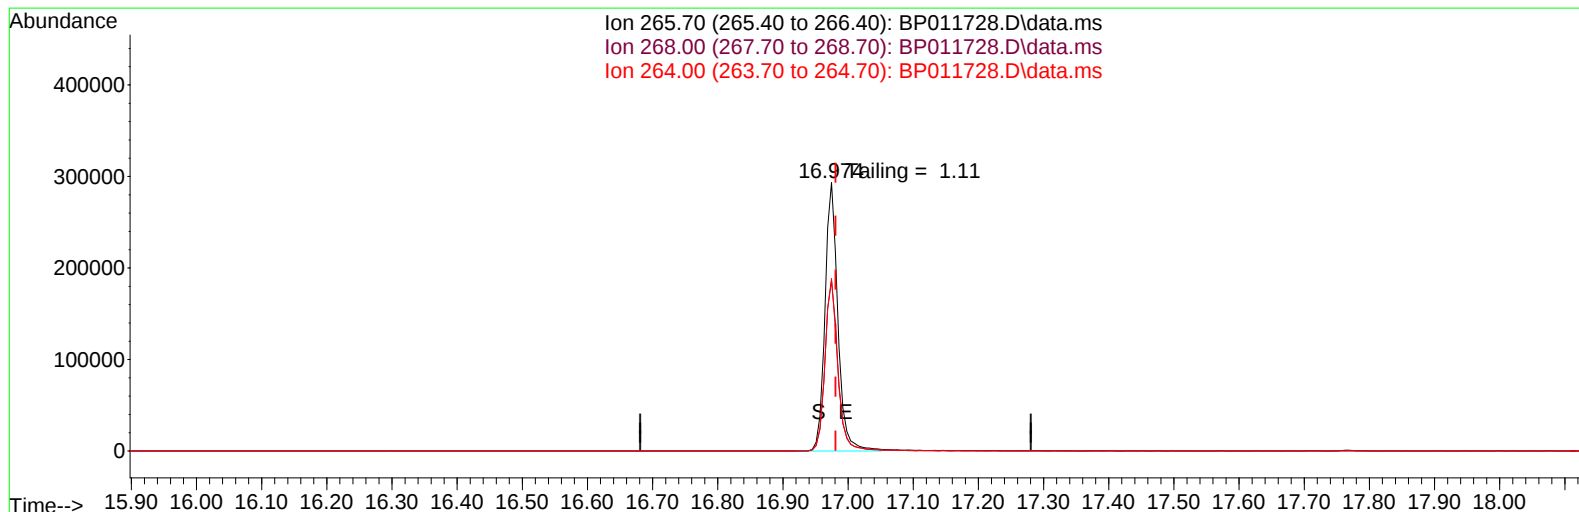

TIC: BP011728.D\data.ms

(70) Pentachlorophenol (C)




16.974min (-0.007) 627114.63 ng

response 409118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.58
264.00	63.00	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
Data File : BP011728.D
Acq On : 19 Sep 2022 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 18:04:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

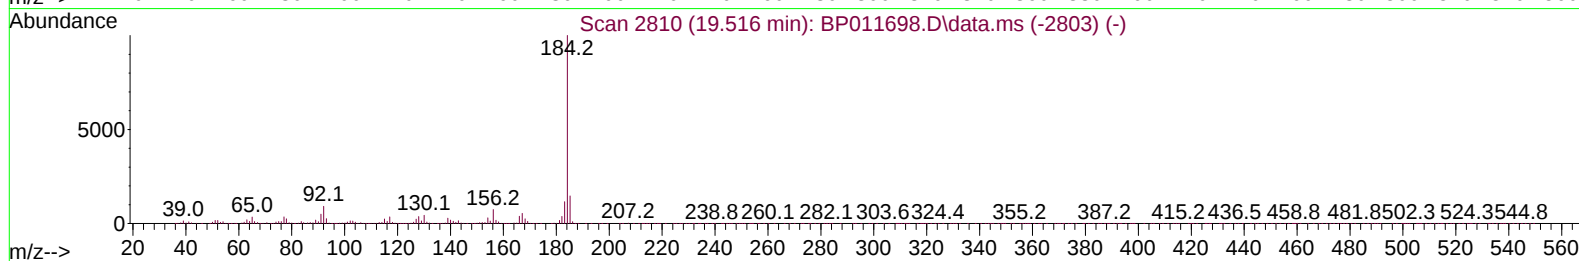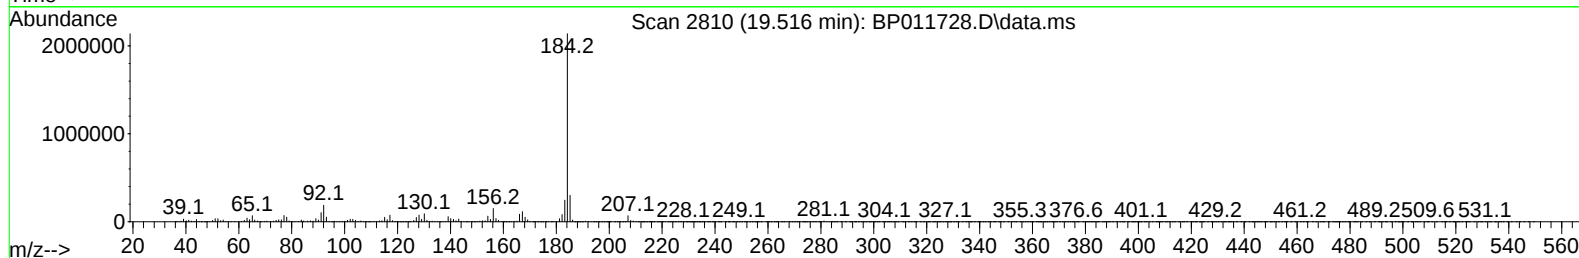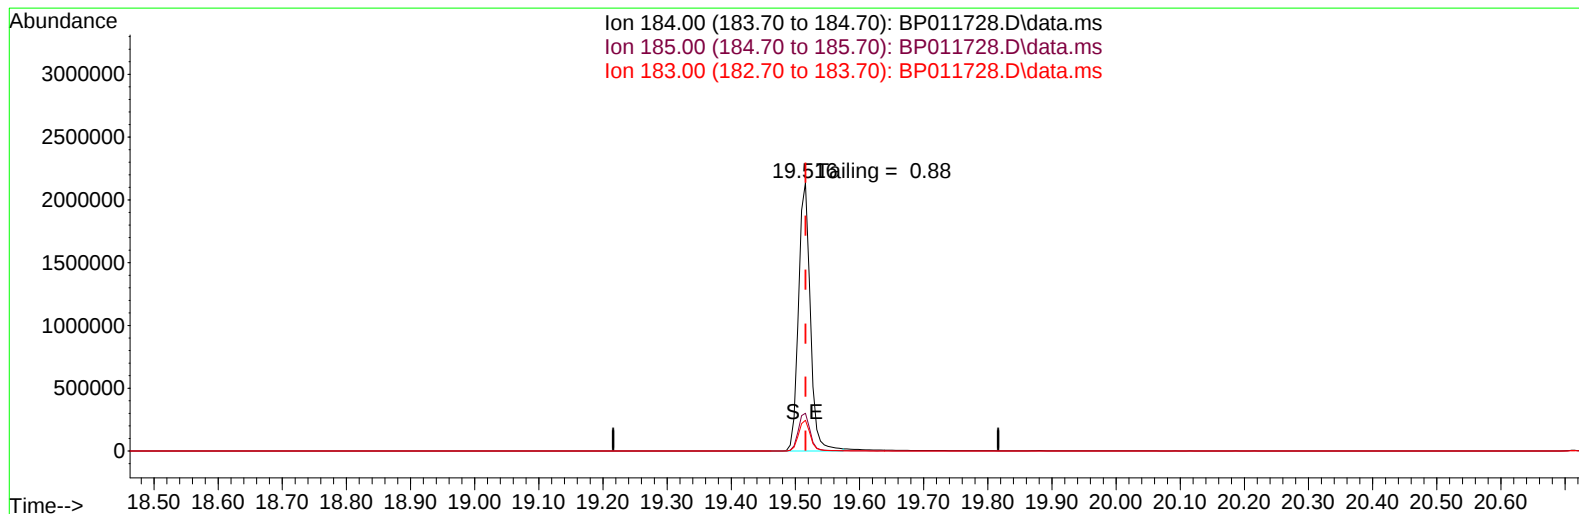

TIC: BP011728.D\data.ms

(77) Benzidine

19.516min (-0.000) 322549.26 ng

response 2776821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.07
183.00	11.30	11.47
0.00	0.00	0.00