
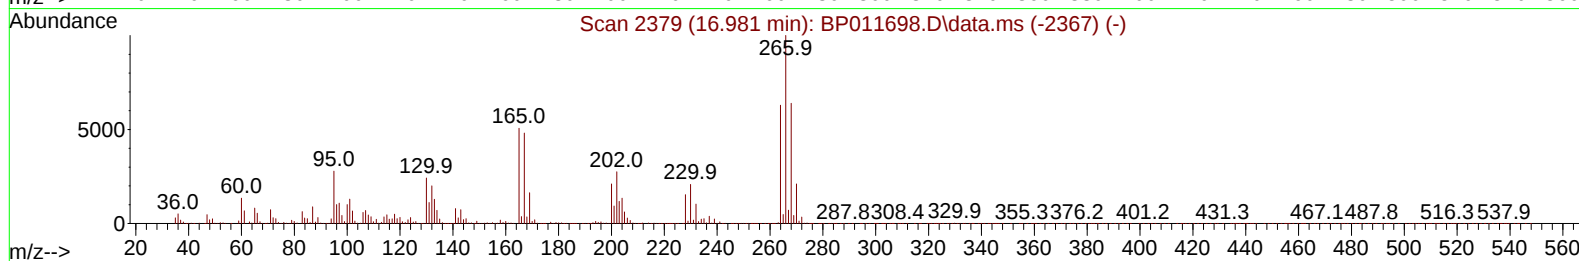
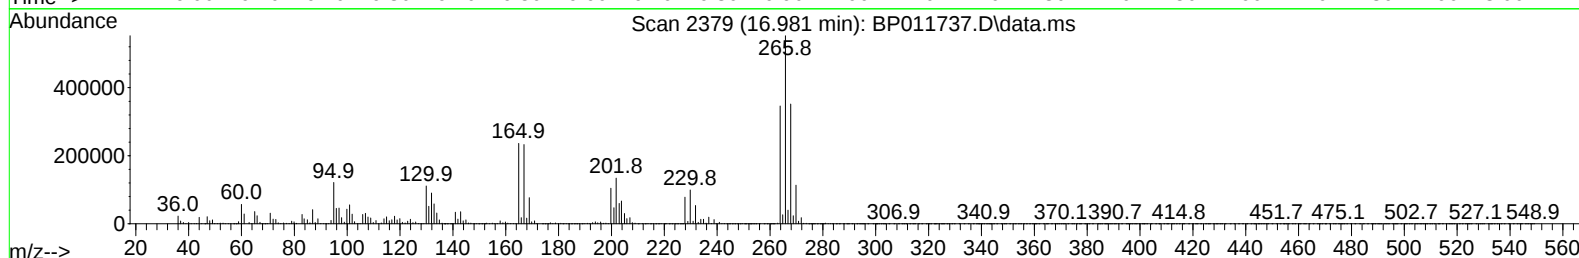


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
 Data File : BP011737.D
 Acq On : 19 Sep 2022 16:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 07:05:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 04:42:52 2022
 Response via : Initial Calibration

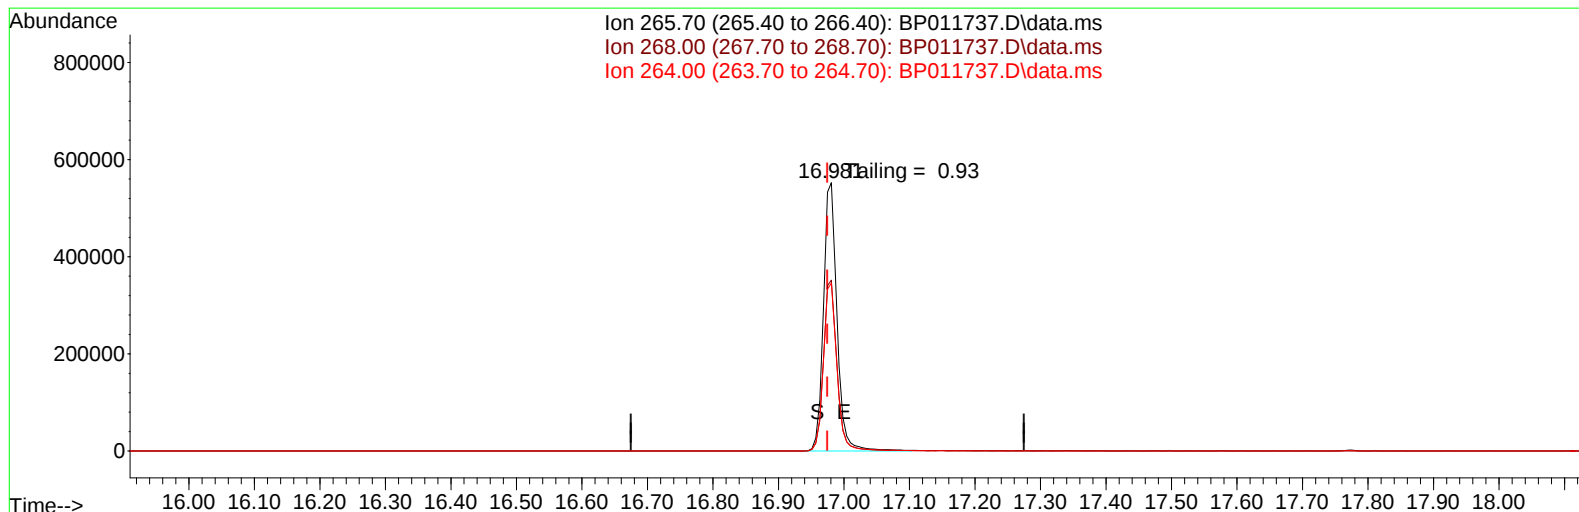

TIC: BP011737.D\data.ms

(70) Pentachlorophenol (C)




16.981min (+ 0.006) 72116.88 ng

response 797505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.70
264.00	63.00	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
Data File : BP011737.D
Acq On : 19 Sep 2022 16:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 07:05:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 04:42:52 2022
Response via : Initial Calibration

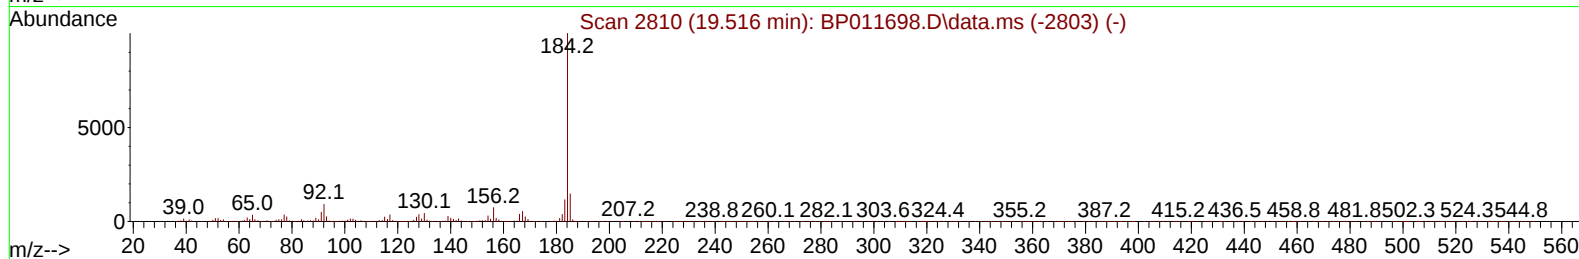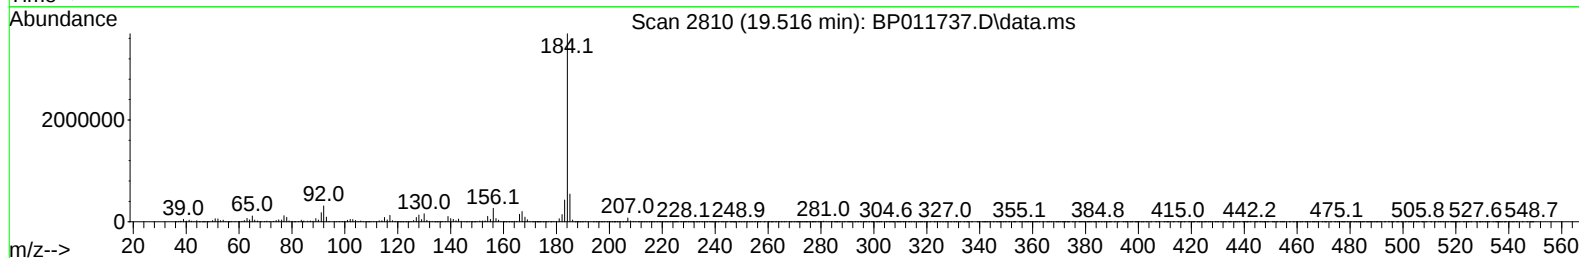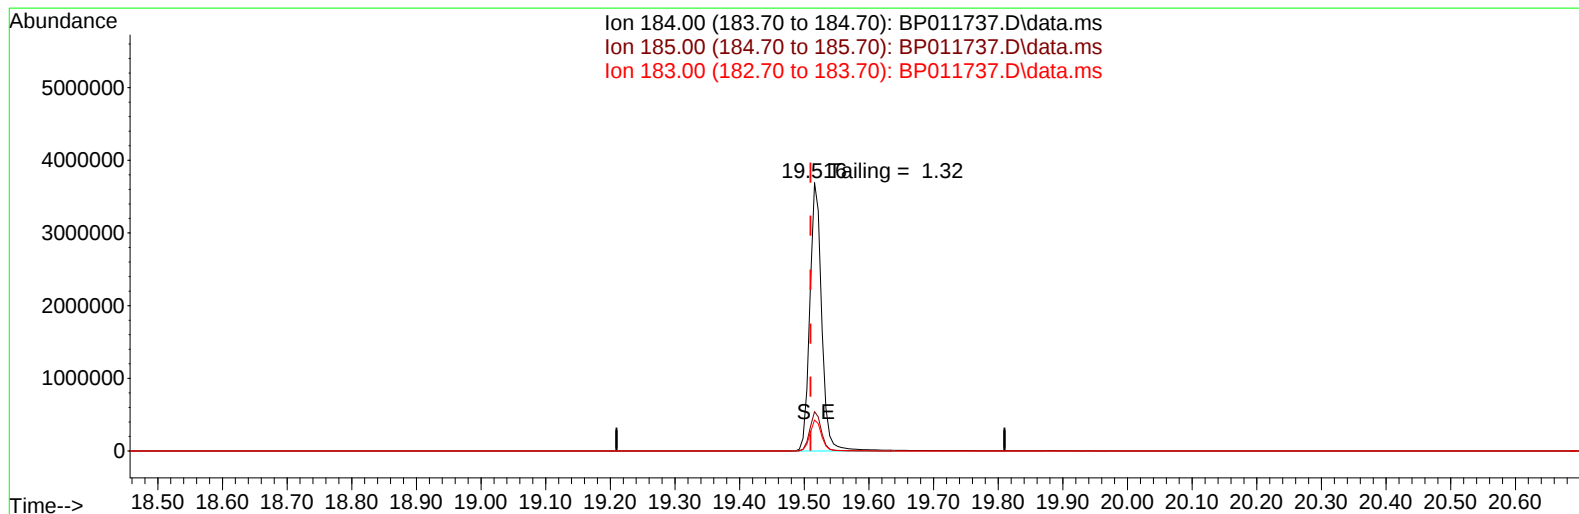

TIC: BP011737.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 43204.73 ng

response 4736696

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.70
183.00	11.30	11.60
0.00	0.00	0.00