

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
 Data File : BP011752.D
 Acq On : 20 Sep 2022 01:03
 Operator : CG/JU
 Sample : N4675-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 006-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP011752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	9	14	38	rVB	8174828	12146918	38.88%	9.577%
2	5.493	419	426	444	rBV	3939687	6006434	19.22%	4.736%
3	7.093	690	698	712	rBV	2570401	4125707	13.21%	3.253%
4	7.934	834	841	849	rBV	1259567	2073463	6.64%	1.635%
5	9.104	1031	1040	1054	rBV	4985737	8478641	27.14%	6.685%
6	10.745	1310	1319	1333	rBV	1907148	3244682	10.39%	2.558%
7	13.198	1727	1736	1752	rBV	14087548	20685676	66.21%	16.309%
8	14.575	1962	1970	1985	rBV	3173739	4673418	14.96%	3.685%
9	16.063	2216	2223	2244	rBV	10950035	15629177	50.02%	12.322%
10	17.327	2431	2438	2448	rBV	3939854	5631875	18.03%	4.440%
11	19.880	2866	2872	2877	rBV	25377235	31243478	100.00%	24.633%
12	21.110	3078	3081	3090	rBV2	281508	407957	1.31%	0.322%
13	21.404	3126	3131	3139	rBV	4874485	6279662	20.10%	4.951%
14	23.857	3541	3548	3558	rVB2	2998650	6209241	19.87%	4.895%




Sum of corrected areas: 126836329

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
Data File : BP011752.D
Acq On : 20 Sep 2022 01:03
Operator : CG/JU
Sample : N4675-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
006-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

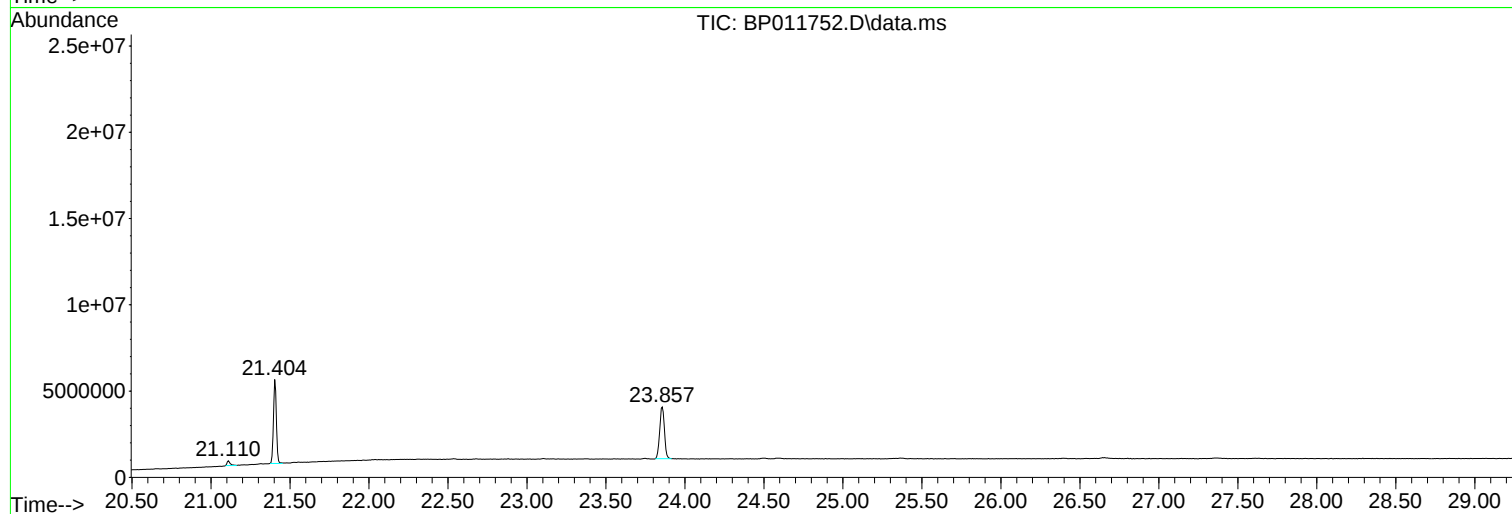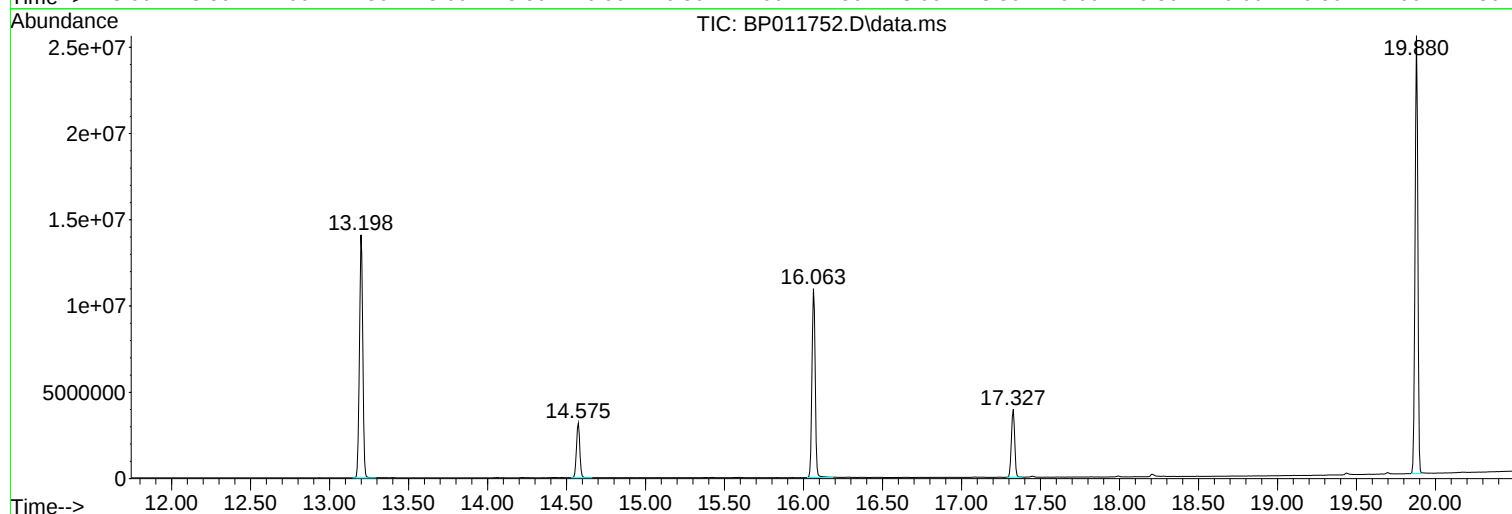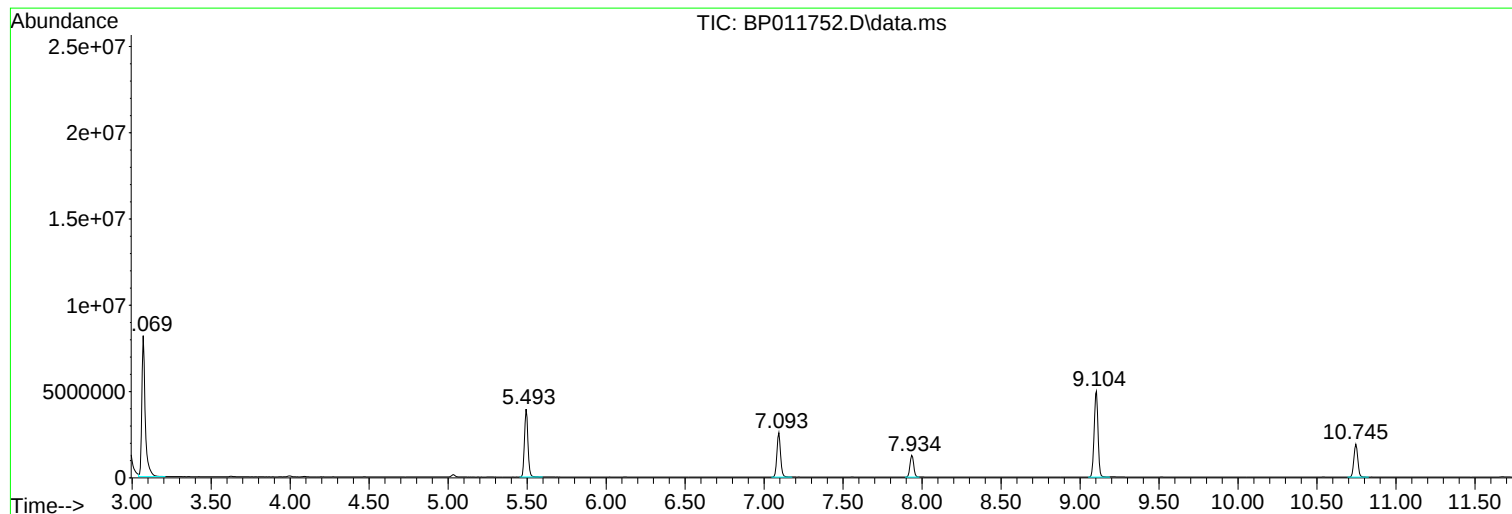

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
Data File : BP011752.D
Acq On : 20 Sep 2022 01:03
Operator : CG/JU
Sample : N4675-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
006-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.069	117.17 ng	12146900	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83		
2	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39		
3	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23		
4	1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

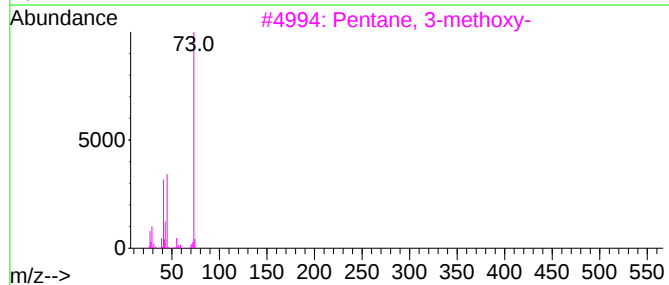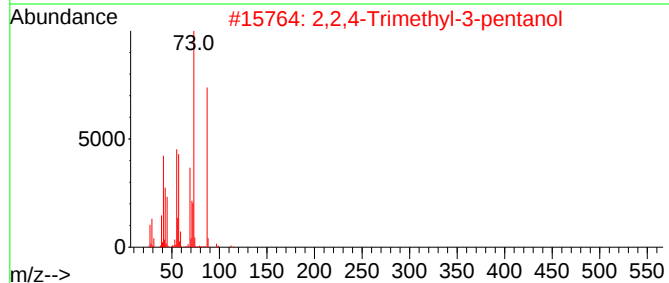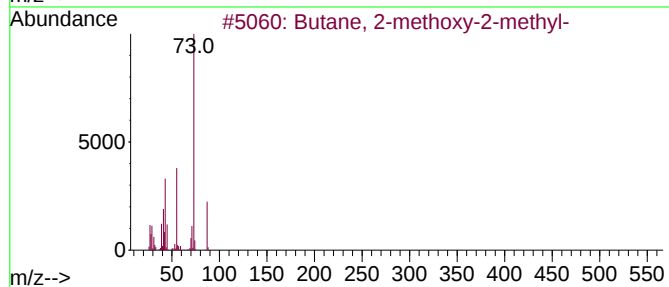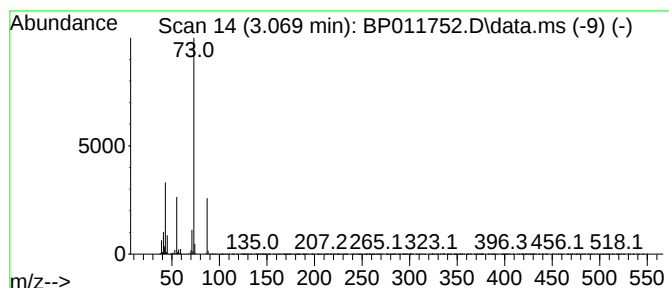

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
Data File : BP011752.D
Acq On : 20 Sep 2022 01:03
Operator : CG/JU
Sample : N4675-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
006-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.069	117.2	ng	12146900	1	7.934	2073460	20.0