


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
 Data File : BP011728.D
 Acq On : 19 Sep 2022 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 20 04:42:52 2022

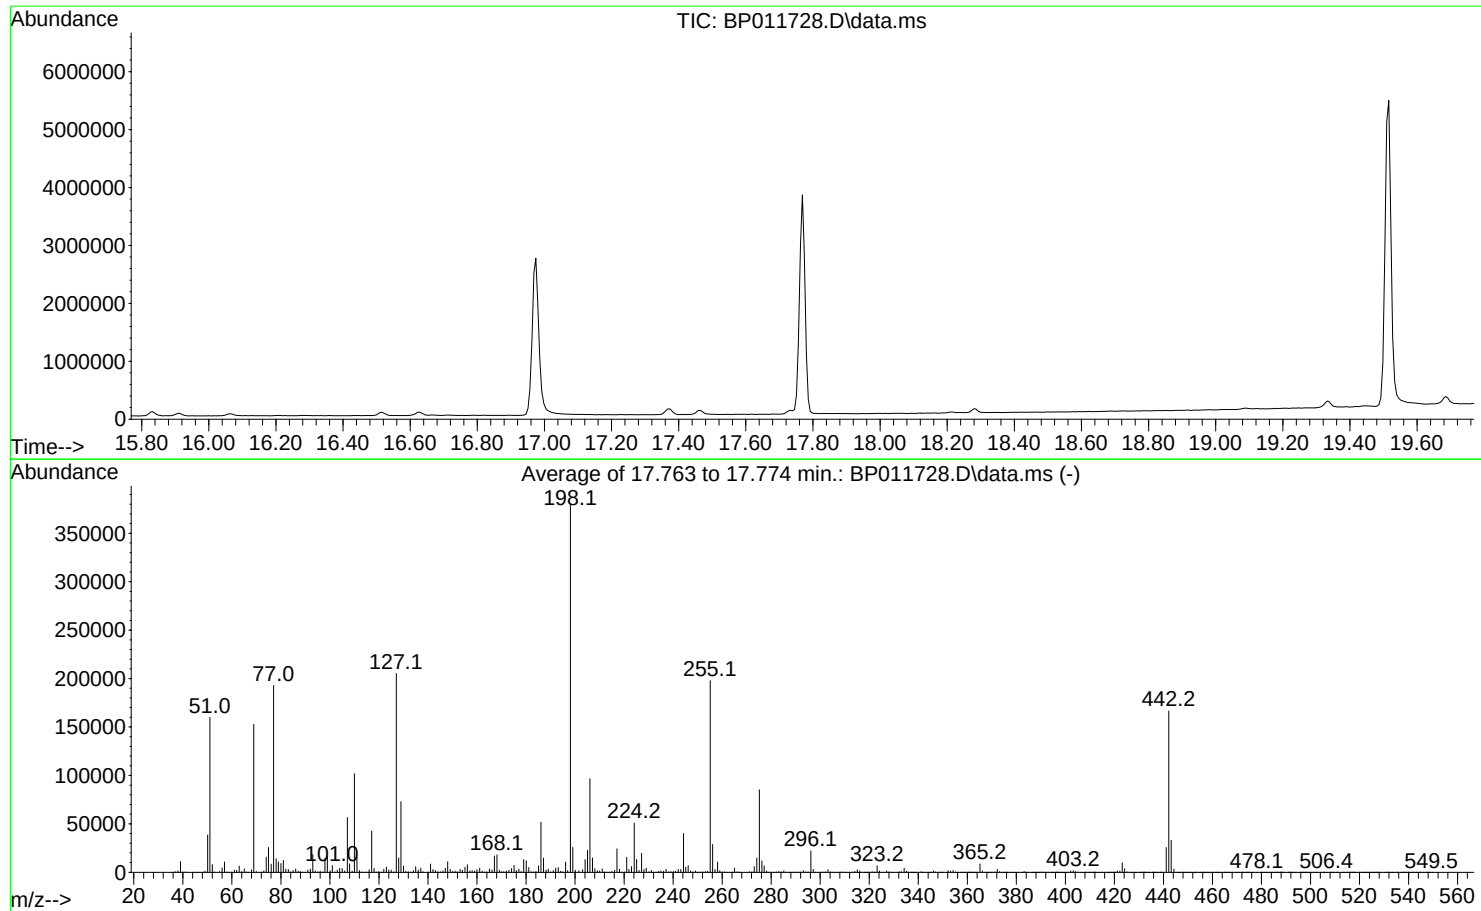




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	159955	PASS
68	69	0.00	2	1.7	2600	PASS
69	198	0.00	100	40.2	152781	PASS
70	69	0.00	2	0.5	715	PASS
127	198	10	80	54.1	205285	PASS
197	198	0.00	2	0.4	1667	PASS
198	198	100	100	100.0	379765	PASS
199	198	5	9	6.8	25729	PASS
275	198	10	60	22.4	85239	PASS
365	198	1	100	2.3	8636	PASS
441	198	0.01	100	6.7	25531	PASS
442	442	100	100	100.0	166613	PASS
443	442	15	24	19.7	32895	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
Data File : BP011728.D
Acq On : 19 Sep 2022 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Sep 19 18:04:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 19:12:50 2022
Response via : Initial Calibration

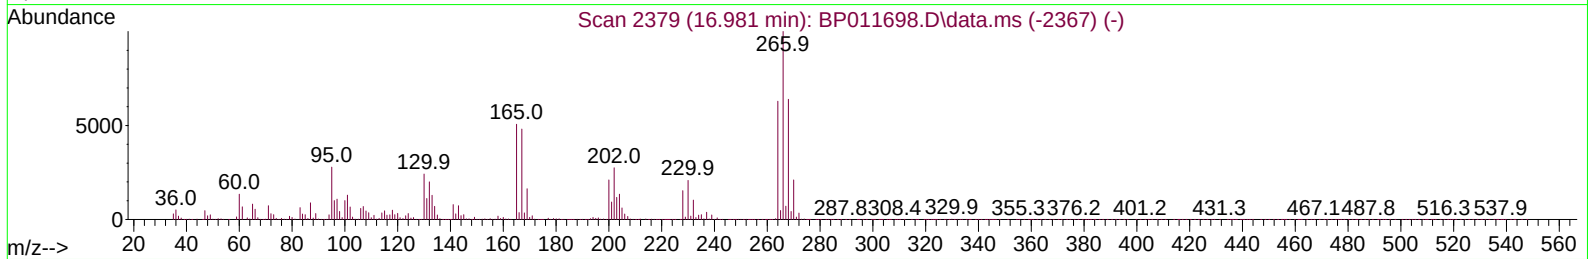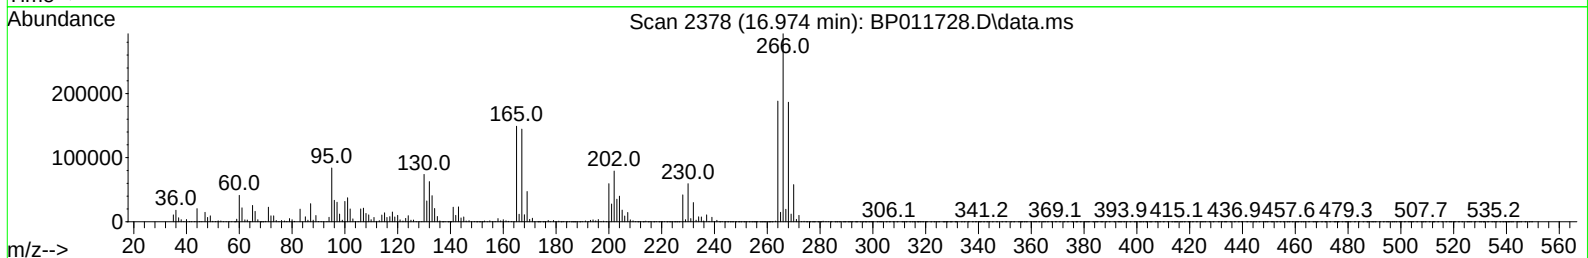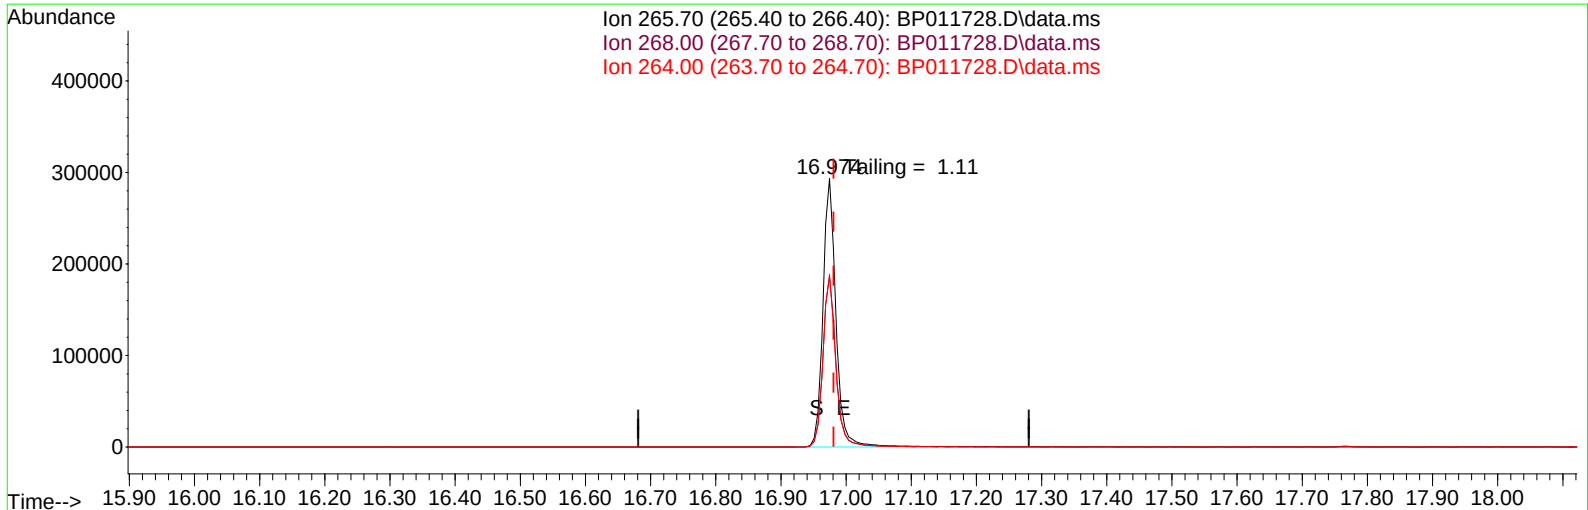

TIC: BP011728.D\data.ms

(70) Pentachlorophenol (C)

16.974min (-0.007) 627114.63 ng




response 409118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.58
264.00	63.00	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP091922\
 Data File : BP011728.D
 Acq On : 19 Sep 2022 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Sep 19 18:04:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 19:12:50 2022
 Response via : Initial Calibration

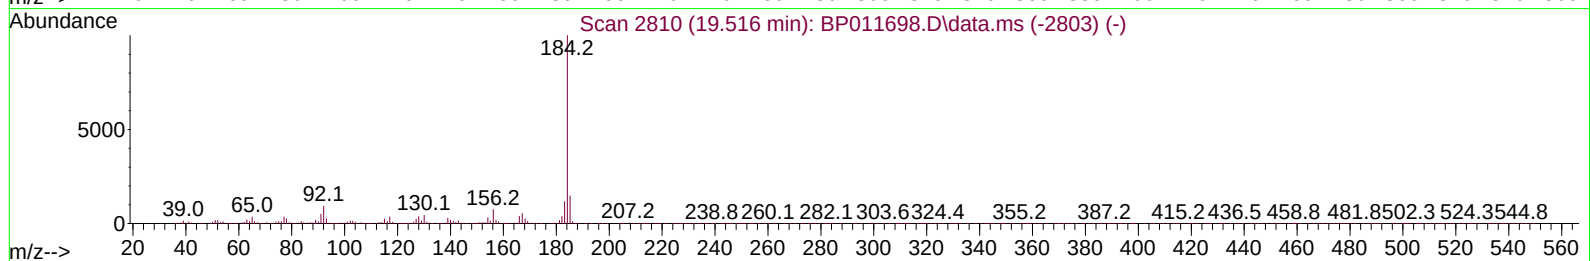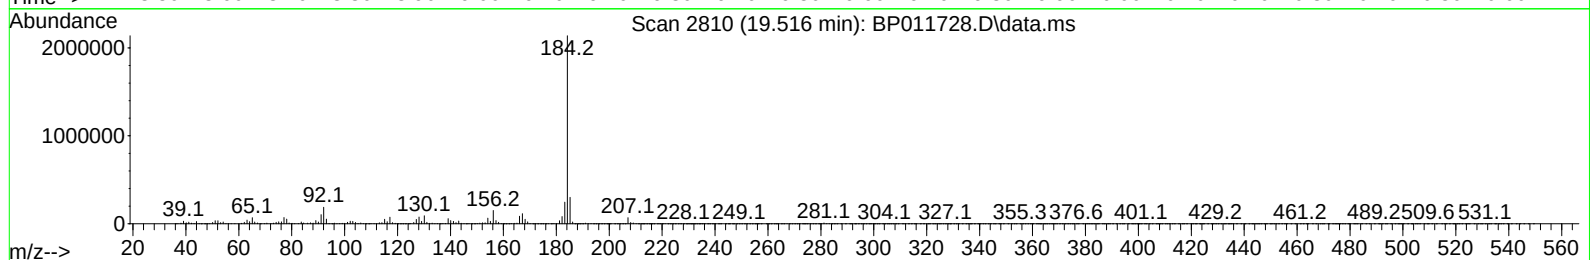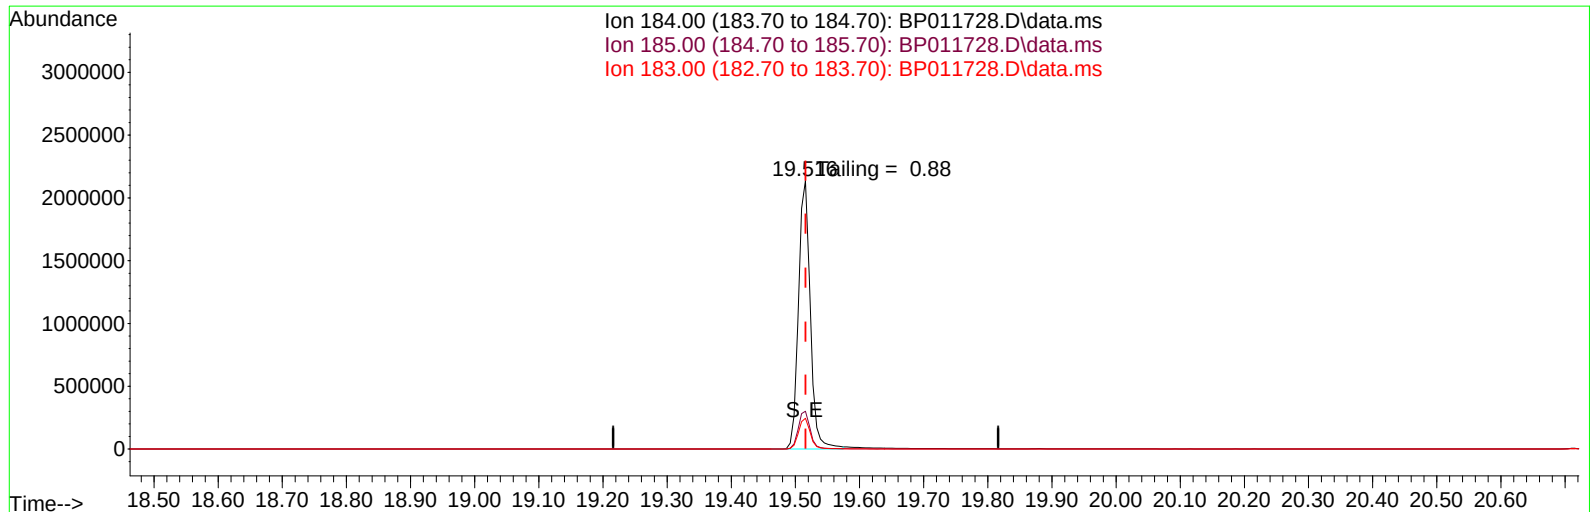

TIC: BP011728.D\data.ms

(77) Benzidine

19.516min (-0.000) 322549.26 ng

response 2776821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.07
183.00	11.30	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2022	BNA_P	<u>BP011728.D</u>
Compound Name	Response	Retention Time
DDT	1229120	20.71
DDD	5063	20.28
DDE	2490	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7553	1236673	0.61

Instrument :
BNA_P
ClientSampleId :
DFTPP